

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF051122\
 Data File : BF128196.D
 Acq On : 11 May 2022 15:54
 Operator : CG\JU
 Sample : N2761-01
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 TWP04

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF050922.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF128196.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.510	544	548	563	rBV	912228	808815	23.81%	5.172%
2	6.510	715	718	729	rBV	534167	507097	14.93%	3.243%
3	6.893	779	783	786	rBV	581900	531736	15.65%	3.400%
4	7.457	873	879	882	rBV	1694472	1801485	53.04%	11.520%
5	8.175	996	1001	1004	rBV	763111	685014	20.17%	4.381%
6	9.251	1178	1184	1187	rBV	3346012	3128173	92.10%	20.004%
7	9.934	1294	1300	1303	rBV	922163	813266	23.94%	5.201%
8	10.722	1430	1434	1448	rBV	1527321	1530671	45.06%	9.789%
9	11.422	1549	1553	1557	rBV	1080620	884503	26.04%	5.656%
10	13.016	1818	1824	1827	rBV	3388483	3396649	100.00%	21.721%
11	13.974	1979	1987	1999	rBV6	43703	185428	5.46%	1.186%
12	14.069	1999	2003	2007	rVB	841017	752401	22.15%	4.812%
13	14.157	2014	2018	2023	rVB	32462	35479	1.04%	0.227%
14	15.568	2252	2258	2271	rBV	424191	576644	16.98%	3.688%




Sum of corrected areas: 15637361

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF051122\
Data File : BF128196.D
Acq On : 11 May 2022 15:54
Operator : CG\JU
Sample : N2761-01
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
TWP04

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF050922.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

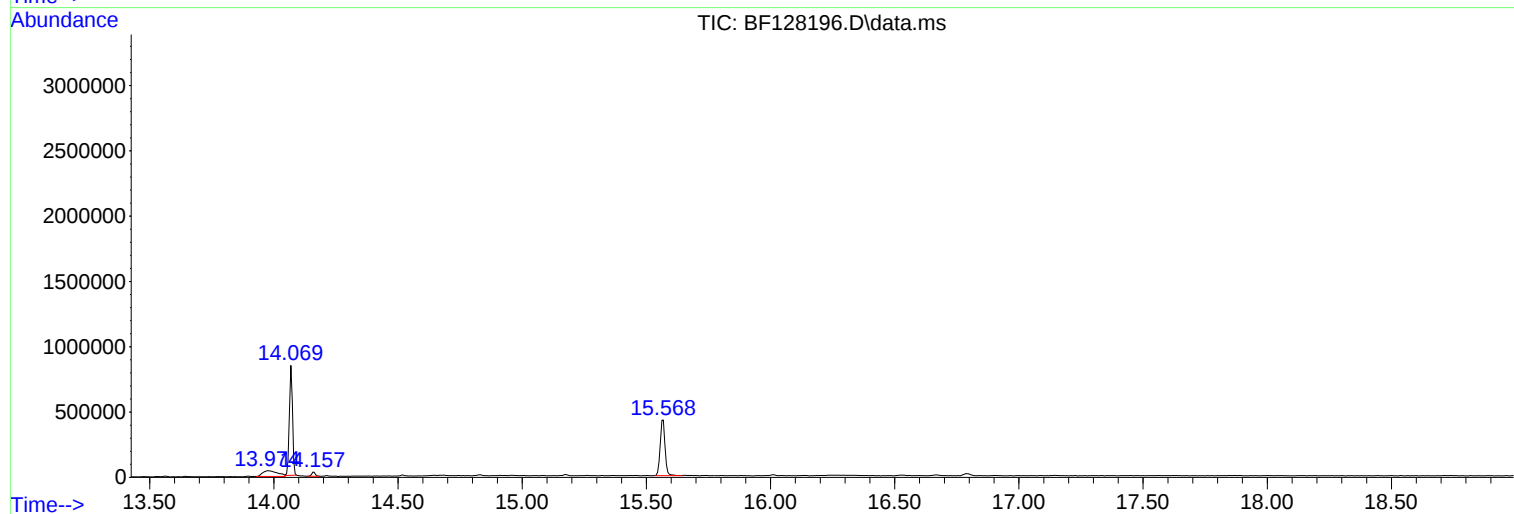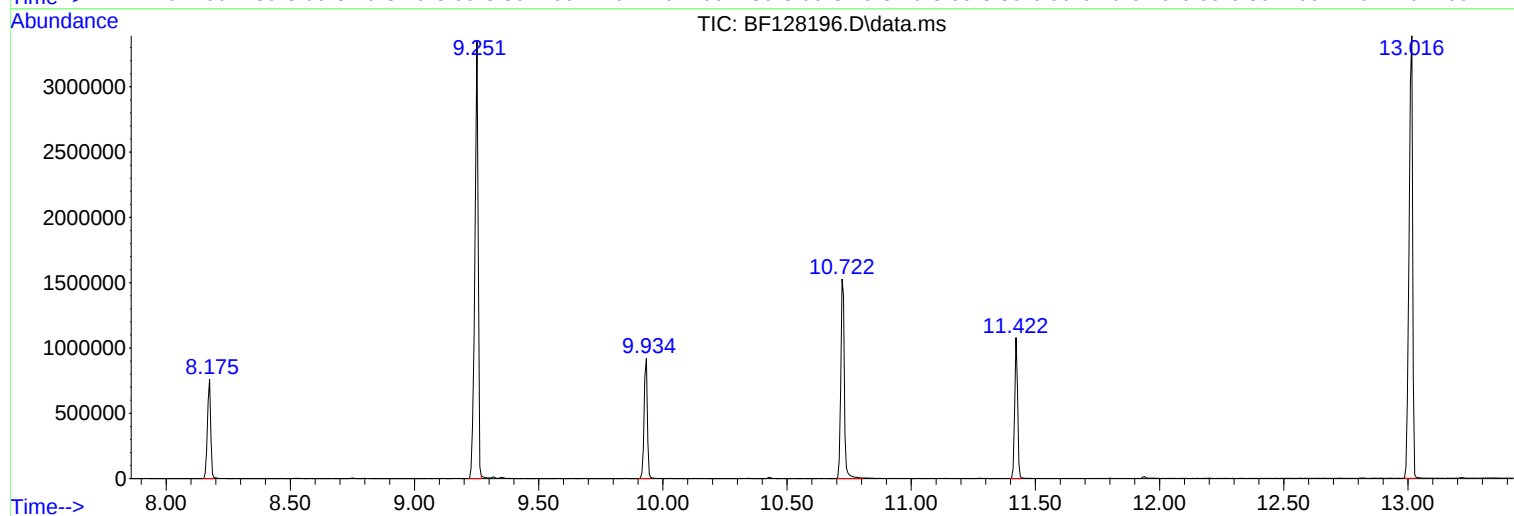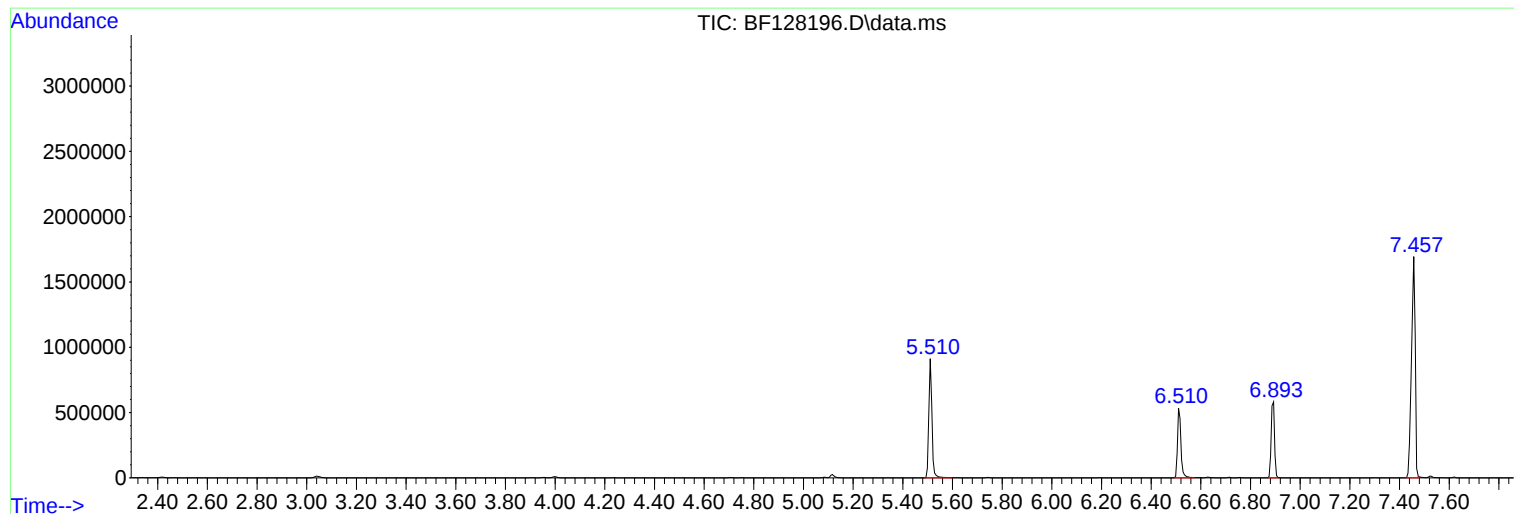

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF051122\
Data File : BF128196.D
Acq On : 11 May 2022 15:54
Operator : CG\JU
Sample : N2761-01
Misc :
ALS Vial : 7 Sample Multiplier: 1










Instrument :
BNA_F
ClientSampleId :
TWP04

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF050922.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Trifluoroacetoxy hexadecane Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.	
13.975	4.93 ng	185428	Chrysene-d12	14.069	
Hit# of 5	Tentative ID	MW	MolForm	CAS#	Qual
1	Trifluoroacetoxy hexadecane	338	C18H33F3O2	006222-03-3	94
2	n-Tetracosanol-1	354	C24H50O	000506-51-4	91
3	Behenic alcohol	326	C22H46O	000661-19-8	91
4	Trichloroacetic acid, pentadecyl...	372	C17H31Cl3O2	074339-53-0	91
5	1-Heptacosanol	396	C27H56O	002004-39-9	91

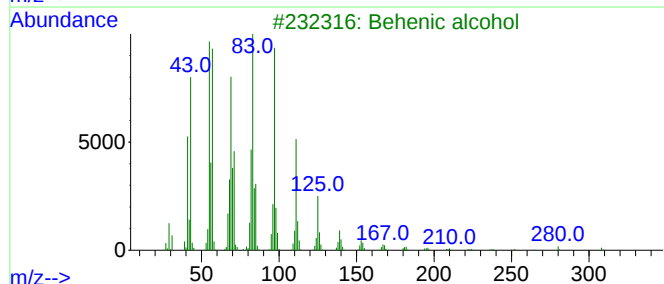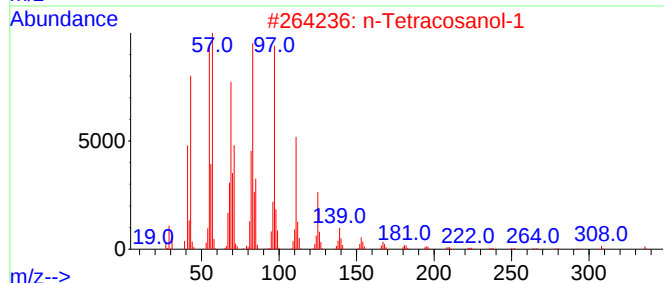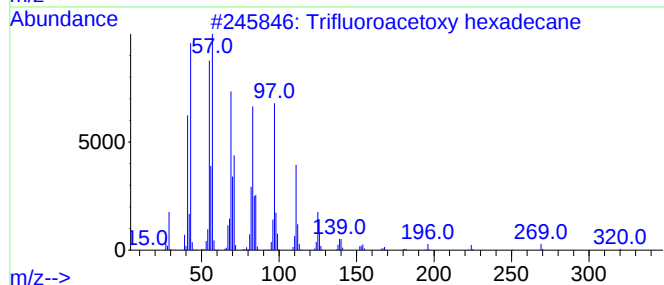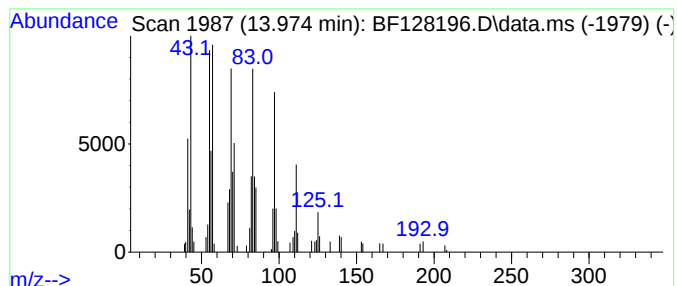

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF051122\
Data File : BF128196.D
Acq On : 11 May 2022 15:54
Operator : CG\JU
Sample : N2761-01
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
TWP04

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF050922.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Trifluoroacetox...	13.975	4.9	ng	185428	5	14.069	752401	20.0