

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF051122\
 Data File : BF128197.D
 Acq On : 11 May 2022 16:23
 Operator : CG\JU
 Sample : N2761-02
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 TWP05

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF050922.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF128197.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.510	544	548	566	rBV	945278	834523	24.95%	5.476%
2	6.510	715	718	731	rBV	550555	530963	15.87%	3.484%
3	6.892	779	783	786	rBV	606192	521798	15.60%	3.424%
4	7.457	874	879	882	rBV	1635562	1781638	53.27%	11.691%
5	8.175	996	1001	1004	rBV	752654	671342	20.07%	4.405%
6	9.251	1178	1184	1187	rBV	3383195	3113444	93.08%	20.430%
7	9.933	1295	1300	1303	rBV	892320	792934	23.71%	5.203%
8	10.722	1430	1434	1445	rBV	1532990	1473382	44.05%	9.668%
9	11.422	1549	1553	1557	rBV	1004865	854170	25.54%	5.605%
10	13.016	1818	1824	1827	rBV	3404382	3344757	100.00%	21.948%
11	13.968	1979	1986	1995	rBV	20380	78531	2.35%	0.515%
12	14.068	1999	2003	2007	rBV	811553	711463	21.27%	4.668%
13	15.562	2252	2257	2267	rBV	409570	530733	15.87%	3.483%




Sum of corrected areas: 15239678

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF051122\
Data File : BF128197.D
Acq On : 11 May 2022 16:23
Operator : CG\JU
Sample : N2761-02
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
TWP05

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF050922.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

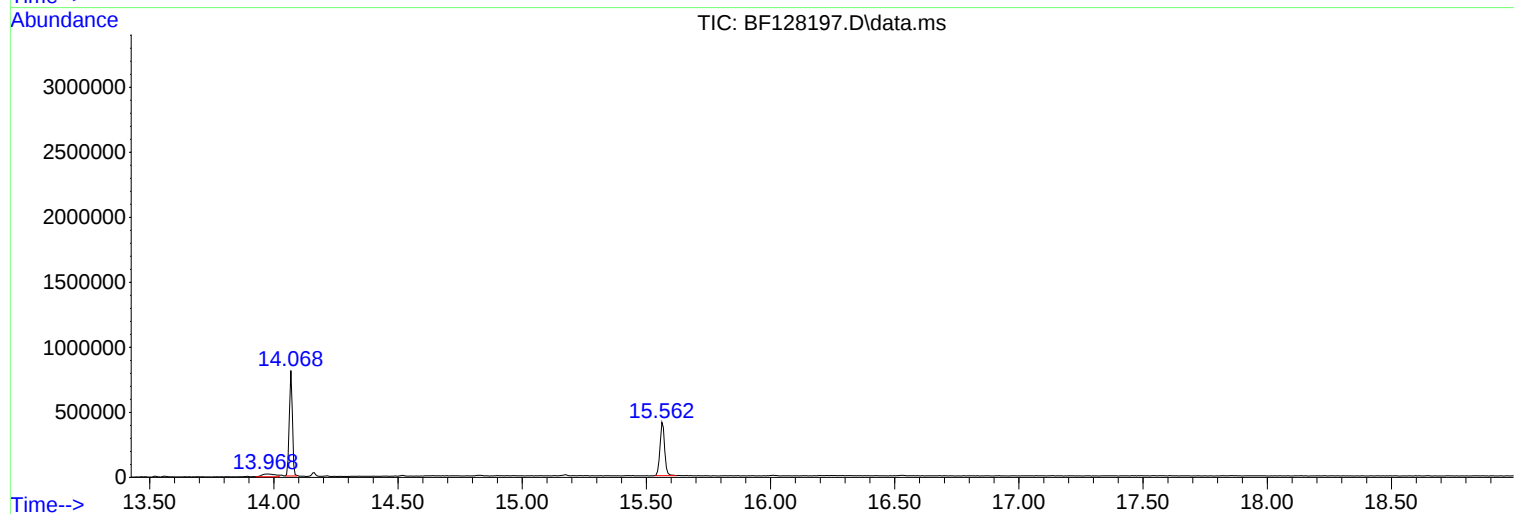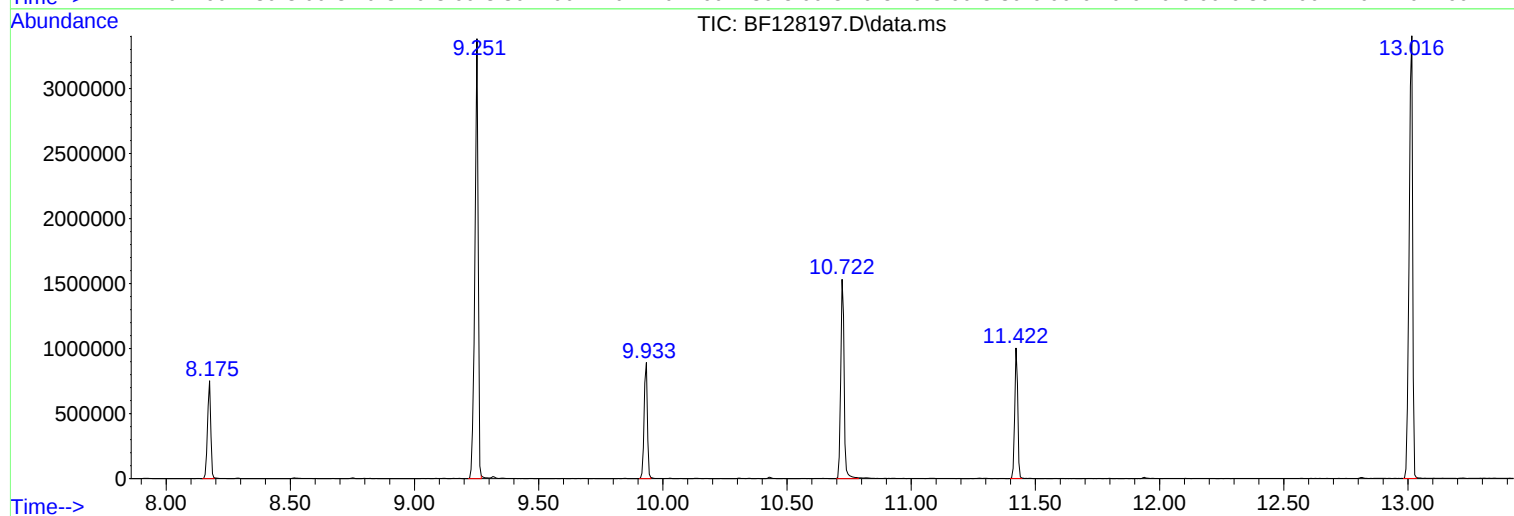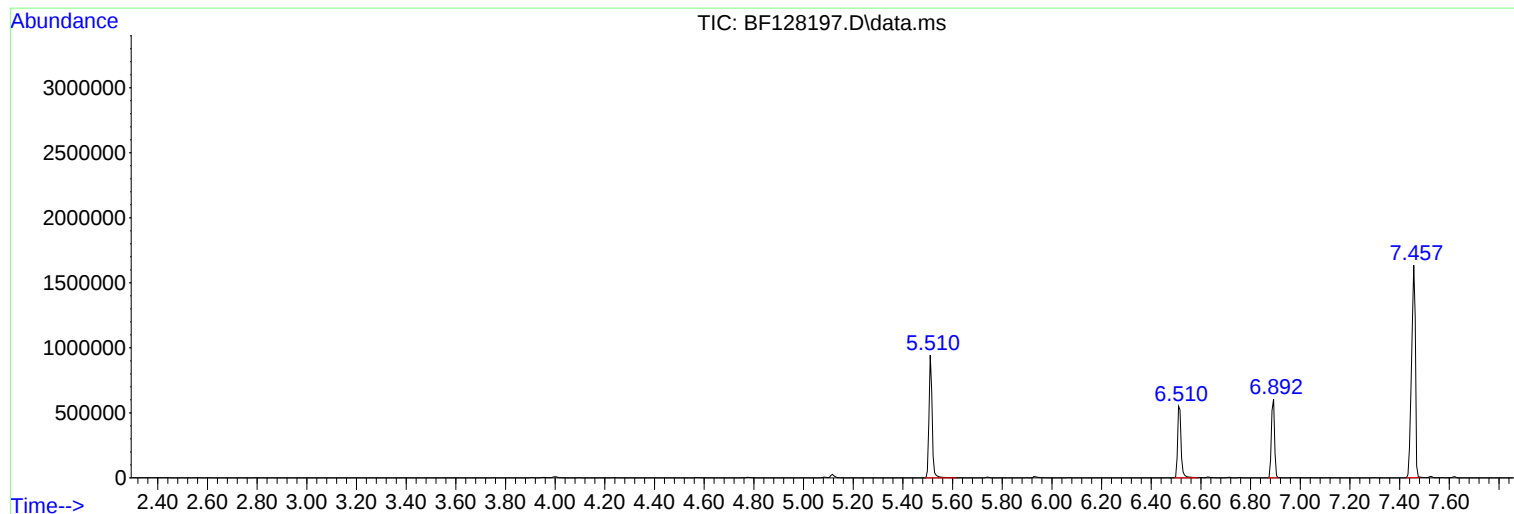

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF051122\
Data File : BF128197.D
Acq On : 11 May 2022 16:23
Operator : CG\JU
Sample : N2761-02
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
TWP05










Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF050922.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Dichloroacetic acid, heptad... Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
13.969	2.21 ng	78531	Chrysene-d12	14.069

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Dichloroacetic acid, heptadecyl ...	366	C19H36Cl2O2	1000282-98-2	93
2			Acetic acid, chloro-, octadecyl ...	346	C20H39ClO2	005348-82-3	91
3			Acetic acid, chloro-, hexadecyl ...	318	C18H35ClO2	052132-58-8	91
4			Carbonic acid, octadecyl 2,2,2-t...	444	C21H39Cl3O3	1000314-56-3	91
5			Heptafluorobutyric acid, n-tetra...	410	C18H29F7O2	007365-36-8	90

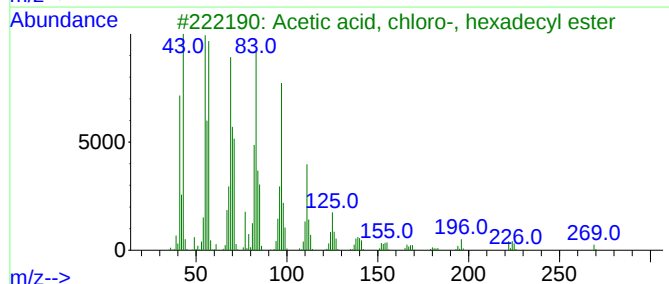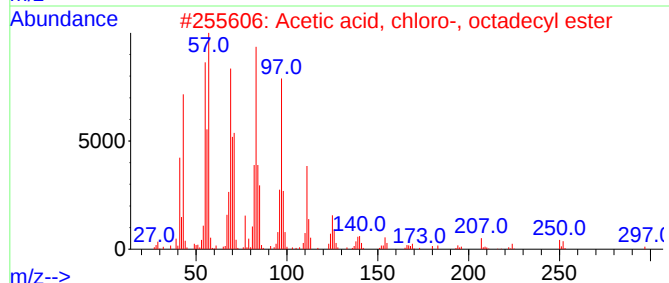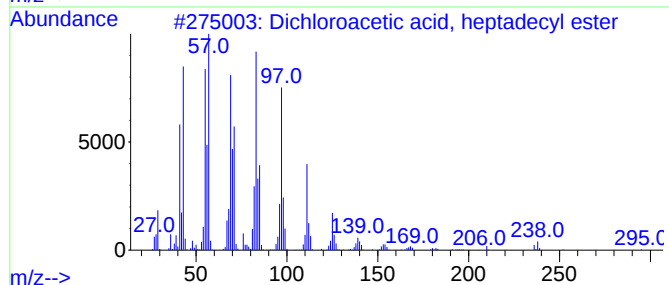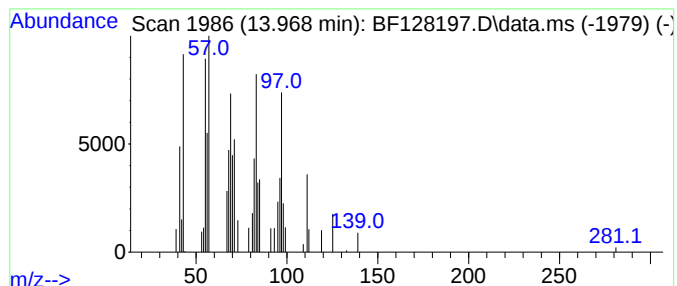

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF051122\
Data File : BF128197.D
Acq On : 11 May 2022 16:23
Operator : CG\JU
Sample : N2761-02
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
TWP05

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF050922.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Dichloroacetic ...	13.969	2.2	ng	78531	5	14.069	711463	20.0