

Data Path : Z:\svoasrv\HPCHEM1\BNA\_F\Data\BF051122\  
 Data File : BF128202.D  
 Acq On : 11 May 2022 18:49  
 Operator : CG\JU  
 Sample : N2762-03  
 Misc :  
 ALS Vial : 13 Sample Multiplier: 1

Instrument :  
 BNA\_F  
 ClientSampleId :  
 SB04

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA\_F\Methods\8270-BF050922.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF128202.D\data.ms

| peak<br># | R.T.<br>min | first<br>scan | max<br>scan | last<br>scan | PK<br>TY | peak<br>height | corr.<br>area | corr.<br>% max. | % of<br>total |
|-----------|-------------|---------------|-------------|--------------|----------|----------------|---------------|-----------------|---------------|
| 1         | 5.140       | 481           | 485         | 493          | rVB      | 28108          | 37274         | 1.57%           | 0.218%        |
| 2         | 5.516       | 545           | 549         | 552          | rBV      | 2171298        | 2165967       | 91.30%          | 12.685%       |
| 3         | 6.522       | 714           | 720         | 723          | rBV      | 2167947        | 2280731       | 96.13%          | 13.357%       |
| 4         | 6.892       | 779           | 783         | 786          | rBV      | 626419         | 556551        | 23.46%          | 3.259%        |
| 5         | 7.457       | 873           | 879         | 882          | rBV      | 1541160        | 1527978       | 64.40%          | 8.948%        |
| 6         | 8.175       | 996           | 1001        | 1004         | rBV      | 797188         | 724507        | 30.54%          | 4.243%        |
| 7         | 9.251       | 1178          | 1184        | 1187         | rBV      | 2555984        | 2372492       | 100.00%         | 13.894%       |
| 8         | 9.933       | 1295          | 1300        | 1303         | rBV      | 914873         | 845466        | 35.64%          | 4.951%        |
| 9         | 10.722      | 1430          | 1434        | 1438         | rBV      | 1832604        | 1828380       | 77.07%          | 10.707%       |
| 10        | 11.421      | 1549          | 1553        | 1556         | rBV      | 1058583        | 891120        | 37.56%          | 5.219%        |
| 11        | 11.445      | 1556          | 1557        | 1561         | rVB      | 49490          | 27426         | 1.16%           | 0.161%        |
| 12        | 11.939      | 1632          | 1641        | 1645         | rBV2     | 24630          | 33079         | 1.39%           | 0.194%        |
| 13        | 12.639      | 1756          | 1760        | 1763         | rVB      | 61073          | 56938         | 2.40%           | 0.333%        |
| 14        | 12.868      | 1793          | 1799        | 1801         | rBV      | 63189          | 62519         | 2.64%           | 0.366%        |
| 15        | 13.010      | 1818          | 1823        | 1826         | rBV      | 2436239        | 2119276       | 89.33%          | 12.411%       |
| 16        | 13.563      | 1913          | 1917        | 1920         | rBV2     | 40815          | 43376         | 1.83%           | 0.254%        |
| 17        | 13.892      | 1970          | 1973        | 1976         | rBV      | 45995          | 40201         | 1.69%           | 0.235%        |
| 18        | 13.951      | 1976          | 1983        | 1984         | rBV6     | 26971          | 43688         | 1.84%           | 0.256%        |
| 19        | 14.068      | 1999          | 2003        | 2006         | rBV      | 736883         | 658783        | 27.77%          | 3.858%        |
| 20        | 14.157      | 2014          | 2018        | 2023         | rBV      | 34955          | 38313         | 1.61%           | 0.224%        |
| 21        | 14.210      | 2024          | 2027        | 2032         | rVB      | 50427          | 44773         | 1.89%           | 0.262%        |
| 22        | 14.515      | 2076          | 2079        | 2082         | rVB      | 50784          | 42255         | 1.78%           | 0.247%        |
| 23        | 14.827      | 2128          | 2132        | 2136         | rBV      | 37767          | 44441         | 1.87%           | 0.260%        |
| 24        | 15.121      | 2178          | 2182        | 2185         | rBV      | 18636          | 26575         | 1.12%           | 0.156%        |
| 25        | 15.174      | 2188          | 2191        | 2196         | rVB      | 32056          | 34550         | 1.46%           | 0.202%        |
| 26        | 15.562      | 2252          | 2257        | 2273         | rVB2     | 395584         | 529039        | 22.30%          | 3.098%        |




Sum of corrected areas: 17075698

Data Path : Z:\svoasrv\HPCHEM1\BNA\_F\Data\BF051122\  
Data File : BF128202.D  
Acq On : 11 May 2022 18:49  
Operator : CG\JU  
Sample : N2762-03  
Misc :  
ALS Vial : 13 Sample Multiplier: 1

Instrument :  
BNA\_F  
ClientSampleId :  
SB04

Quant Method : Z:\svoasrv\HPCHEM1\BNA\_F\Methods\8270-BF050922.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L  
TIC Integration Parameters: LSCINT.P

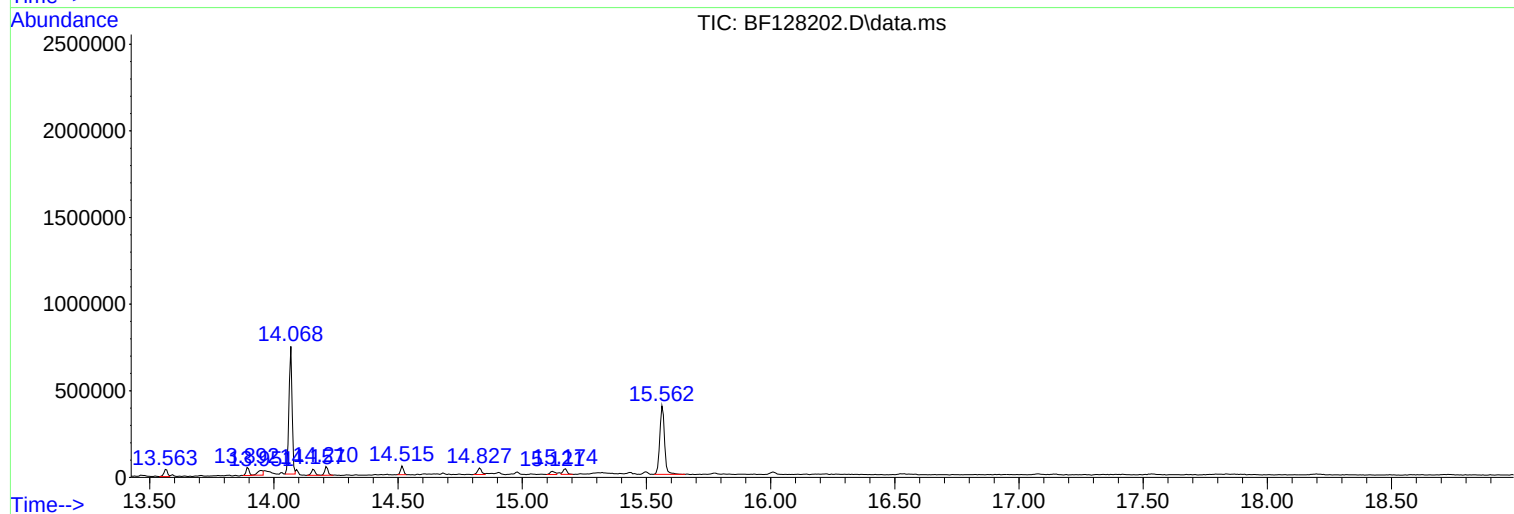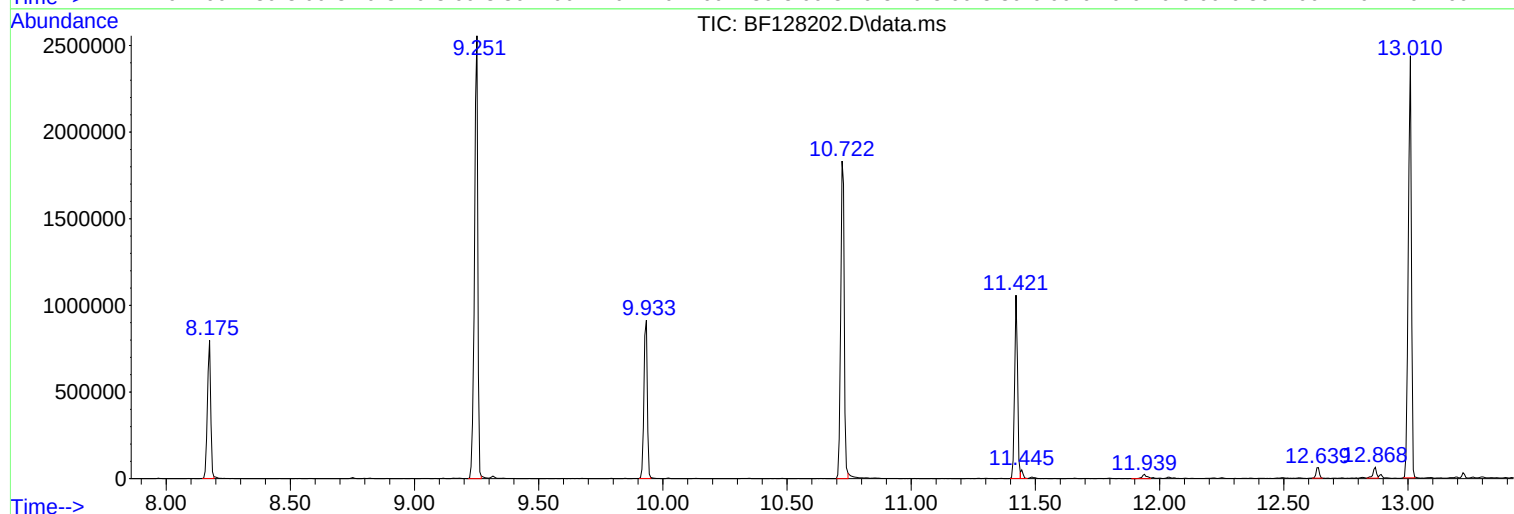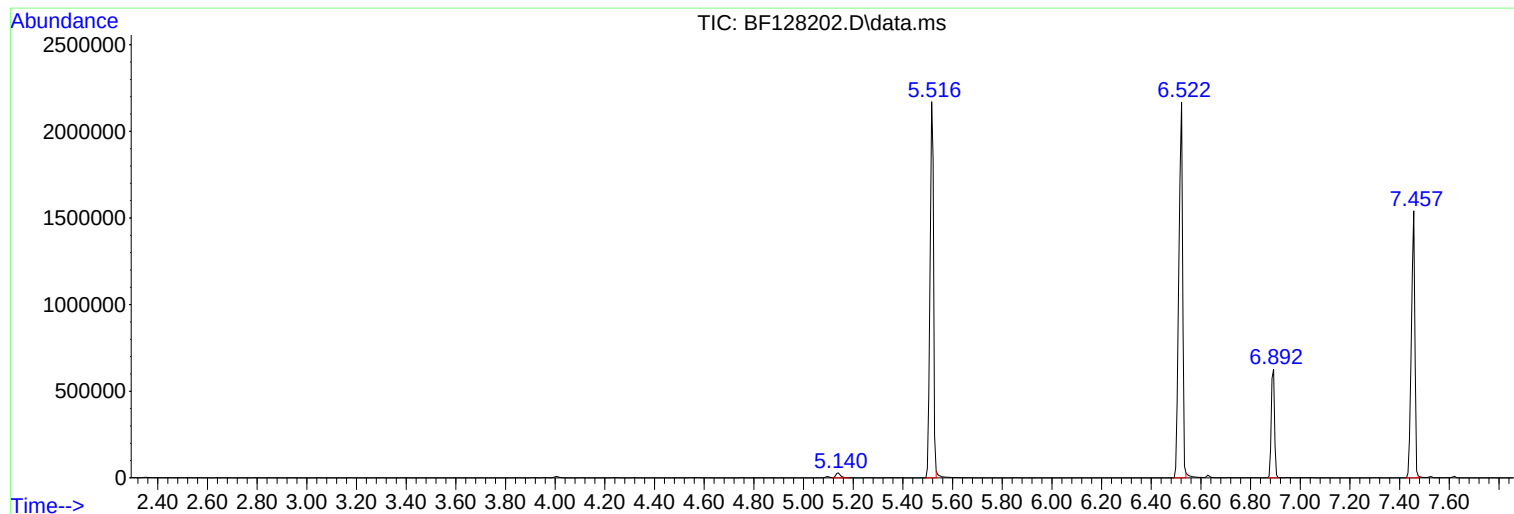

Data Path : Z:\svoasrv\HPCHEM1\BNA\_F\Data\BF051122\  
Data File : BF128202.D  
Acq On : 11 May 2022 18:49  
Operator : CG\JU  
Sample : N2762-03  
Misc :  
ALS Vial : 13 Sample Multiplier: 1

Instrument :  
BNA\_F  
ClientSampleId :  
SB04

Quant Method : Z:\svoasrv\HPCHEM1\BNA\_F\Methods\8270-BF050922.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L  
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

\*\*\*\*\*

Data Path : Z:\svoasrv\HPCHEM1\BNA\_F\Data\BF051122\  
Data File : BF128202.D  
Acq On : 11 May 2022 18:49  
Operator : CG\JU  
Sample : N2762-03  
Misc :  
ALS Vial : 13 Sample Multiplier: 1

Instrument :  
BNA\_F  
ClientSampleId :  
SB04

Quant Method : Z:\svoasrv\HPCHEM1\BNA\_F\Methods\8270-BF050922.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L  
TIC Integration Parameters: LSCINT.P

| TIC Top Hit name | RT | EstConc | Units | Response | # | RT | Resp | Conc |
|------------------|----|---------|-------|----------|---|----|------|------|
|------------------|----|---------|-------|----------|---|----|------|------|