

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF051122\
 Data File : BF128208.D
 Acq On : 11 May 2022 21:43
 Operator : CG\JU
 Sample : N2762-01
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 SB02

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF050922.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF128208.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.516	544	549	552	rBV	1908725	1729353	85.80%	13.196%
2	6.522	715	720	723	rBV	1850754	1817902	90.19%	13.872%
3	6.892	779	783	786	rBV	604013	494318	24.53%	3.772%
4	7.457	874	879	882	rBV	1311641	1227446	60.90%	9.366%
5	8.175	997	1001	1004	rBV	762537	624927	31.01%	4.769%
6	9.251	1179	1184	1187	rBV	2370052	2015528	100.00%	15.380%
7	9.933	1296	1300	1303	rBV	802356	686986	34.08%	5.242%
8	10.722	1430	1434	1448	rBV	1391418	1289808	63.99%	9.842%
9	11.422	1549	1553	1556	rBV	769575	631524	31.33%	4.819%
10	12.639	1757	1760	1765	rVB	55317	49195	2.44%	0.375%
11	12.869	1793	1799	1802	rBV	53654	53890	2.67%	0.411%
12	13.010	1818	1823	1826	rBV	1679015	1497578	74.30%	11.428%
13	14.033	1994	1997	1999	rBV	24915	23120	1.15%	0.176%
14	14.068	1999	2003	2006	rBV	518110	462129	22.93%	3.526%
15	14.157	2016	2018	2025	rVB	32996	36377	1.80%	0.278%
16	15.563	2253	2257	2267	rVB	336559	464863	23.06%	3.547%


Sum of corrected areas: 13104944

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF051122\
Data File : BF128208.D
Acq On : 11 May 2022 21:43
Operator : CG\JU
Sample : N2762-01
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
SB02

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF050922.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

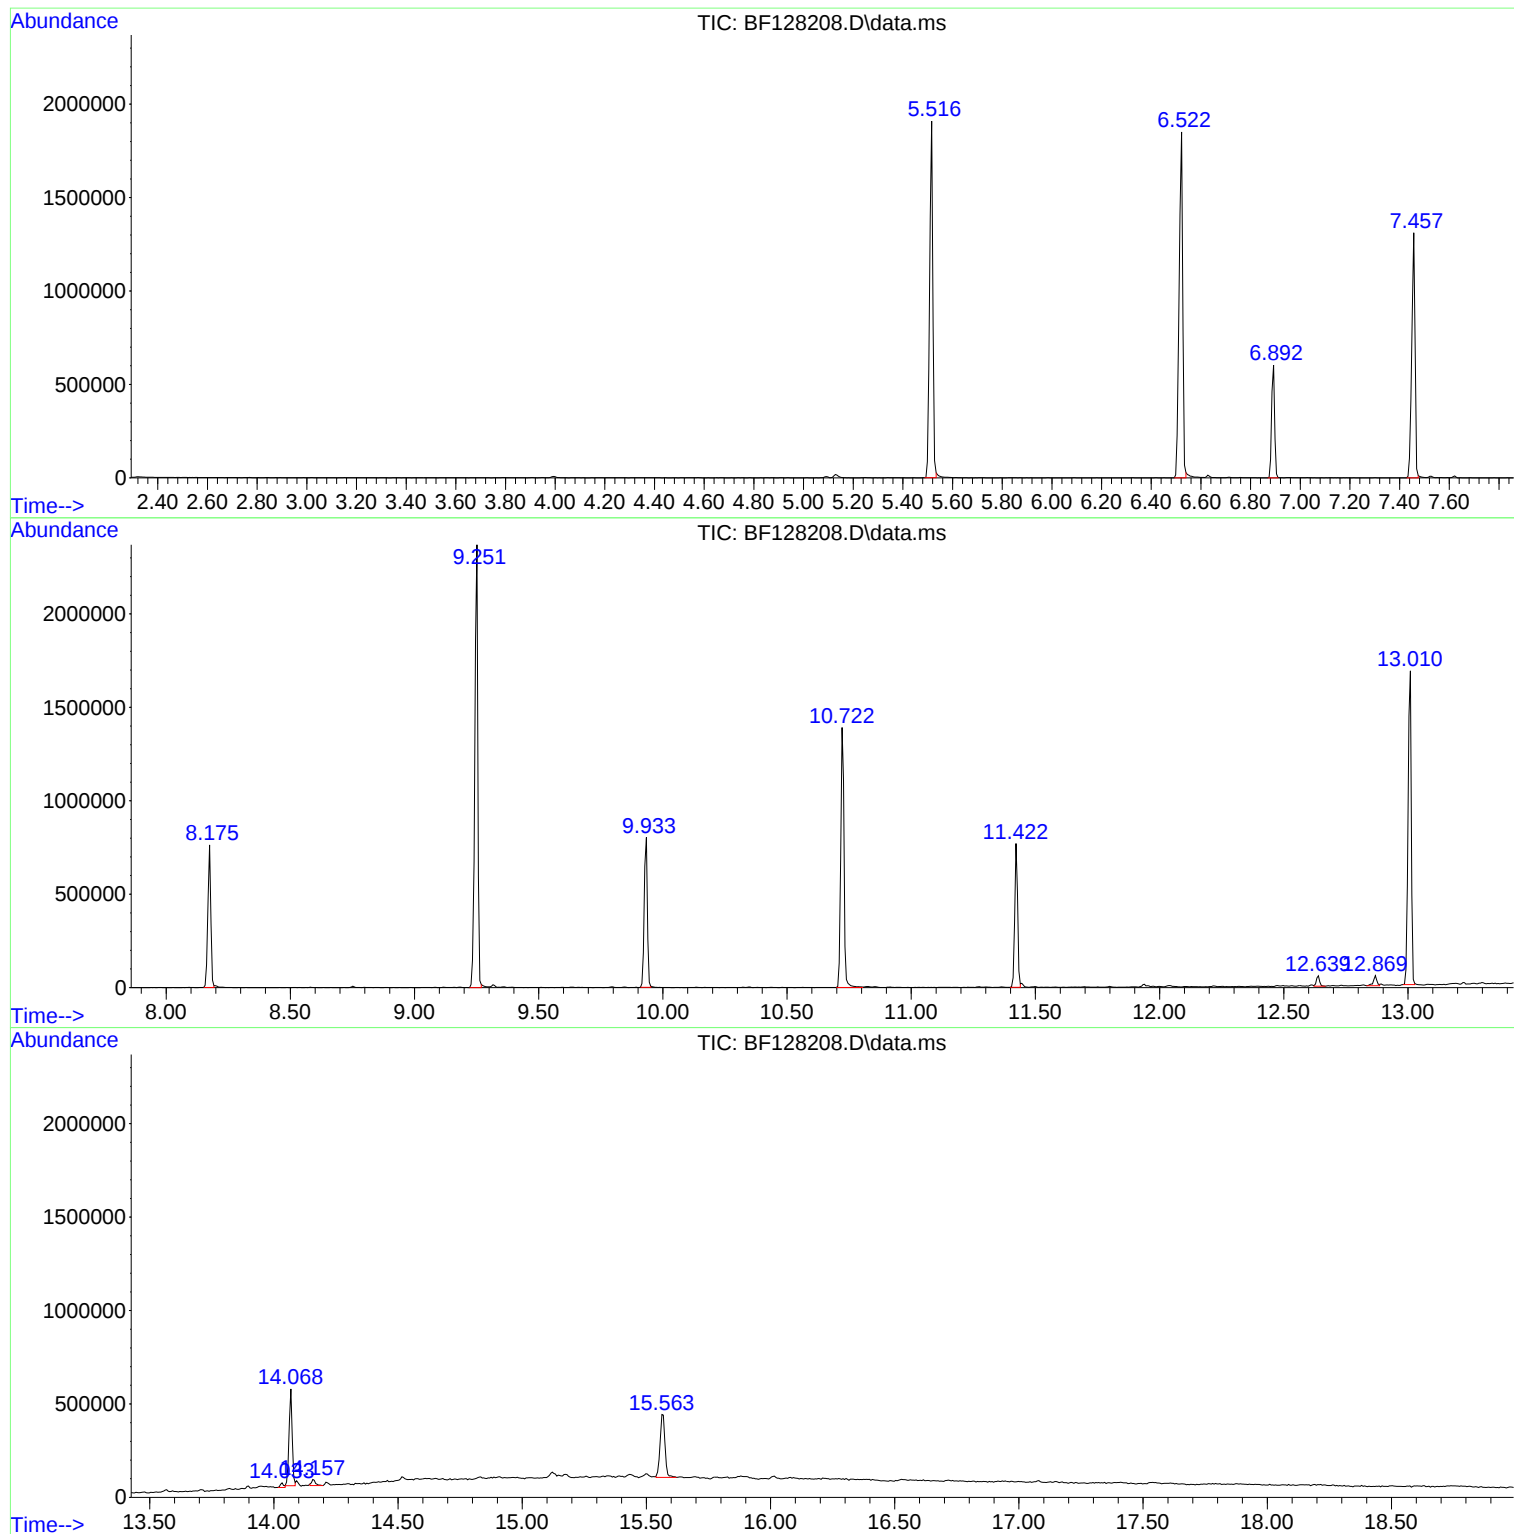

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF051122\
Data File : BF128208.D
Acq On : 11 May 2022 21:43
Operator : CG\JU
Sample : N2762-01
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
SB02

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF050922.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF051122\
Data File : BF128208.D
Acq On : 11 May 2022 21:43
Operator : CG\JU
Sample : N2762-01
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
SB02

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF050922.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------