

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF051122\
 Data File : BF128210.D
 Acq On : 11 May 2022 22:41
 Operator : CG\JU
 Sample : N2775-01
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 MH-35S

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF050922.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF128210.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.516	545	549	553	rBV	1943309	1994927	87.20%	14.182%
2	6.522	715	720	723	rBV	1872628	2042997	89.30%	14.524%
3	6.892	779	783	786	rBV	592770	480636	21.01%	3.417%
4	7.457	874	879	882	rBV	1442376	1379838	60.32%	9.810%
5	8.175	997	1001	1004	rBV	733319	595117	26.01%	4.231%
6	9.251	1179	1184	1187	rBV	2709452	2287696	100.00%	16.264%
7	9.933	1296	1300	1303	rBV	733585	619276	27.07%	4.403%
8	10.722	1430	1434	1449	rBV	1318265	1301511	56.89%	9.253%
9	11.422	1549	1553	1557	rBV	662203	556659	24.33%	3.957%
10	12.869	1793	1799	1802	rBV	21732	26609	1.16%	0.189%
11	13.010	1818	1823	1826	rBV	1977790	1678308	73.36%	11.931%
12	13.933	1976	1980	1995	rBV5	54219	192484	8.41%	1.368%
13	14.068	1999	2003	2006	rBV	502612	450226	19.68%	3.201%
14	14.157	2015	2018	2022	rBV	34911	40414	1.77%	0.287%
15	14.515	2077	2079	2085	rBV6	23730	26994	1.18%	0.192%
16	15.562	2253	2257	2264	rBV	292144	392522	17.16%	2.791%




Sum of corrected areas: 14066214

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF051122\
Data File : BF128210.D
Acq On : 11 May 2022 22:41
Operator : CG\JU
Sample : N2775-01
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
MH-35S

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF050922.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

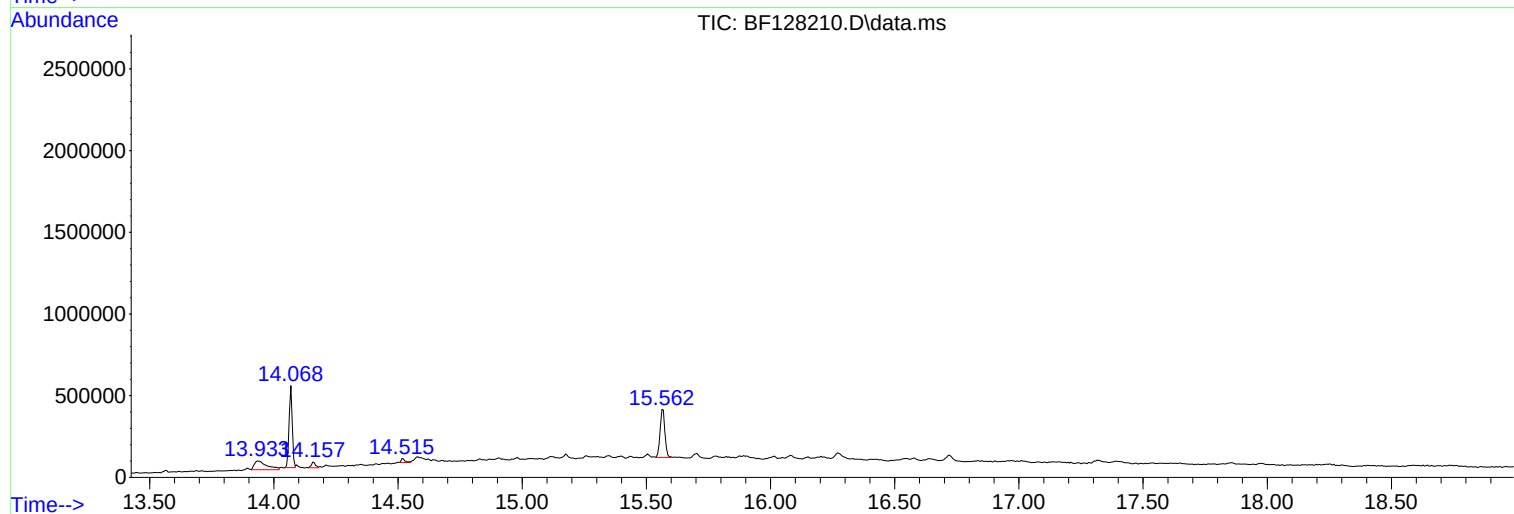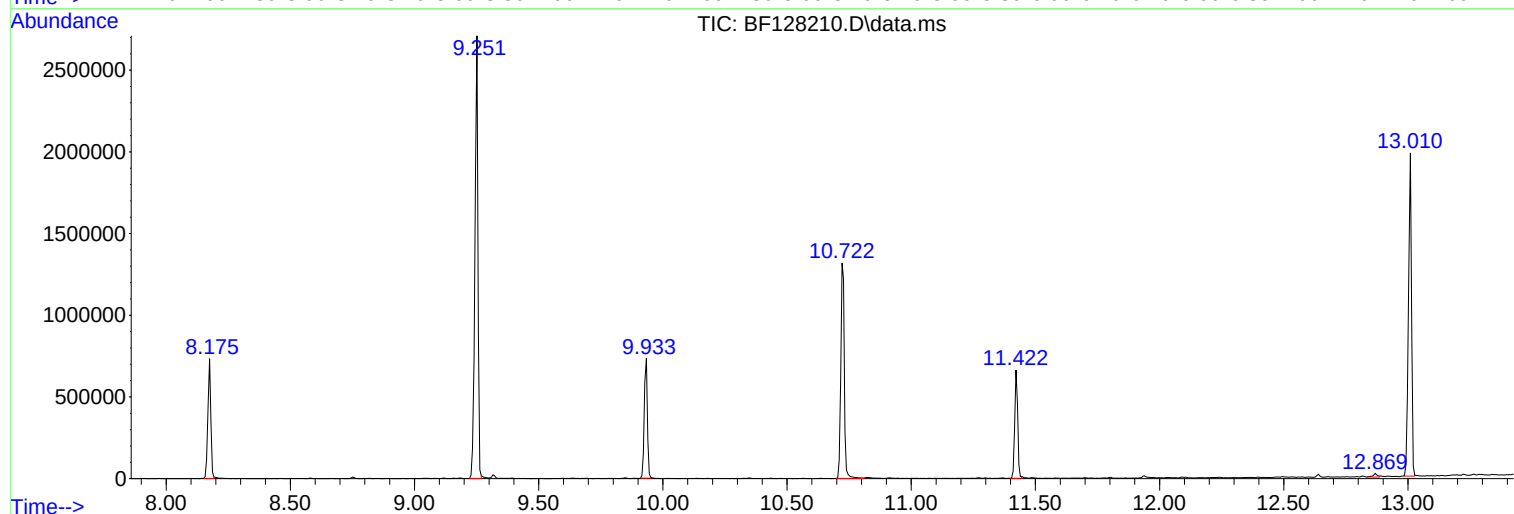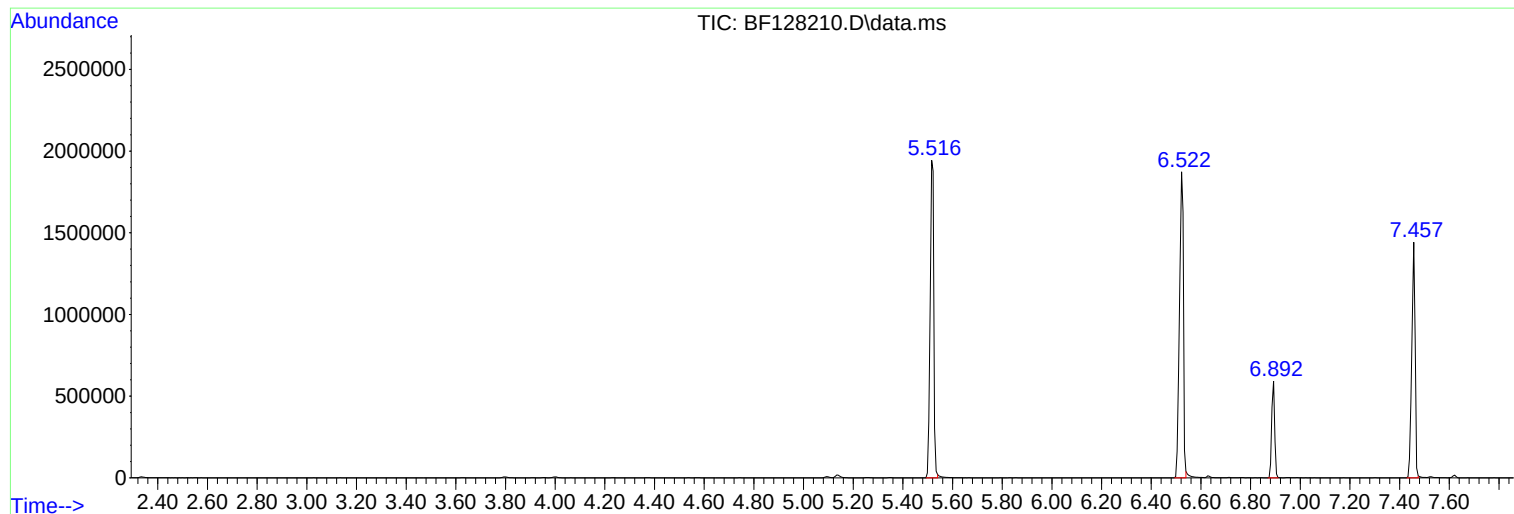

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF051122\
Data File : BF128210.D
Acq On : 11 May 2022 22:41
Operator : CG\JU
Sample : N2775-01
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
MH-35S

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF050922.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF051122\
Data File : BF128210.D
Acq On : 11 May 2022 22:41
Operator : CG\JU
Sample : N2775-01
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
MH-35S

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF050922.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------