


Data Path : Z:\svoasrv\HPCHEM1\BNA\_F\Data\BF051122\  
 Data File : BF128190.D  
 Acq On : 11 May 2022 12:55  
 Operator : CG\JU  
 Sample : DFTPP  
 Misc :  
 ALS Vial : 1 Sample Multiplier: 1

Instrument :  
 BNA\_F  
 ClientSampleId :  
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA\_F\Methods\8270-BF050922.M  
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 Last Update : Mon May 09 15:30:11 2022

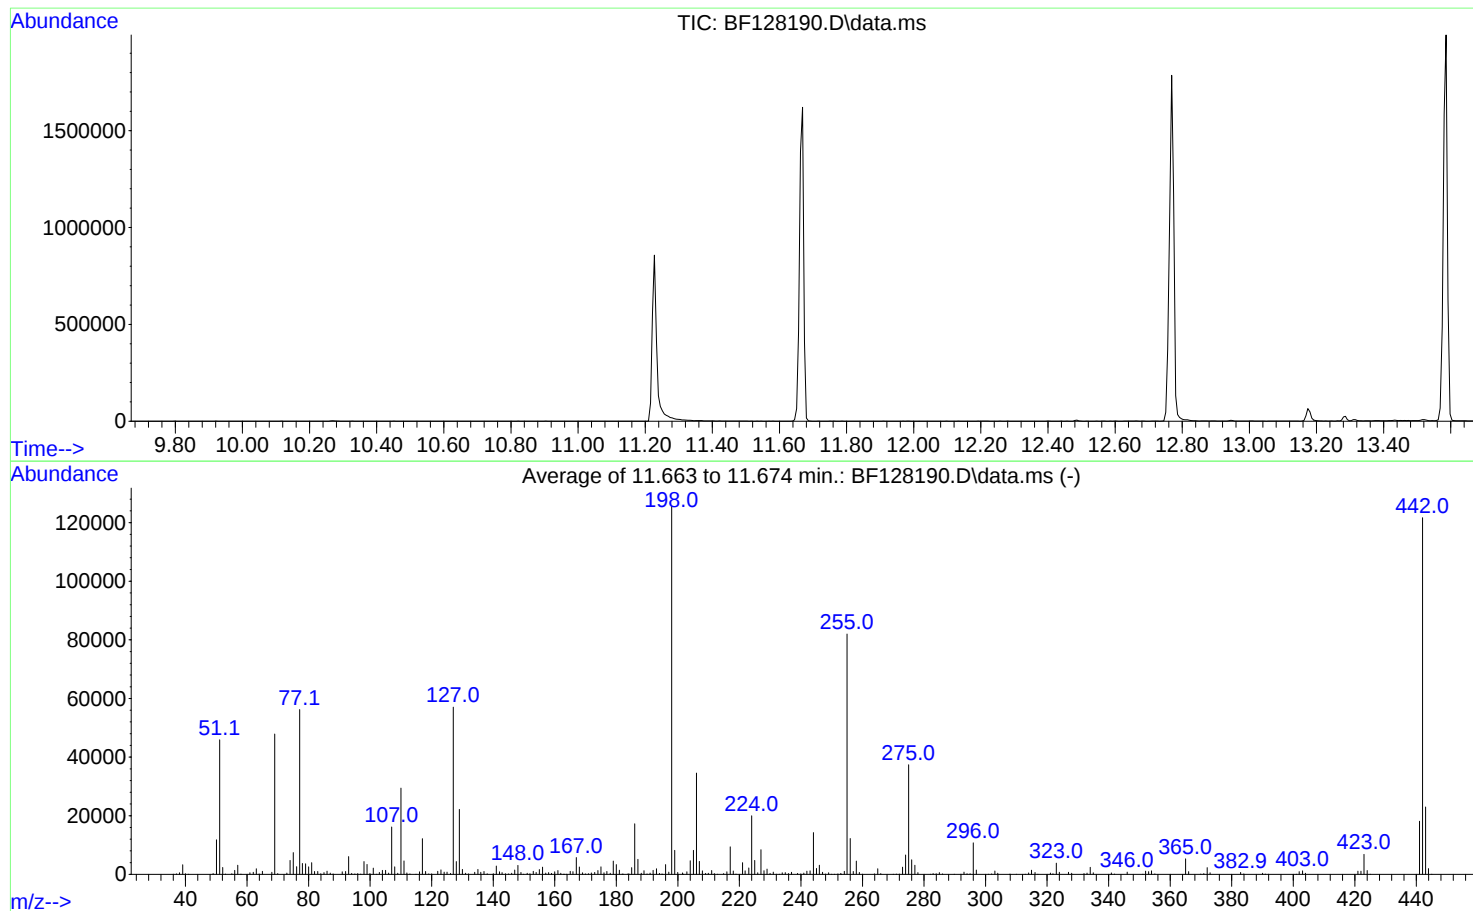




AutoFind: Scans 1594, 1595, 1596; Background Corrected with Scan 1588

| Target<br>Mass | Rel. to<br>Mass | Lower<br>Limit% | Upper<br>Limit% | Rel.<br>Abn% | Raw<br>Abn | Result<br>Pass/Fail |
|----------------|-----------------|-----------------|-----------------|--------------|------------|---------------------|
| 51             | 198             | 10              | 80              | 36.6         | 45926      | PASS                |
| 68             | 69              | 0.00            | 2               | 1.5          | 706        | PASS                |
| 69             | 198             | 0.00            | 100             | 38.1         | 47853      | PASS                |
| 70             | 69              | 0.00            | 2               | 0.5          | 255        | PASS                |
| 127            | 198             | 10              | 80              | 45.5         | 57055      | PASS                |
| 197            | 198             | 0.00            | 2               | 0.6          | 764        | PASS                |
| 198            | 198             | 100             | 100             | 100.0        | 125493     | PASS                |
| 199            | 198             | 5               | 9               | 6.5          | 8172       | PASS                |
| 275            | 198             | 10              | 60              | 29.8         | 37371      | PASS                |
| 365            | 198             | 1               | 100             | 4.2          | 5294       | PASS                |
| 441            | 198             | 0.01            | 100             | 14.5         | 18136      | PASS                |
| 442            | 442             | 50              | 100             | 100.0        | 121667     | PASS                |
| 443            | 442             | 15              | 24              | 18.9         | 22981      | PASS                |

Data Path : Z:\svoasrv\HPCHEM1\BNA\_F\Data\BF051122\  
 Data File : BF128190.D  
 Acq On : 11 May 2022 12:55  
 Operator : CG\JU  
 Sample : DFTPP  
 Misc :  
 ALS Vial : 1 Sample Multiplier: 1

Instrument :  
 BNA\_F  
 ClientSampleId :  
 DFTPP

Quant Time: May 12 09:44:59 2022  
 Quant Method : Z:\svoasrv\HPCHEM1\BNA\_F\Methods\8270-BF050922.M  
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 QLast Update : Mon May 09 15:30:11 2022  
 Response via : Initial Calibration

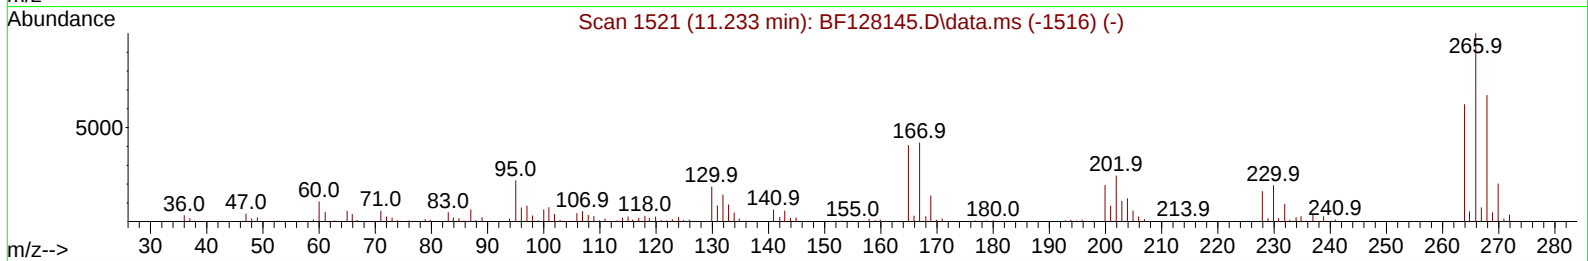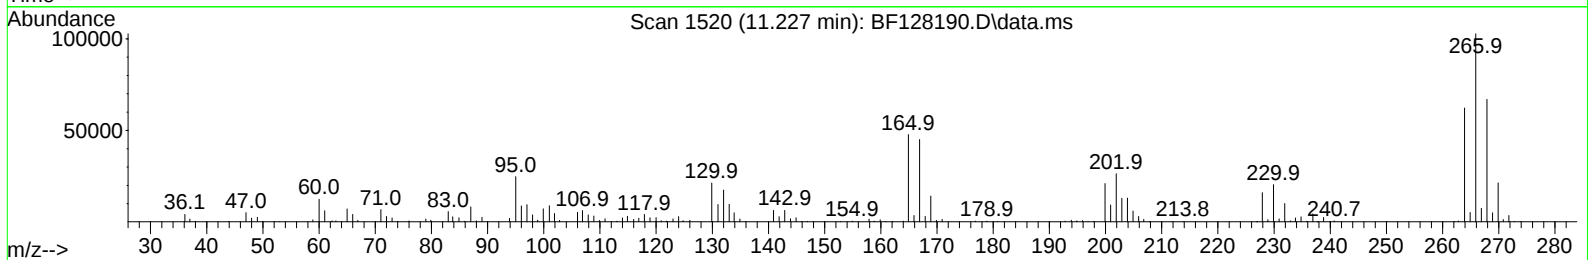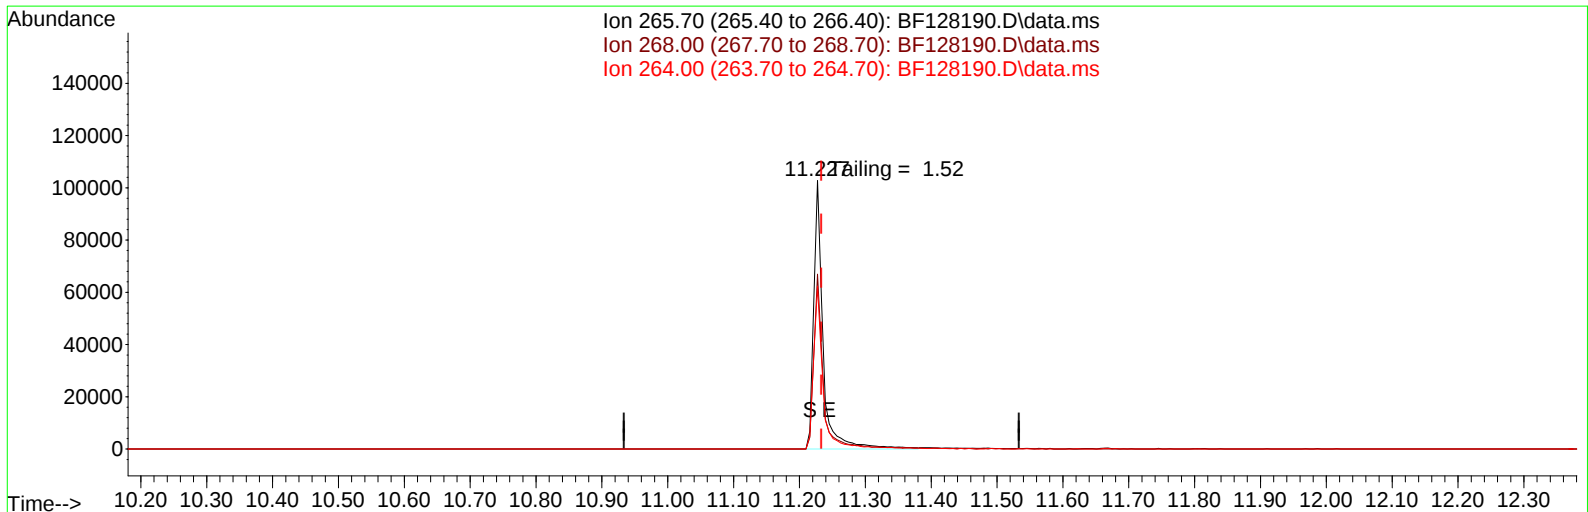

TIC: BF128190.D\data.ms

**(70) Pentachlorophenol (C)**

11.227min (-0.006) 38769.75 ng




response 102305

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 265.70 | 100.00 | 100.00 |
| 268.00 | 66.30  | 65.18  |
| 264.00 | 66.40  | 60.60  |
| 0.00   | 0.00   | 0.00   |

Data Path : Z:\svoasrv\HPCHEM1\BNA\_F\Data\BF051122\  
Data File : BF128190.D  
Acq On : 11 May 2022 12:55  
Operator : CG\JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Instrument :  
BNA\_F  
ClientSampleId :  
DFTPP

Quant Time: May 12 09:44:59 2022  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_F\Methods\8270-BF050922.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Mon May 09 15:30:11 2022  
Response via : Initial Calibration

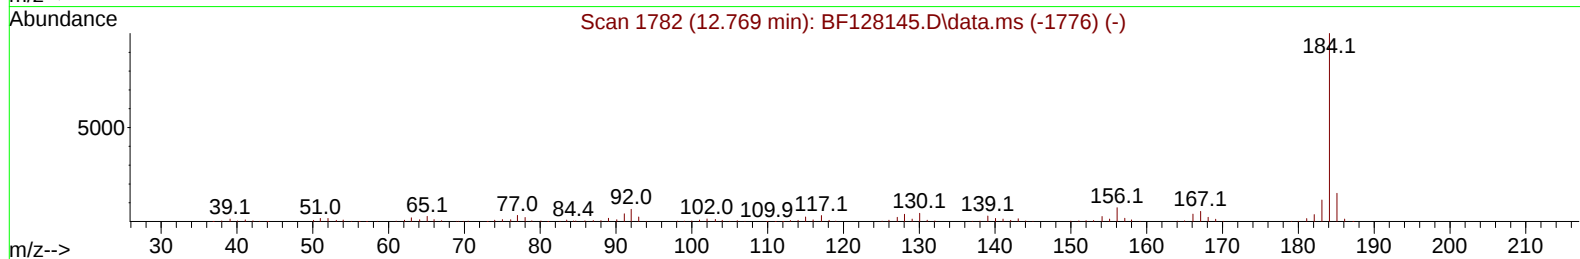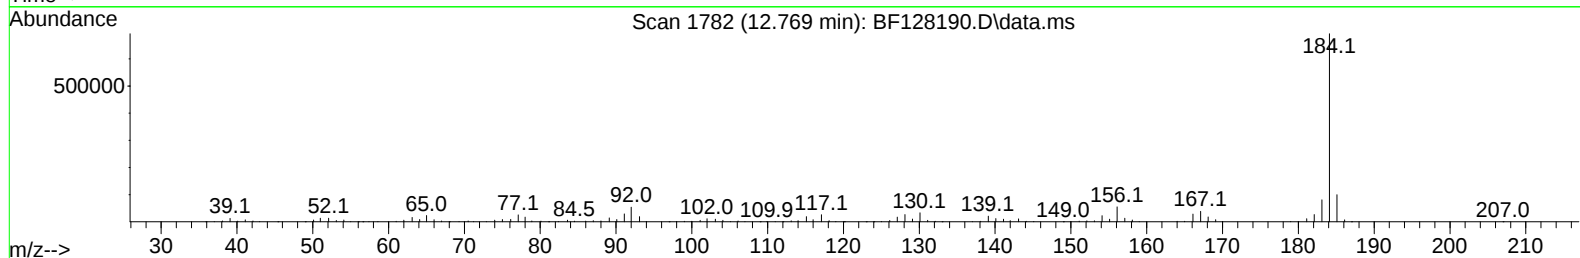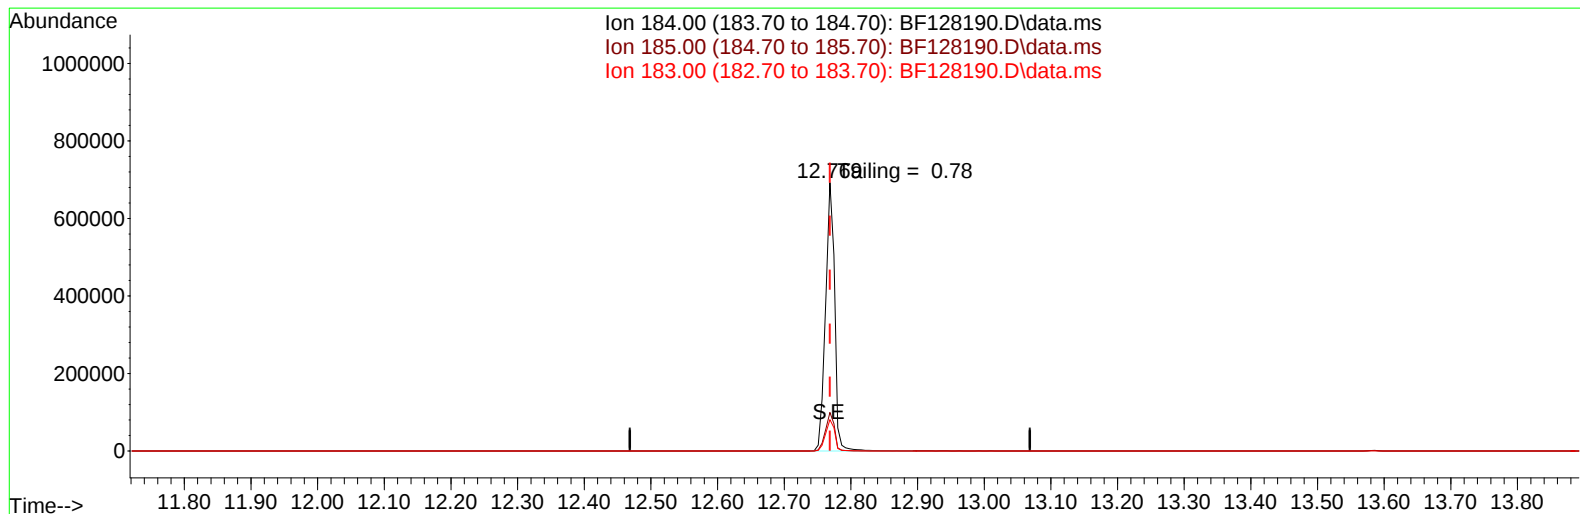

TIC: BF128190.D\data.ms

(77) Benzidine

12.769min (-0.000) 0.00 ng

response 659675

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 184.00 | 100.00 | 100.00 |
| 185.00 | 15.10  | 14.37  |
| 183.00 | 11.20  | 11.69  |
| 0.00   | 0.00   | 0.00   |

# DDT Breakdown

| Date          | Instrument Name  | DFTPP Data File    |
|---------------|------------------|--------------------|
| 5/11/2022     | BNA_F            | <u>BF128190.D</u>  |
|               |                  |                    |
|               |                  |                    |
| Compound Name | Response         | Retention Time     |
|               |                  |                    |
| DDT           | 330302           | 13.586             |
| DDD           | 6751             | 13.286             |
| DDE           | 672              | 12.945             |
|               |                  |                    |
|               |                  |                    |
| SUM(DDD+DDE)  | SUM(DDT+DDD+DDE) | % Breakdown Of DDT |
|               |                  |                    |
| 7423          | 337725           | 2.20               |
|               |                  |                    |

Instrument :  
BNA\_F  
ClientSampleId :  
DFTPP