
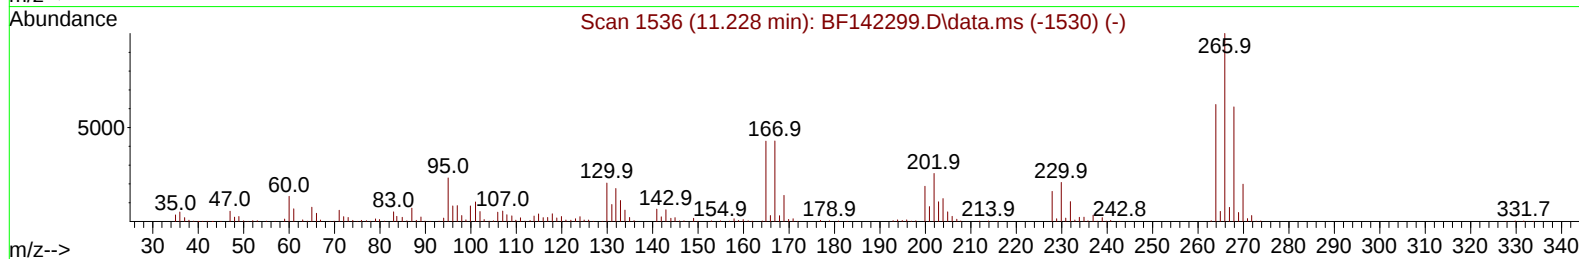
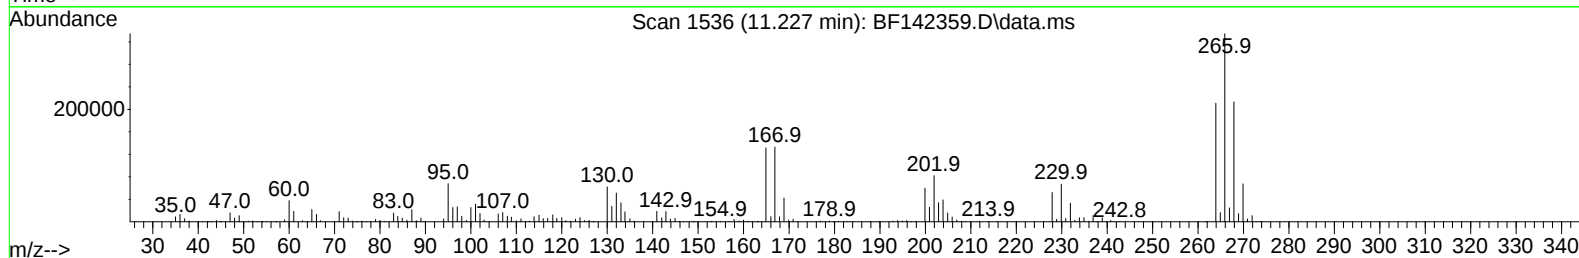


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF051425\
Data File : BF142359.D
Acq On : 14 May 2025 11:22
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 14 12:47:31 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF050525.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon May 05 18:41:44 2025
Response via : Initial Calibration

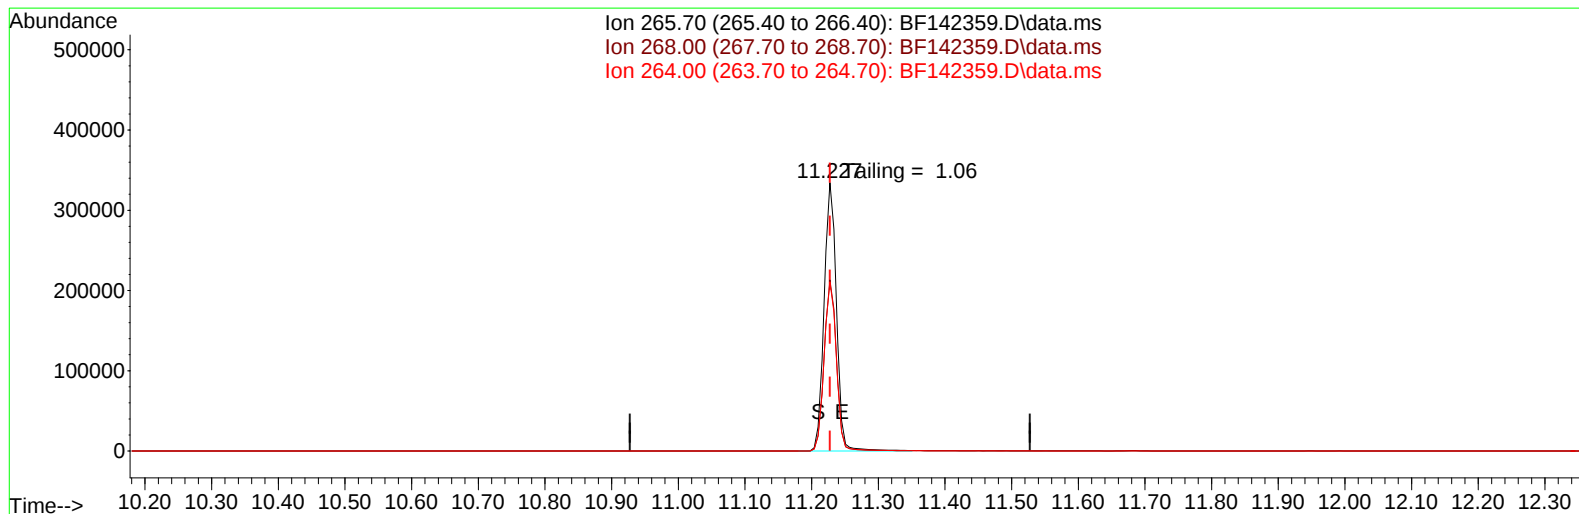

TIC: BF142359.D\data.ms

(70) Pentachlorophenol (C)




11.227min (-0.000) 177289.14 ng

response 430200

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	60.90	63.74
264.00	62.20	63.05
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF051425\
Data File : BF142359.D
Acq On : 14 May 2025 11:22
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 14 12:47:31 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF050525.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon May 05 18:41:44 2025
Response via : Initial Calibration

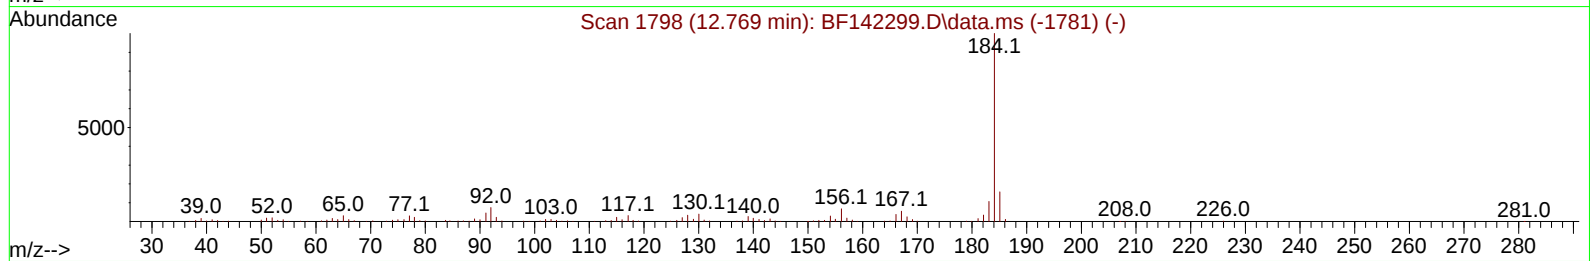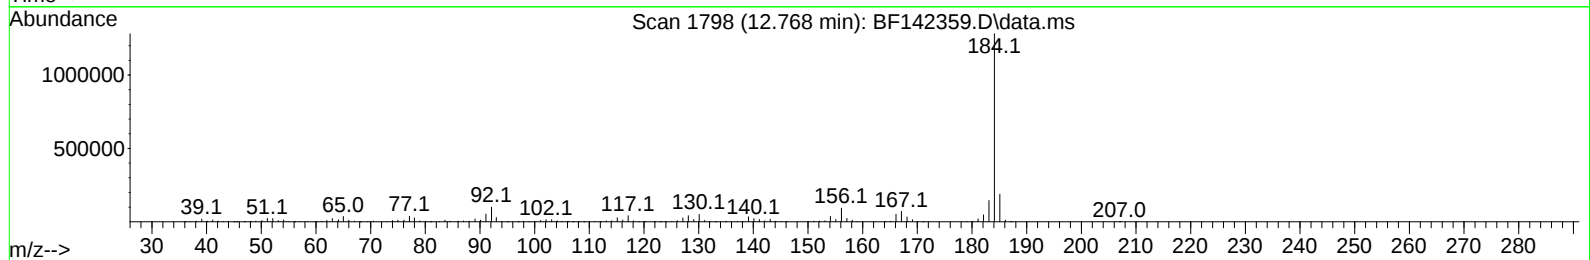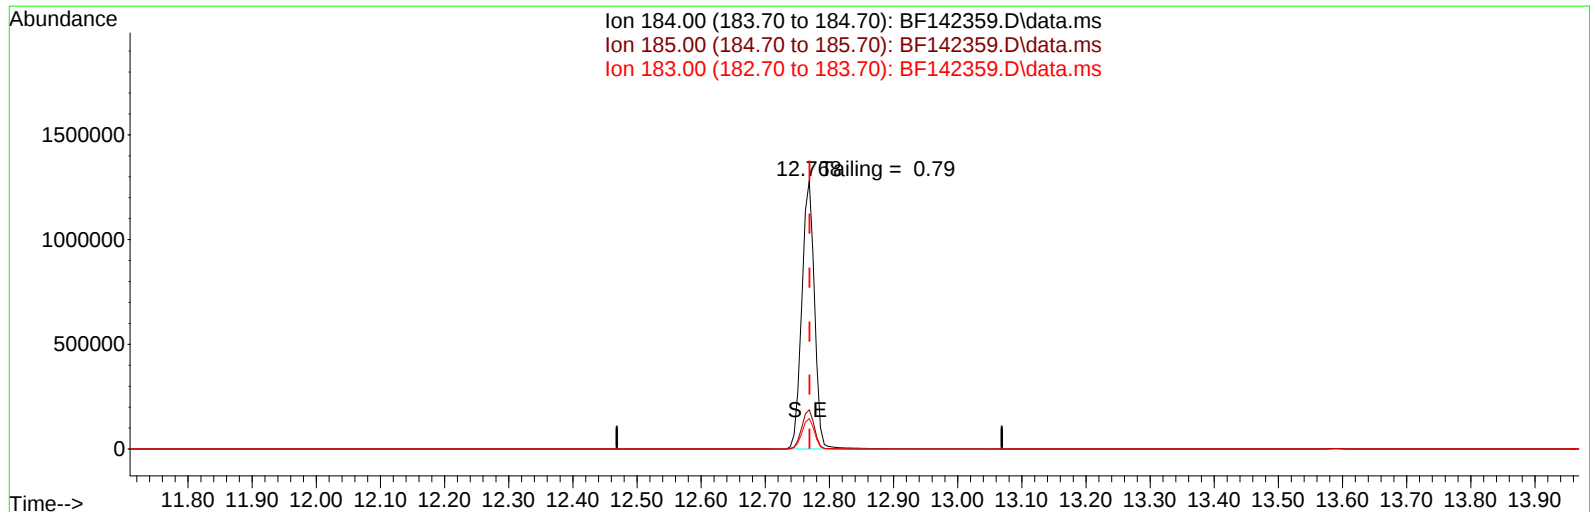

TIC: BF142359.D\data.ms

(77) Benzidine**12.768min (-0.001) 344992.34 ng****response 1767995**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.70	14.65
183.00	10.70	11.35
0.00	0.00	0.00