
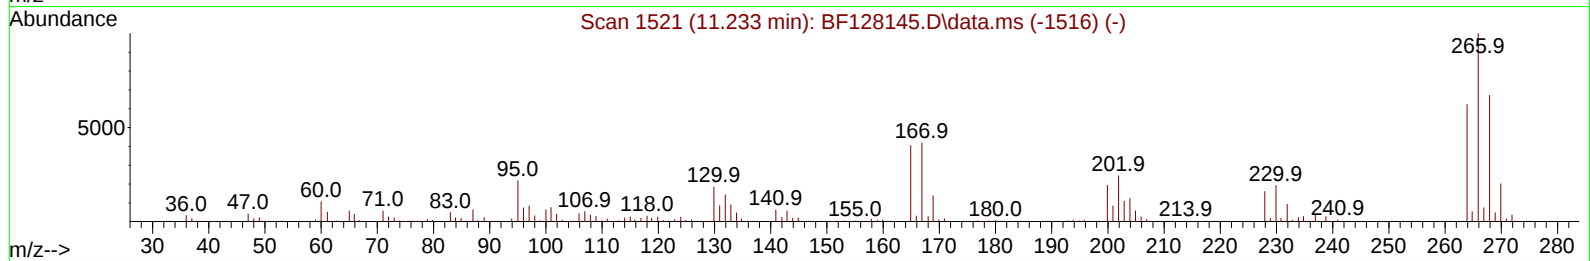
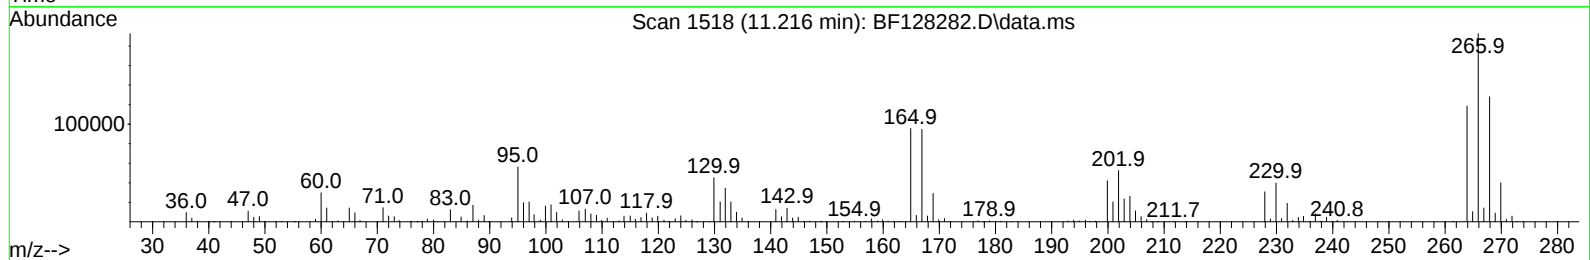


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF051722\
Data File : BF128282.D
Acq On : 17 May 2022 10:37
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 18 04:23:09 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF050922.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed May 18 01:31:11 2022
Response via : Initial Calibration

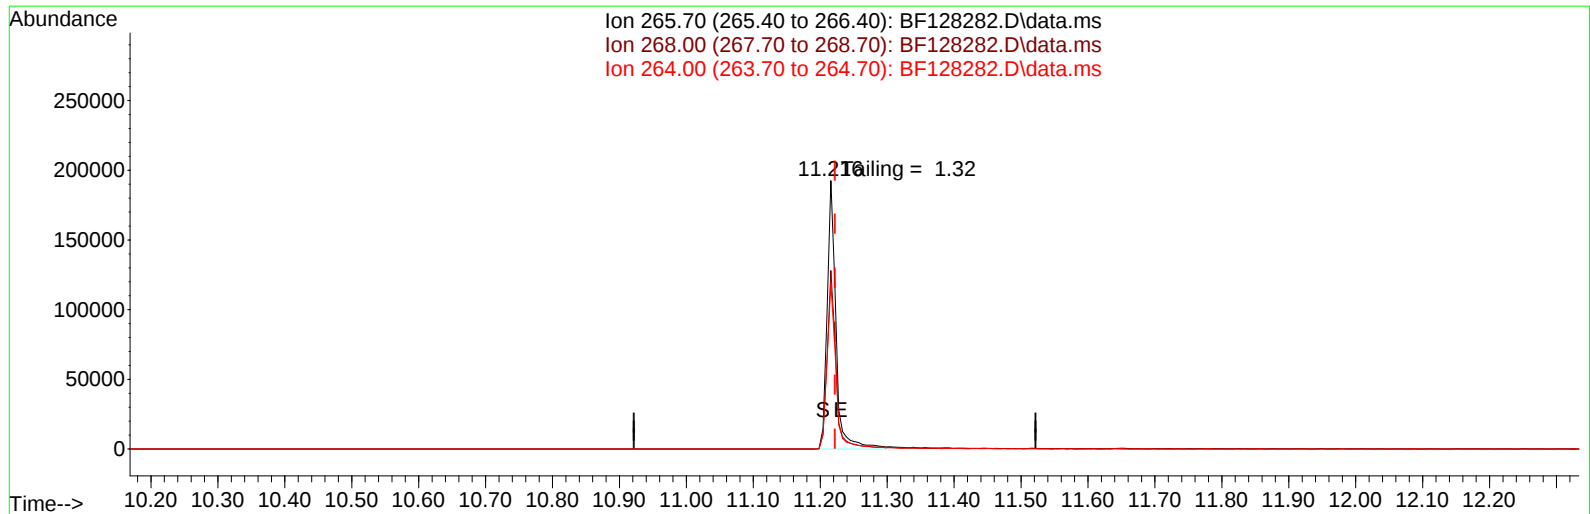

TIC: BF128282.D\data.ms

(70) Pentachlorophenol (C)




11.216min (-0.006) 545717.28 ng

response 180783

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	66.30	66.46
264.00	66.40	61.54
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF051722\
Data File : BF128282.D
Acq On : 17 May 2022 10:37
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 18 04:23:09 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF050922.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed May 18 01:31:11 2022
Response via : Initial Calibration

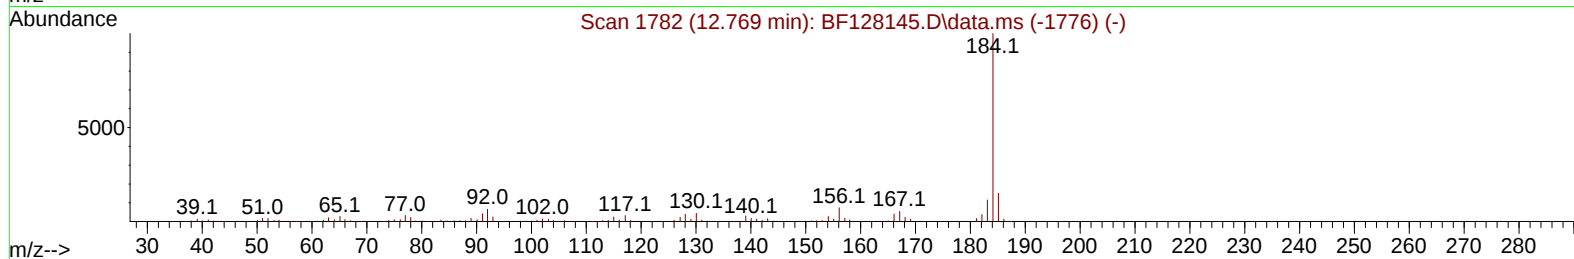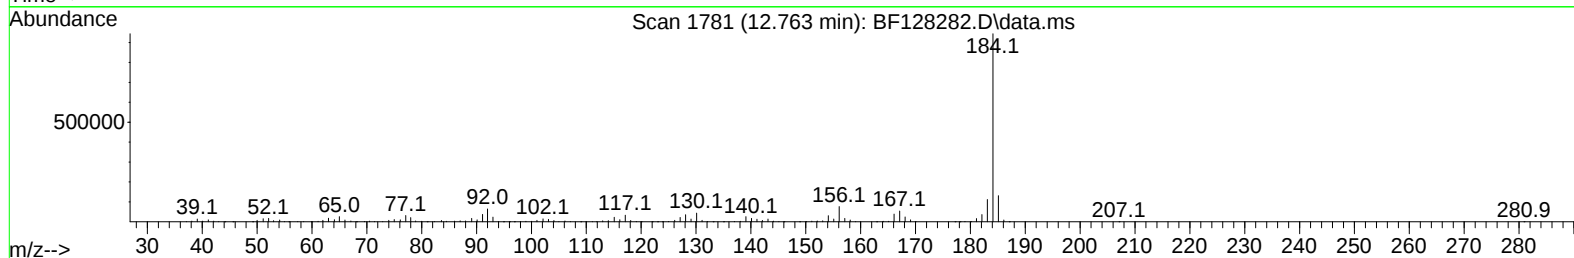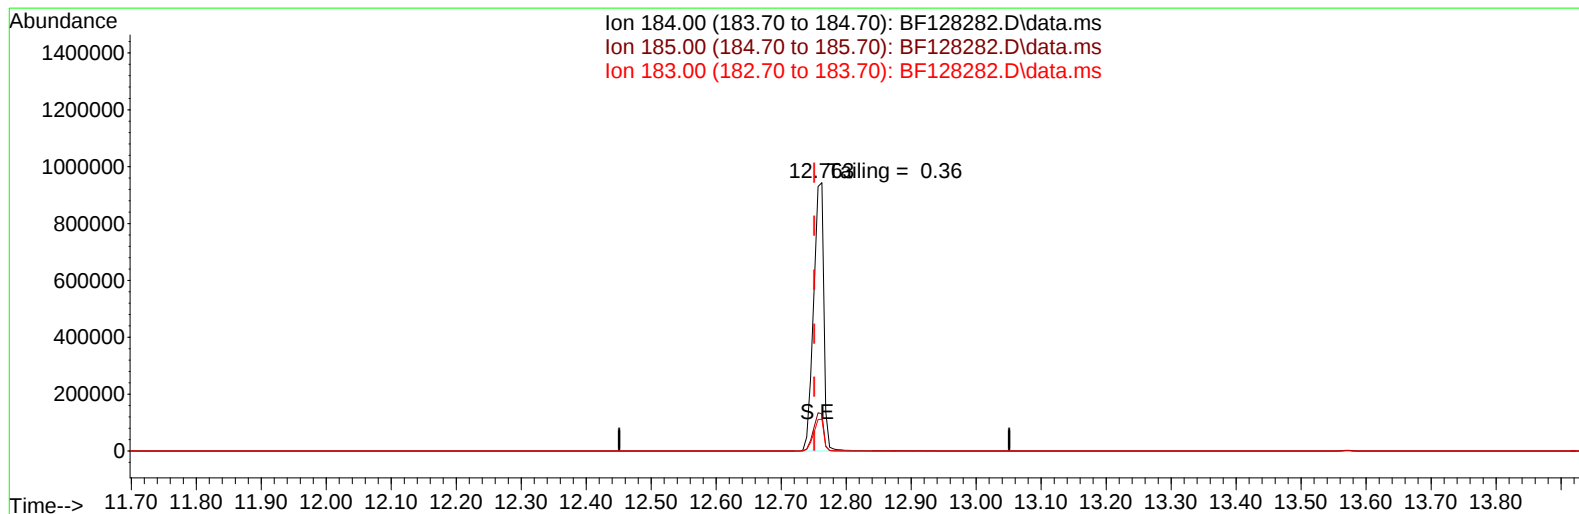

TIC: BF128282.D\data.ms

(77) Benzidine**12.763min (+ 0.012) 106474.37 ng****response 1046949**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.10	13.86
183.00	11.20	11.83
0.00	0.00	0.00