

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF051722\
 Data File : BF128287.D
 Acq On : 17 May 2022 13:10
 Operator : CG\JU
 Sample : PB144839BL
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB144839BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF050922.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF128287.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.516	544	549	552	rBV	3305295	3322081	80.60%	13.124%
2	6.510	712	718	721	rBV	2901094	3459944	83.95%	13.669%
3	6.875	776	780	783	rBV	858498	712895	17.30%	2.816%
4	7.445	870	877	880	rBV	2040436	2395409	58.12%	9.463%
5	8.157	993	998	1002	rBV	966727	925863	22.46%	3.658%
6	9.233	1174	1181	1184	rBV	3578278	4085834	99.13%	16.141%
7	9.916	1291	1297	1301	rBV	1188315	1054673	25.59%	4.167%
8	10.710	1426	1432	1436	rBV	2356310	2537883	61.58%	10.026%
9	11.410	1545	1551	1554	rBV	1304206	1089773	26.44%	4.305%
10	13.004	1816	1822	1825	rBV	4224116	4121520	100.00%	16.282%
11	14.057	1997	2001	2005	rBV	955904	863317	20.95%	3.411%
12	15.551	2249	2255	2264	rBV	571651	743776	18.05%	2.938%




Sum of corrected areas: 25312968

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF051722\
Data File : BF128287.D
Acq On : 17 May 2022 13:10
Operator : CG\JU
Sample : PB144839BL
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB144839BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF050922.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

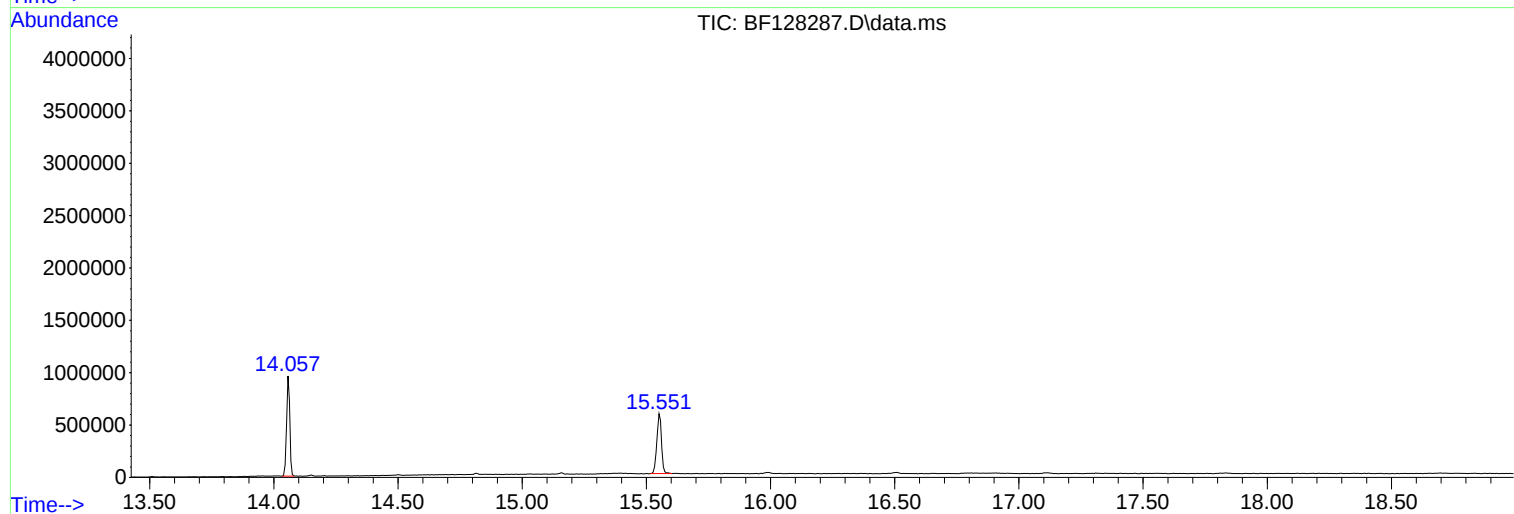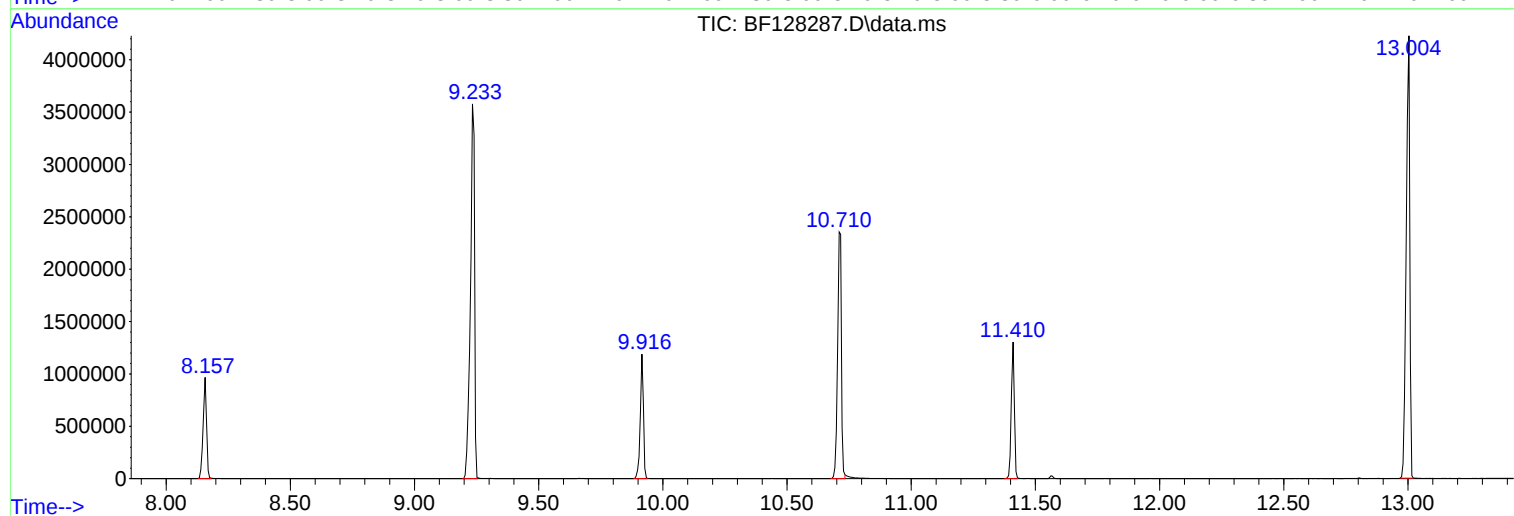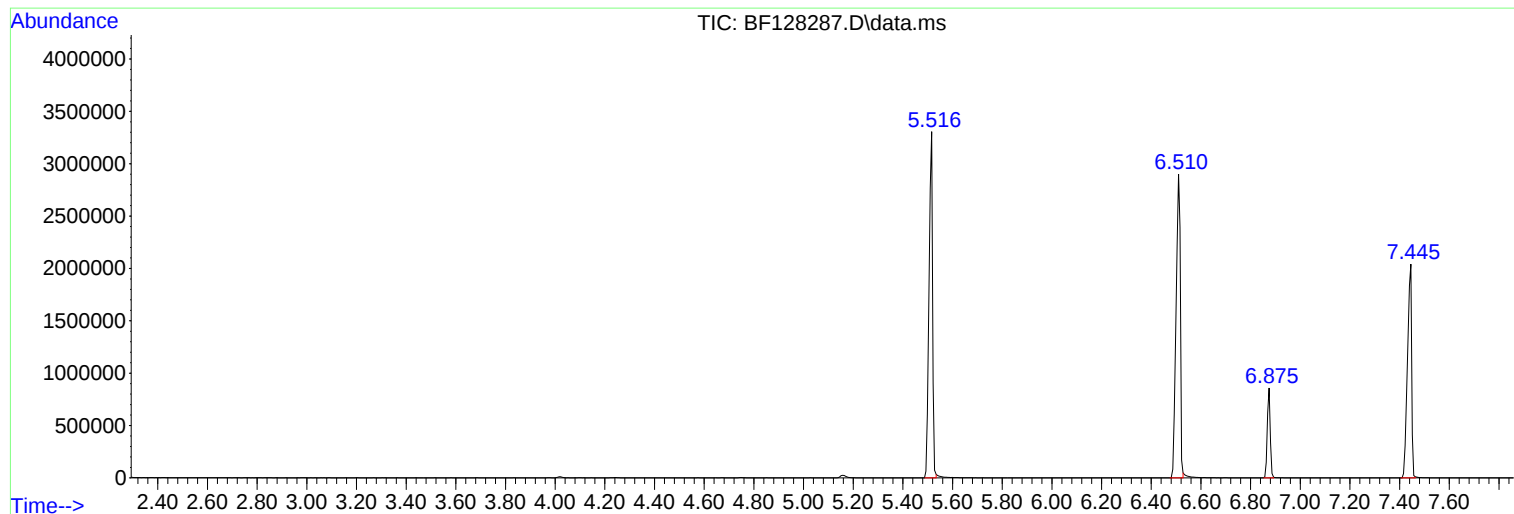

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF051722\
Data File : BF128287.D
Acq On : 17 May 2022 13:10
Operator : CG\JU
Sample : PB144839BL
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB144839BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF050922.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF051722\
Data File : BF128287.D
Acq On : 17 May 2022 13:10
Operator : CG\JU
Sample : PB144839BL
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB144839BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF050922.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------