

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF051722\
 Data File : BF128290.D
 Acq On : 17 May 2022 14:45
 Operator : CG\JU
 Sample : N2878-13
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 P007-SS022-0006-01

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF050922.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF128290.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.099	474	478	485	rVB	45607	52451	2.85%	0.413%
2	5.493	542	545	556	rBV	1485014	1477285	80.24%	11.644%
3	6.504	713	717	720	rBV	1676889	1503776	81.68%	11.853%
4	6.875	776	780	783	rBV	627067	513588	27.90%	4.048%
5	7.440	871	876	879	rBV	1252519	1059203	57.53%	8.349%
6	8.157	994	998	1002	rBV	807563	666137	36.18%	5.251%
7	9.234	1176	1181	1184	rBV	2183565	1841037	100.00%	14.511%
8	9.916	1293	1297	1300	rBV	943446	760710	41.32%	5.996%
9	10.710	1428	1432	1435	rBV	1208211	1109079	60.24%	8.742%
10	11.410	1547	1551	1554	rBV	905957	797622	43.32%	6.287%
11	12.992	1816	1820	1824	rBV	1986188	1822742	99.01%	14.367%
12	13.898	1970	1974	1981	rVB6	40112	82663	4.49%	0.652%
13	14.022	1992	1995	1997	rBV2	37444	38665	2.10%	0.305%
14	14.057	1997	2001	2005	rVV	574129	526415	28.59%	4.149%
15	15.551	2250	2255	2260	rVB	360097	435545	23.66%	3.433%


Sum of corrected areas: 12686918

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF051722\
Data File : BF128290.D
Acq On : 17 May 2022 14:45
Operator : CG\JU
Sample : N2878-13
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
P007-SS022-0006-01

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF050922.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

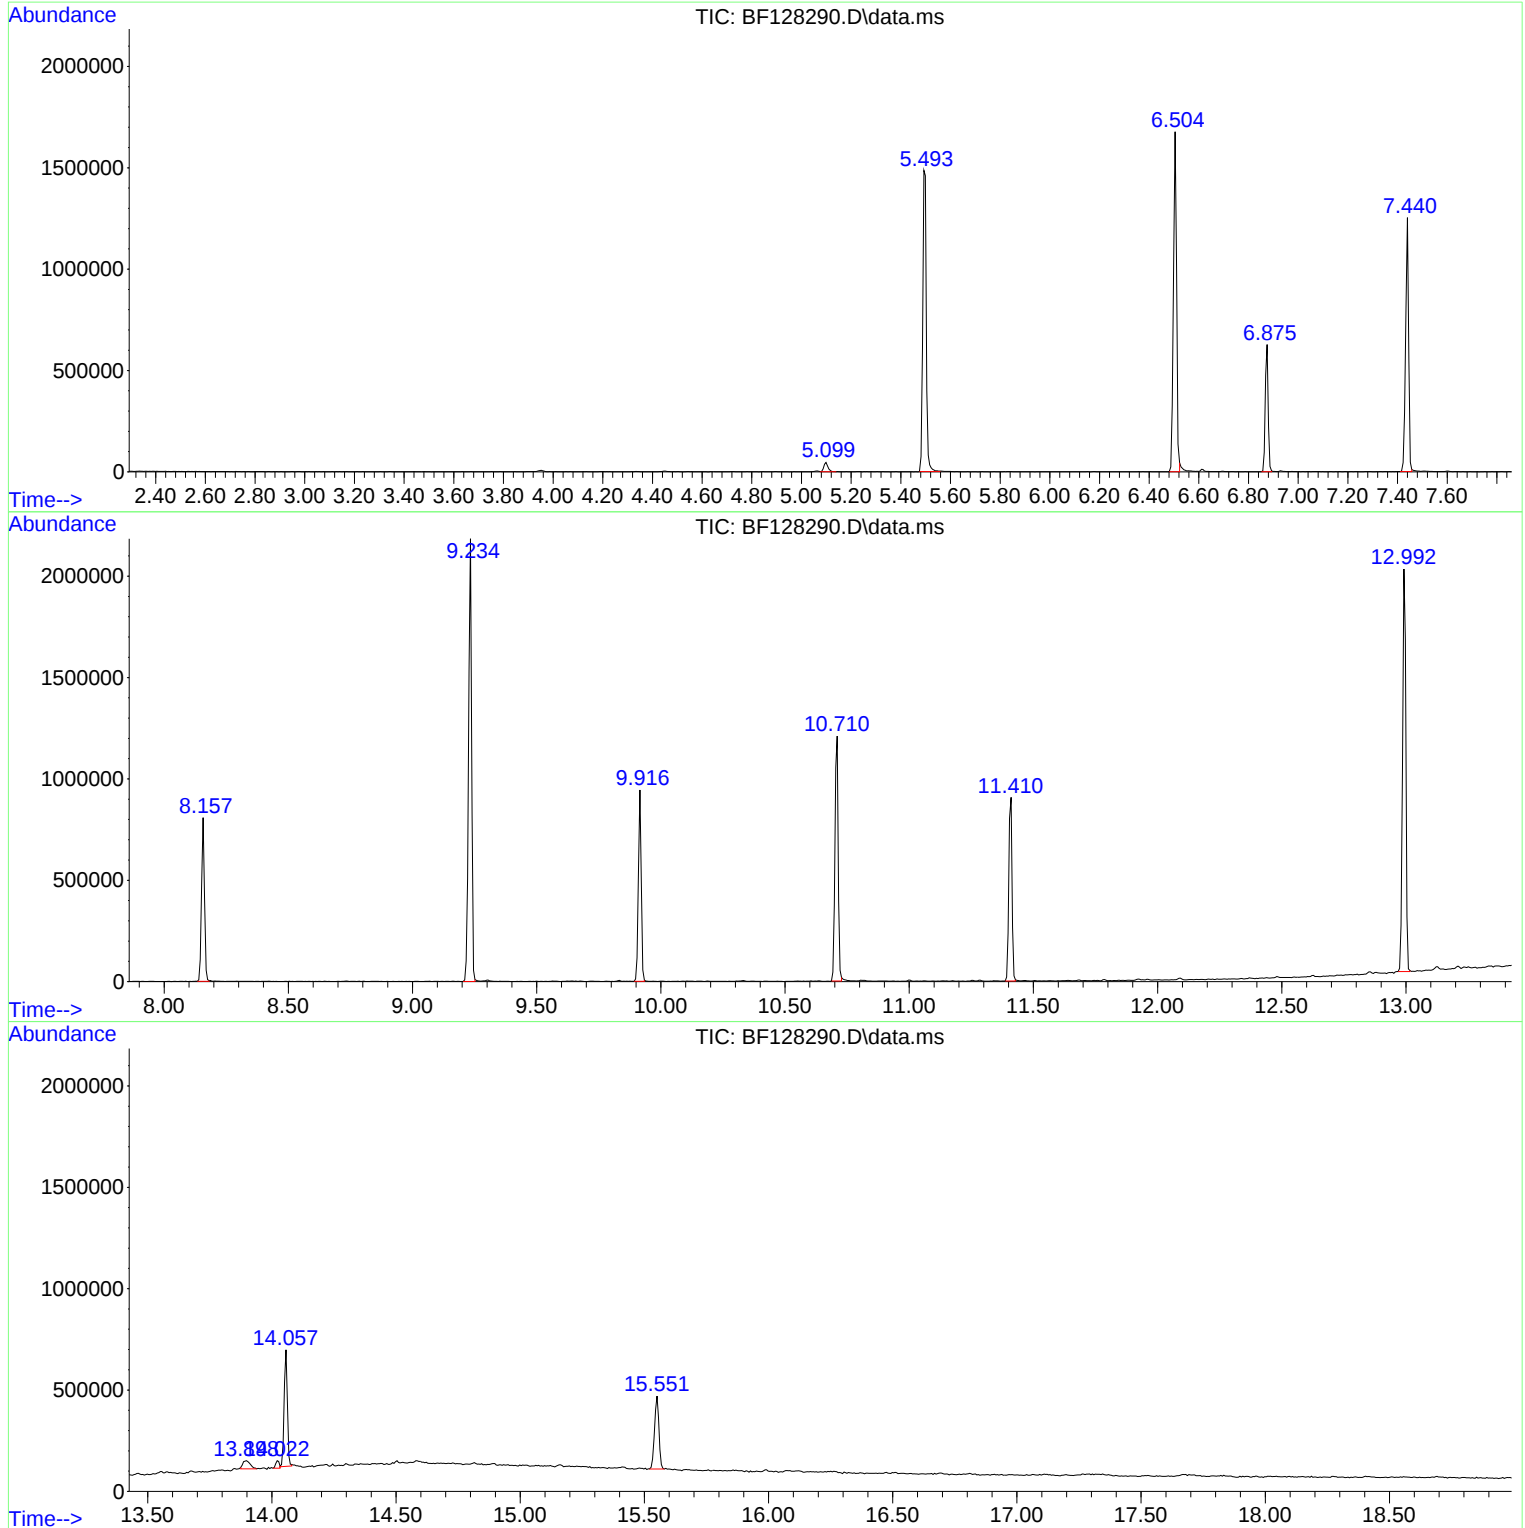

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF051722\
Data File : BF128290.D
Acq On : 17 May 2022 14:45
Operator : CG\JU
Sample : N2878-13
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
P007-SS022-0006-01

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF050922.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF051722\
Data File : BF128290.D
Acq On : 17 May 2022 14:45
Operator : CG\JU
Sample : N2878-13
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
P007-SS022-0006-01

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF050922.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------