

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF051722\
 Data File : BF128293.D
 Acq On : 17 May 2022 16:14
 Operator : CG\JU
 Sample : N2881-02
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 SLP-1

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF050922.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF128293.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.110	476	480	487	rVB	33633	42163	1.78%	0.251%
2	5.499	542	546	561	rBV	2227686	2072972	87.34%	12.354%
3	6.510	713	718	721	rBV	2026633	2120187	89.32%	12.636%
4	6.875	776	780	783	rBV	603899	490405	20.66%	2.923%
5	7.440	871	876	879	rBV	1526555	1427818	60.15%	8.509%
6	8.157	994	998	1001	rBV	763605	628635	26.48%	3.746%
7	9.234	1176	1181	1184	rBV	2719840	2373576	100.00%	14.146%
8	9.916	1293	1297	1300	rBV	854996	705363	29.72%	4.204%
9	10.710	1428	1432	1435	rBV	1749415	1519484	64.02%	9.056%
10	11.410	1547	1551	1553	rBV	779190	710443	29.93%	4.234%
11	11.433	1553	1555	1558	rVB	132954	103867	4.38%	0.619%
12	11.910	1631	1636	1639	rBV2	32642	49019	2.07%	0.292%
13	11.939	1639	1641	1644	rVB	35119	29018	1.22%	0.173%
14	12.022	1651	1655	1657	rBV2	39681	38855	1.64%	0.232%
15	12.622	1754	1757	1761	rBV	199872	171866	7.24%	1.024%
16	12.857	1791	1797	1802	rBV	181057	204101	8.60%	1.216%
17	12.992	1816	1820	1824	rBV	1992895	1851409	78.00%	11.034%
18	13.469	1897	1901	1905	rBV2	33700	36287	1.53%	0.216%
19	13.904	1969	1975	1983	rVB5	55970	123061	5.18%	0.733%
20	14.057	1996	2001	2004	rBV2	517397	553810	23.33%	3.301%
21	14.080	2004	2005	2012	rVB	85693	60568	2.55%	0.361%
22	14.892	2140	2143	2146	rVB	56623	53348	2.25%	0.318%
23	15.110	2176	2180	2183	rBV	66989	99668	4.20%	0.594%
24	15.421	2229	2233	2240	rBV2	57638	104498	4.40%	0.623%
25	15.486	2240	2244	2249	rVB	60159	78050	3.29%	0.465%
26	15.551	2249	2255	2259	rBV	390605	514833	21.69%	3.068%
27	15.810	2294	2299	2307	rBV	213726	377799	15.92%	2.252%
28	17.057	2508	2511	2524	rVB2	31949	76455	3.22%	0.456%
29	18.727	2789	2795	2805	rVB3	58425	161739	6.81%	0.964%




Sum of corrected areas: 16779297

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF051722\
Data File : BF128293.D
Acq On : 17 May 2022 16:14
Operator : CG\JU
Sample : N2881-02
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
SLP-1

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF050922.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

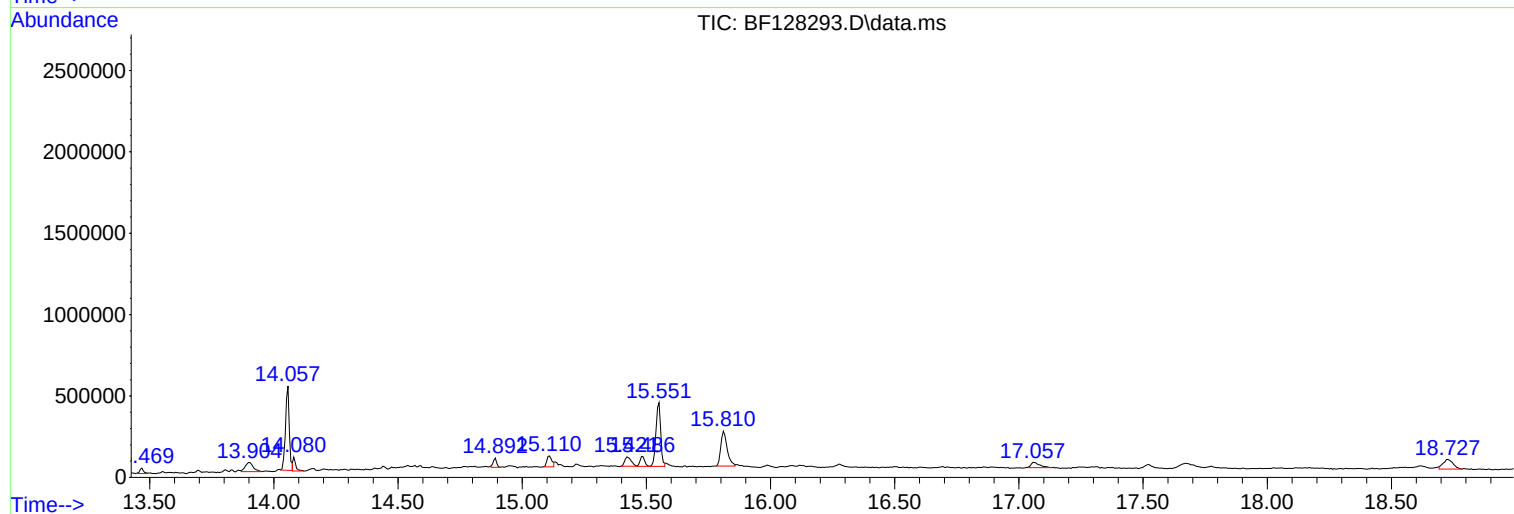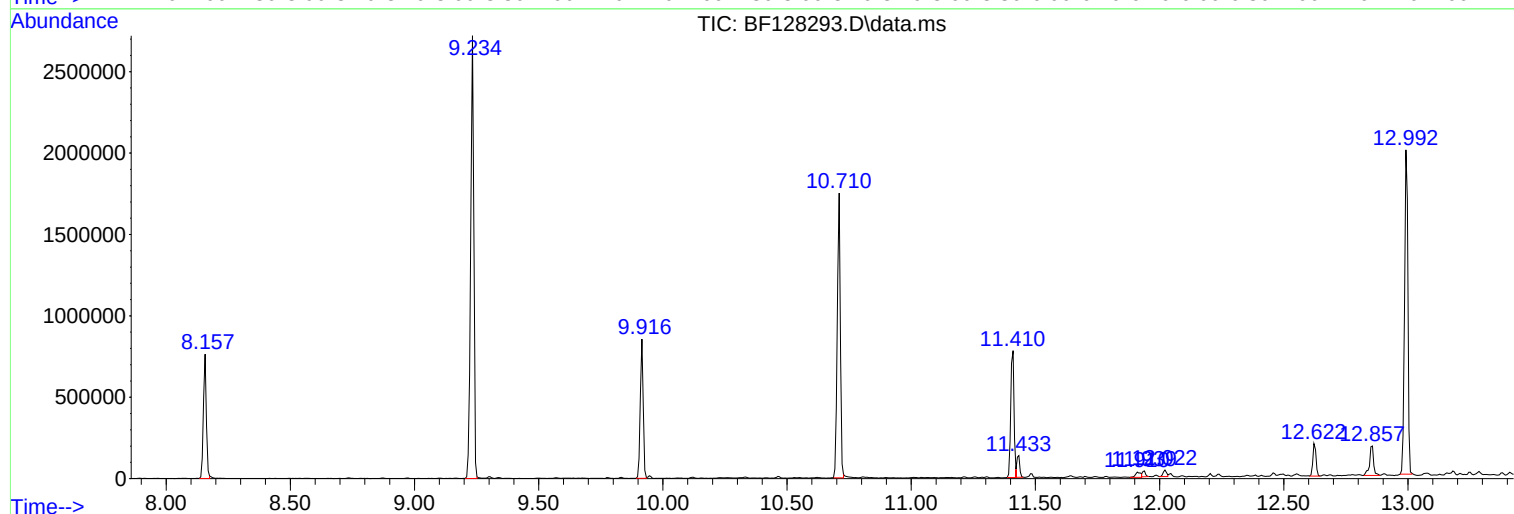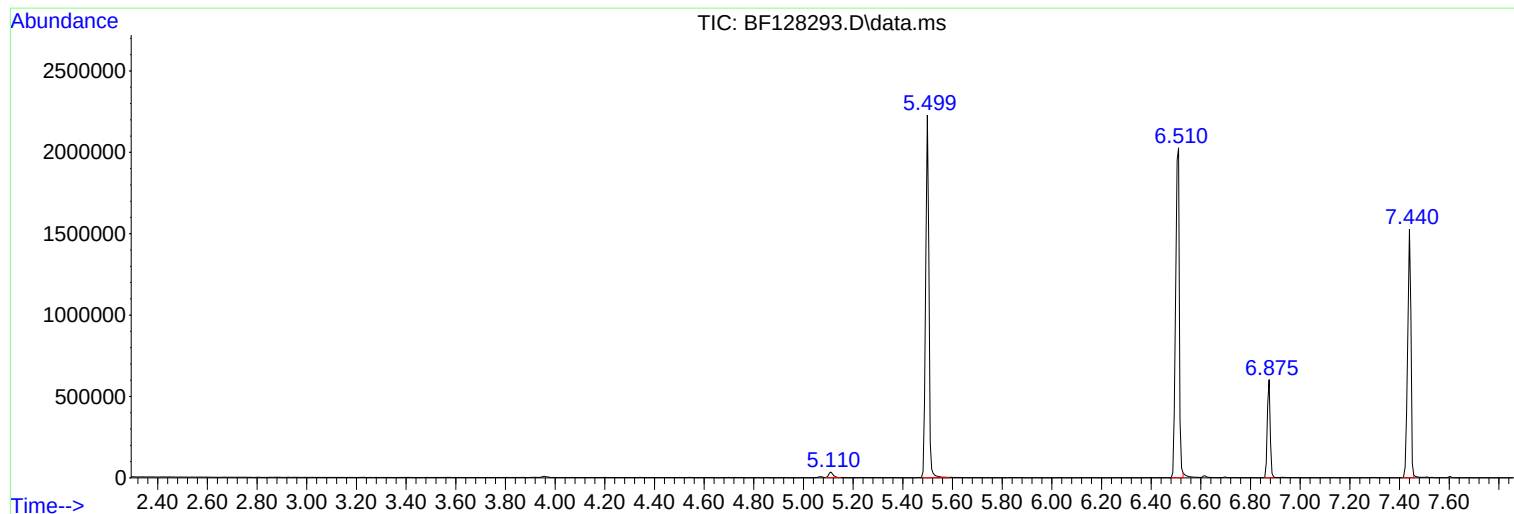

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF051722\
Data File : BF128293.D
Acq On : 17 May 2022 16:14
Operator : CG\JU
Sample : N2881-02
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
SLP-1

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF050922.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF051722\
Data File : BF128293.D
Acq On : 17 May 2022 16:14
Operator : CG\JU
Sample : N2881-02
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
SLP-1

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF050922.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------