

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF051722\
 Data File : BF128294.D
 Acq On : 17 May 2022 16:43
 Operator : CG\JU
 Sample : N2879-04
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 TP2-0516

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF050922.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF128294.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.110	476	480	490	rVB	19066	26438	1.16%	0.170%
2	5.499	542	546	549	rBV	2245722	2037665	89.29%	13.066%
3	6.510	713	718	721	rBV	2033212	2086494	91.43%	13.380%
4	6.875	776	780	783	rBV	595370	476961	20.90%	3.058%
5	7.440	871	876	879	rBV	1465399	1391391	60.97%	8.922%
6	8.157	994	998	1001	rBV	744931	613473	26.88%	3.934%
7	9.234	1176	1181	1184	rBV	2707823	2282095	100.00%	14.634%
8	9.916	1293	1297	1300	rVB	832512	670820	29.39%	4.302%
9	10.710	1427	1432	1435	rBV	1678543	1470345	64.43%	9.429%
10	11.410	1547	1551	1553	rBV	748657	681053	29.84%	4.367%
11	11.433	1553	1555	1559	rVV	148558	119130	5.22%	0.764%
12	11.481	1559	1563	1566	rVV	27511	33594	1.47%	0.215%
13	11.922	1633	1638	1639	rBV2	31660	40292	1.77%	0.258%
14	12.022	1651	1655	1657	rBV2	32313	33918	1.49%	0.217%
15	12.622	1754	1757	1761	rBV	180870	158319	6.94%	1.015%
16	12.857	1790	1797	1800	rBV	163337	182921	8.02%	1.173%
17	12.992	1816	1820	1824	rBV	1992974	1783103	78.13%	11.434%
18	13.898	1969	1974	1984	rVB4	84504	187227	8.20%	1.201%
19	14.057	1996	2001	2004	rBV2	522596	522790	22.91%	3.352%
20	14.080	2004	2005	2013	rVB	69242	52861	2.32%	0.339%
21	15.110	2176	2180	2186	rBV	63143	112700	4.94%	0.723%
22	15.421	2229	2233	2240	rVB	35253	51013	2.24%	0.327%
23	15.486	2240	2244	2249	rBV	53558	67088	2.94%	0.430%
24	15.551	2250	2255	2259	rBV	385076	484817	21.24%	3.109%
25	15.986	2326	2329	2334	rVB4	20322	28143	1.23%	0.180%




Sum of corrected areas: 15594651

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF051722\
Data File : BF128294.D
Acq On : 17 May 2022 16:43
Operator : CG\JU
Sample : N2879-04
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
TP2-0516

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF050922.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

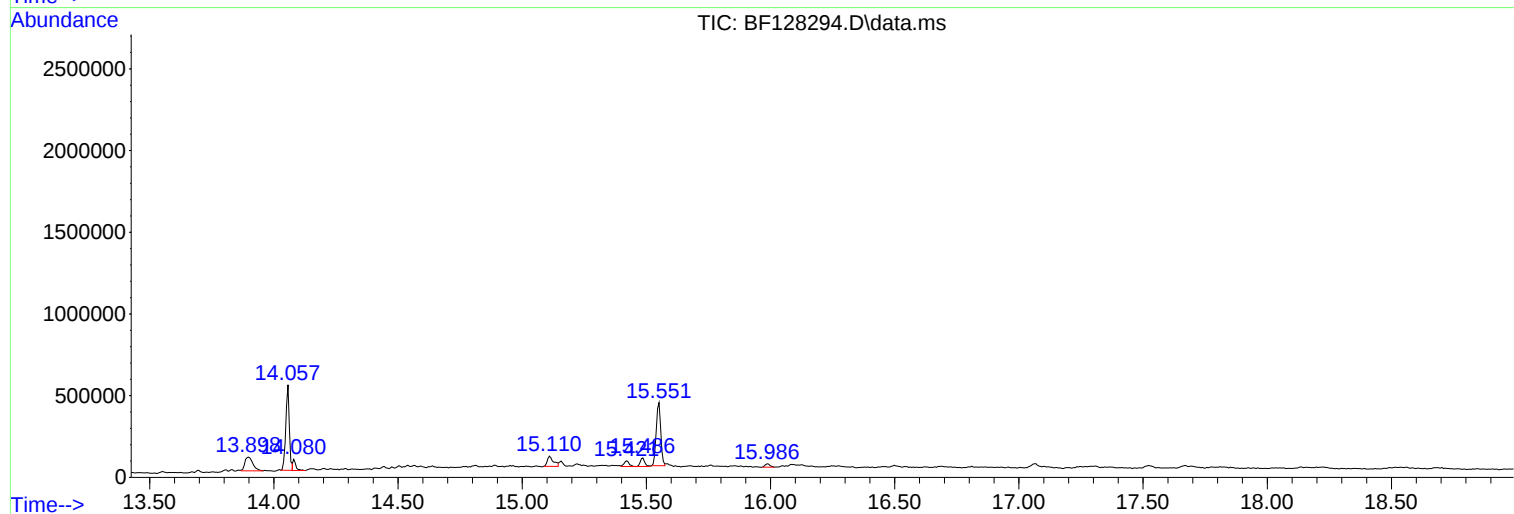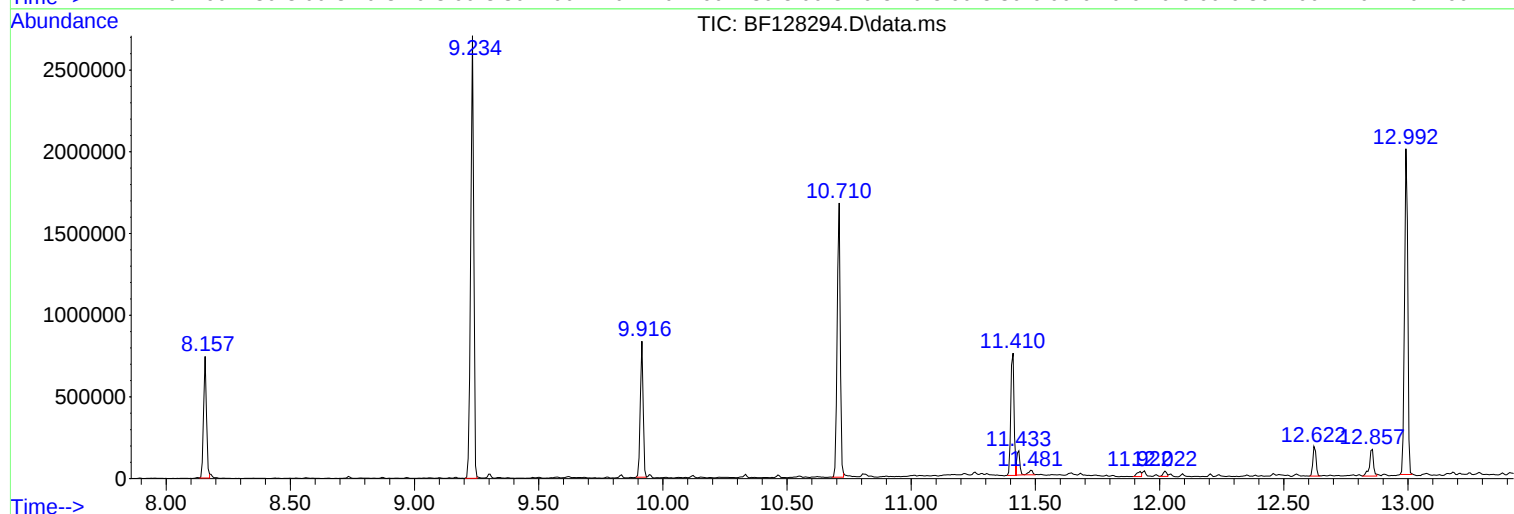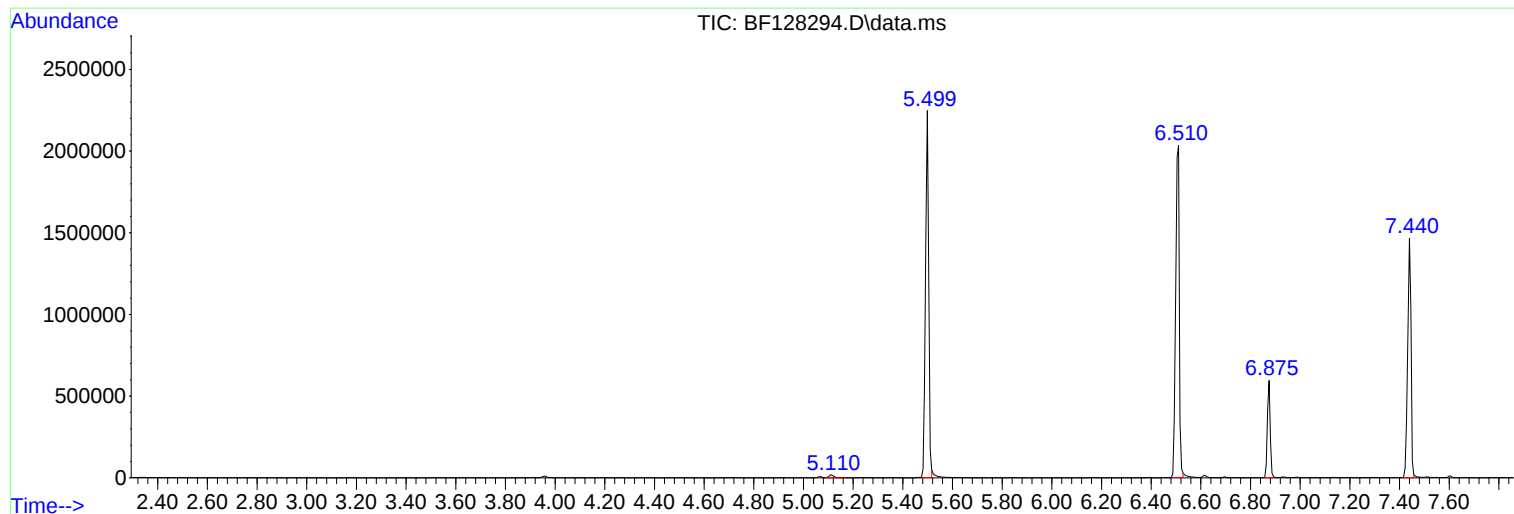

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF051722\
Data File : BF128294.D
Acq On : 17 May 2022 16:43
Operator : CG\JU
Sample : N2879-04
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
TP2-0516

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF050922.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF051722\
Data File : BF128294.D
Acq On : 17 May 2022 16:43
Operator : CG\JU
Sample : N2879-04
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
TP2-0516

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF050922.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------