

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF051722\
 Data File : BF128295.D
 Acq On : 17 May 2022 17:13
 Operator : CG\JU
 Sample : N2879-07
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 TP-3-0516

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF050922.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF128295.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.940	277	281	288	rVB2	11689	16129	1.37%	0.165%
2	5.493	541	545	555	rVB	1150472	1046515	88.71%	10.684%
3	6.504	713	717	733	rBV	1232935	1094382	92.76%	11.173%
4	6.875	776	780	783	rBV	578618	475057	40.27%	4.850%
5	7.440	872	876	879	rBV	797114	704725	59.73%	7.195%
6	8.157	994	998	1001	rBV	764385	611915	51.87%	6.247%
7	9.234	1176	1181	1184	rBV	1263110	1179766	100.00%	12.045%
8	9.916	1293	1297	1300	rBV	843819	672288	56.98%	6.864%
9	9.945	1300	1302	1306	rVB2	14394	12100	1.03%	0.124%
10	10.704	1428	1431	1441	rBV	867016	773867	65.59%	7.901%
11	10.804	1445	1448	1458	rVB6	9284	18754	1.59%	0.191%
12	11.257	1521	1525	1528	rBV5	9321	12948	1.10%	0.132%
13	11.410	1547	1551	1553	rBV	754271	672726	57.02%	6.868%
14	11.427	1553	1554	1559	rVV	97234	78305	6.64%	0.799%
15	11.480	1559	1563	1566	rVV	17692	17859	1.51%	0.182%
16	11.645	1586	1591	1594	rBV3	8397	16023	1.36%	0.164%
17	11.910	1633	1636	1639	rBV2	12506	15842	1.34%	0.162%
18	11.939	1639	1641	1646	rVB2	18751	16452	1.39%	0.168%
19	12.022	1652	1655	1657	rBV2	20869	20550	1.74%	0.210%
20	12.351	1706	1711	1713	rBV6	14722	20533	1.74%	0.210%
21	12.480	1731	1733	1741	rVB9	12004	18547	1.57%	0.189%
22	12.551	1742	1745	1749	rBV5	8907	13179	1.12%	0.135%
23	12.622	1754	1757	1761	rBV	105640	94708	8.03%	0.967%
24	12.857	1790	1797	1802	rBV	89720	119621	10.14%	1.221%
25	12.992	1816	1820	1823	rBV	1116185	921875	78.14%	9.412%
26	13.127	1840	1843	1845	rBV	22873	15716	1.33%	0.160%
27	13.904	1969	1975	1985	rVB6	26659	66342	5.62%	0.677%
28	14.057	1996	2001	2004	rBV	536607	519585	44.04%	5.305%
29	14.080	2004	2005	2010	rVB	45011	32161	2.73%	0.328%
30	15.110	2177	2180	2183	rBV2	27049	37125	3.15%	0.379%
31	15.551	2250	2255	2259	rBV	391668	479448	40.64%	4.895%




Sum of corrected areas: 9795043

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF051722\
Data File : BF128295.D
Acq On : 17 May 2022 17:13
Operator : CG\JU
Sample : N2879-07
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
TP-3-0516

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF050922.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

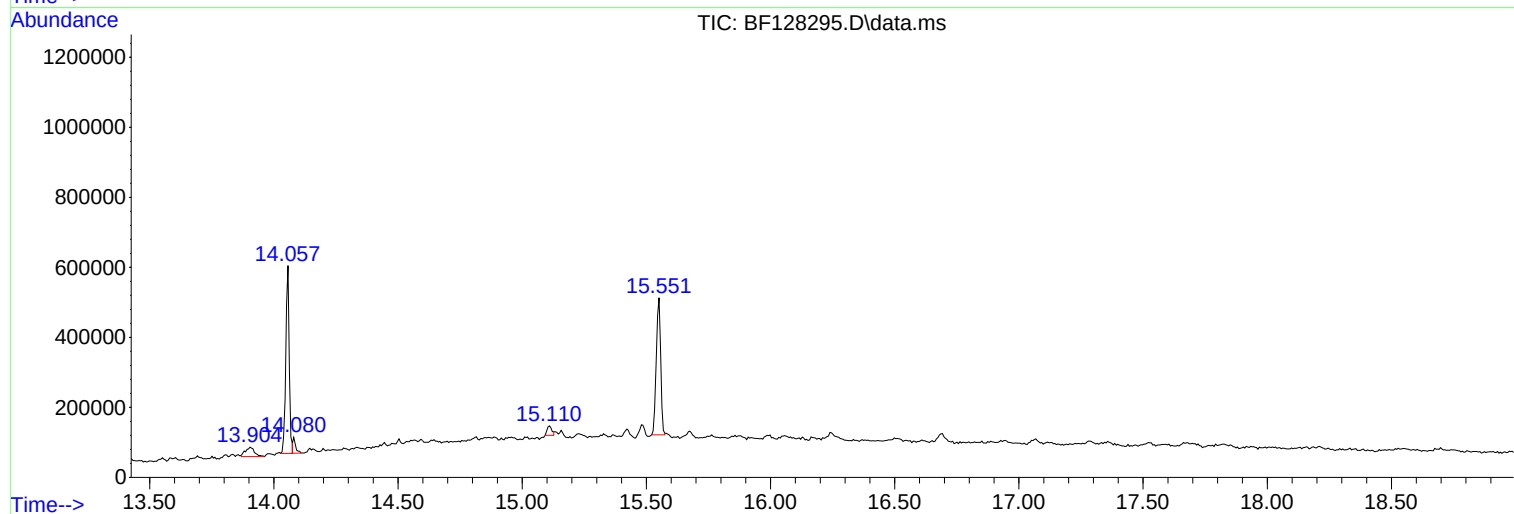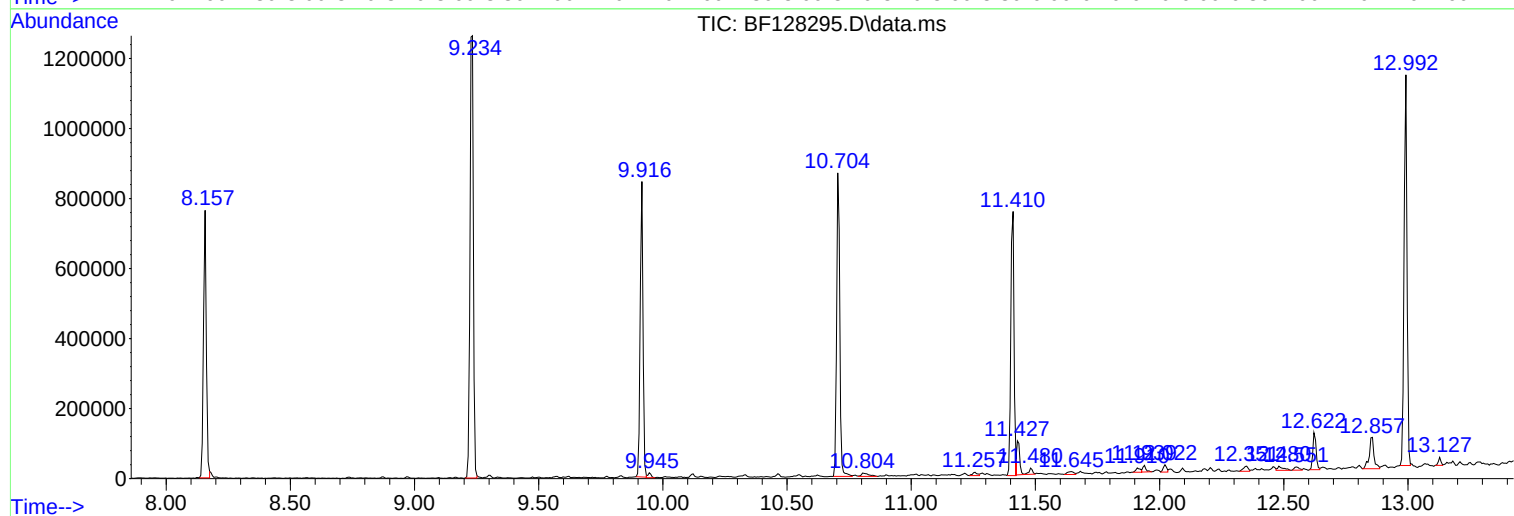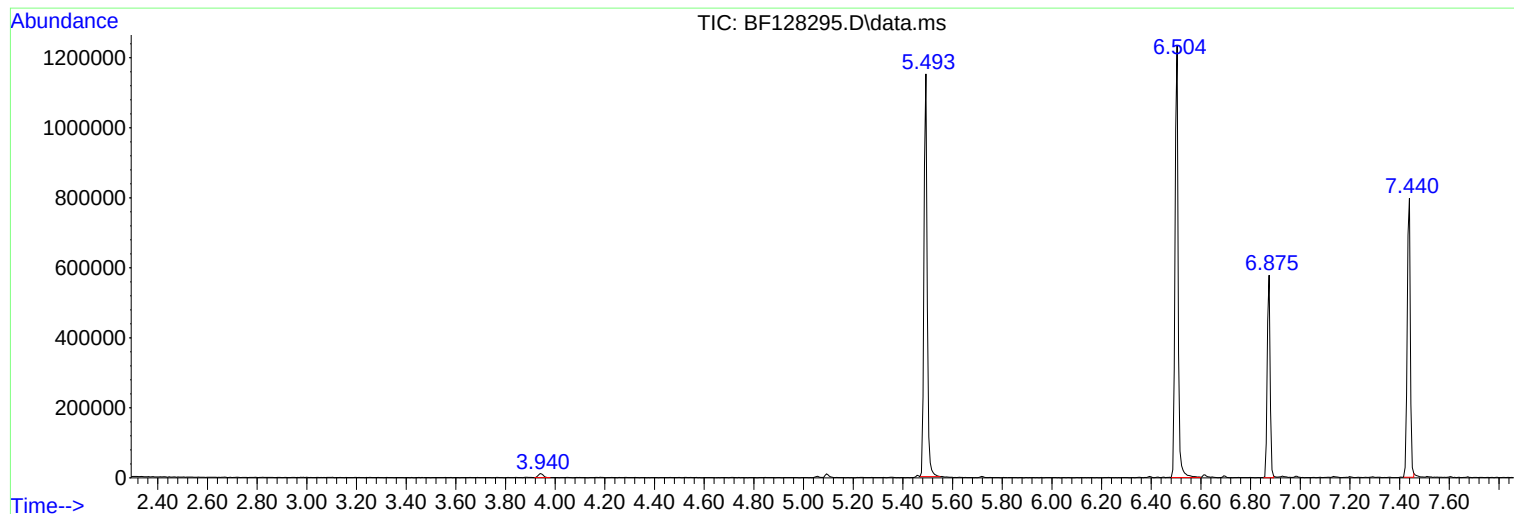

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF051722\
Data File : BF128295.D
Acq On : 17 May 2022 17:13
Operator : CG\JU
Sample : N2879-07
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
TP-3-0516










Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF050922.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Cyclopentadecane Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
13.904	2.55 ng	66342	Chrysene-d12	14.057

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Cyclopentadecane	210	C15H30	000295-48-7	64
2			1-Dodecanethiol	202	C12H26S	000112-55-0	38
3			Pentafluoropropionic acid, penta...	374	C18H31F5O2	959092-08-1	25
4			Fumaric acid, 2,2-dichloroethyl ...	394	C19H32Cl2O4	1000348-58-1	25
5			Trifluoroacetic acid, pentadecyl...	324	C17H31F3O2	959010-23-2	22

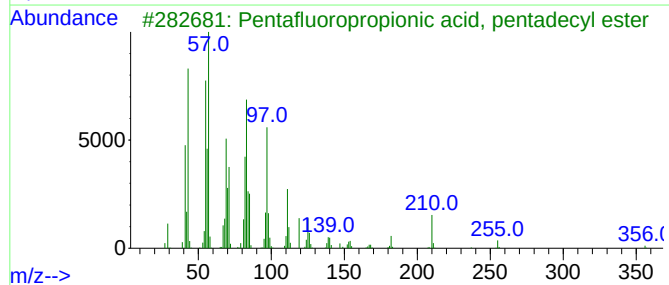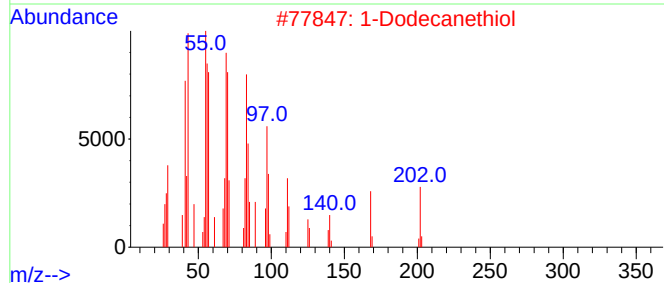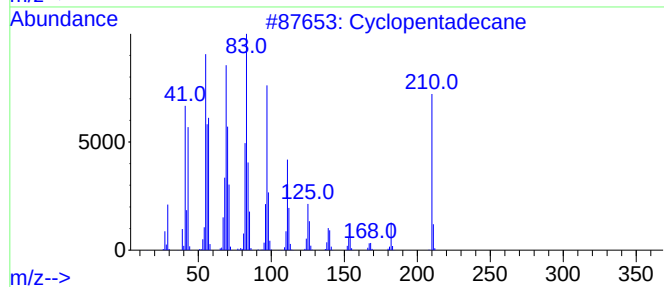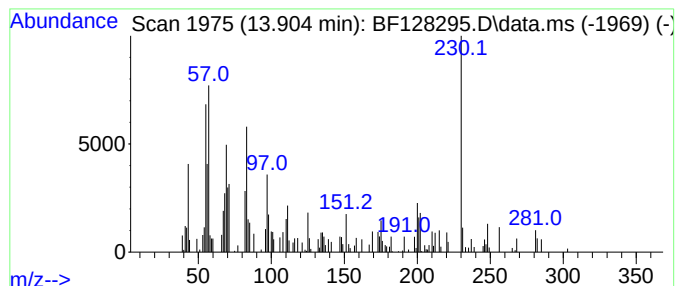

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF051722\
Data File : BF128295.D
Acq On : 17 May 2022 17:13
Operator : CG\JU
Sample : N2879-07
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
TP-3-0516

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF050922.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Cyclopentadecane	13.904	2.5	ng	66342	5	14.057	519585	20.0