

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF051722\
 Data File : BF128304.D
 Acq On : 17 May 2022 21:38
 Operator : CG\JU
 Sample : N2863-06 10X
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 P003-SS004-0006-01

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF050922.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF128304.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.940	277	281	288	rVB	7029	8409	1.36%	0.213%
2	5.498	542	546	556	rBV	94367	105722	17.13%	2.674%
3	6.510	715	718	729	rBV	99706	108733	17.62%	2.750%
4	6.875	776	780	789	rBV	654684	524099	84.94%	13.255%
5	7.287	846	850	858	rBV	22472	27036	4.38%	0.684%
6	7.440	872	876	881	rBV	69978	63772	10.34%	1.613%
7	8.157	994	998	1002	rBV	721239	617043	100.00%	15.606%
8	9.234	1177	1181	1188	rBV	141716	118050	19.13%	2.986%
9	9.916	1293	1297	1301	rBV	749738	609852	98.83%	15.424%
10	10.669	1422	1425	1428	rBV	7954	8112	1.31%	0.205%
11	10.710	1428	1432	1440	rVB	63947	58799	9.53%	1.487%
12	11.410	1547	1551	1554	rBV	719778	593049	96.11%	14.999%
13	12.951	1810	1813	1816	rBV5	8300	10506	1.70%	0.266%
14	12.992	1816	1820	1823	rVV	144591	121060	19.62%	3.062%
15	14.021	1992	1995	1997	rBV	29606	27308	4.43%	0.691%
16	14.057	1997	2001	2005	rBV	665649	573004	92.86%	14.492%
17	15.551	2251	2255	2262	rVB	295860	379356	61.48%	9.594%


Sum of corrected areas: 3953910

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF051722\
Data File : BF128304.D
Acq On : 17 May 2022 21:38
Operator : CG\JU
Sample : N2863-06 10X
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
P003-SS004-0006-01

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF050922.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

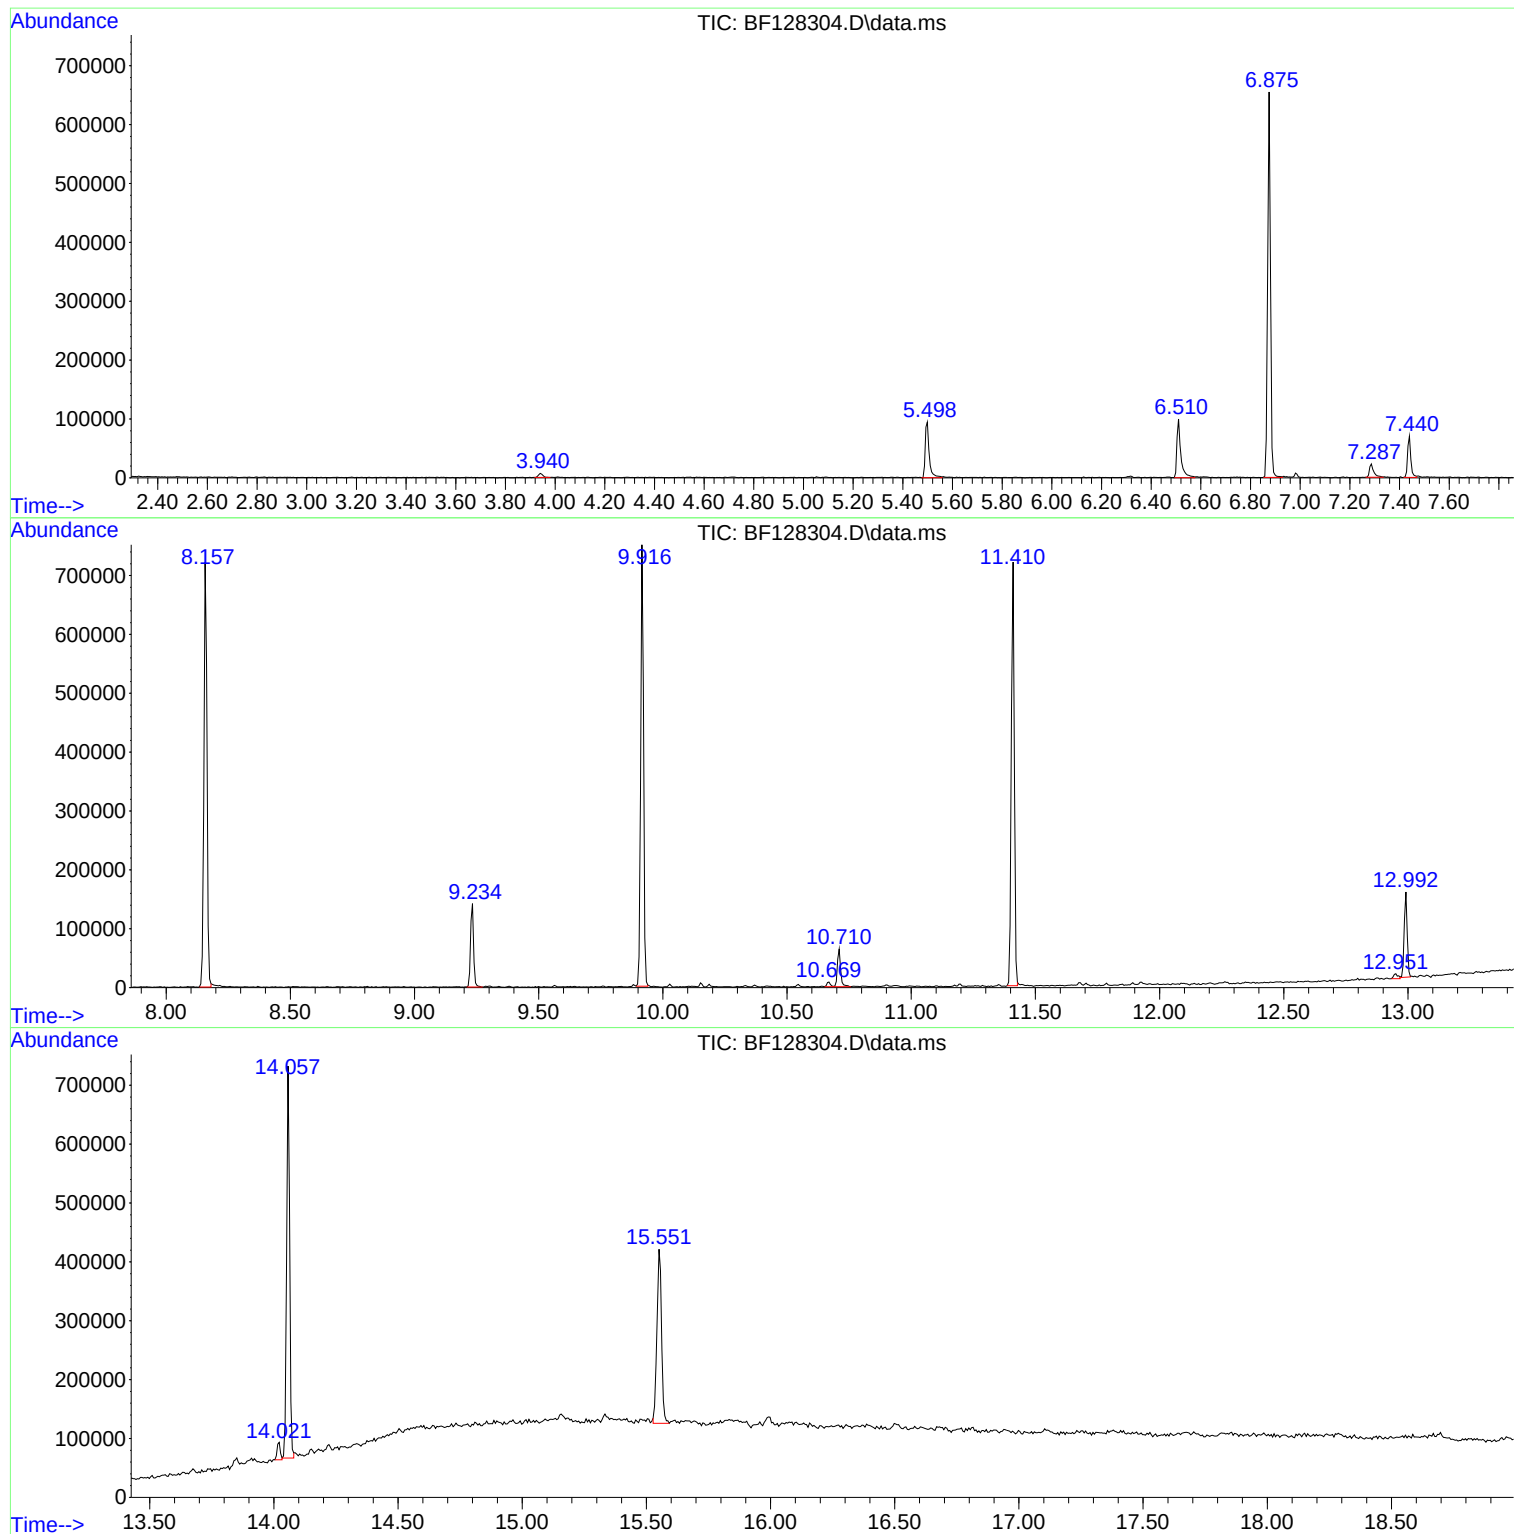

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF051722\
Data File : BF128304.D
Acq On : 17 May 2022 21:38
Operator : CG\JU
Sample : N2863-06 10X
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
P003-SS004-0006-01

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF050922.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF051722\
Data File : BF128304.D
Acq On : 17 May 2022 21:38
Operator : CG\JU
Sample : N2863-06 10X
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
P003-SS004-0006-01

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF050922.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------