
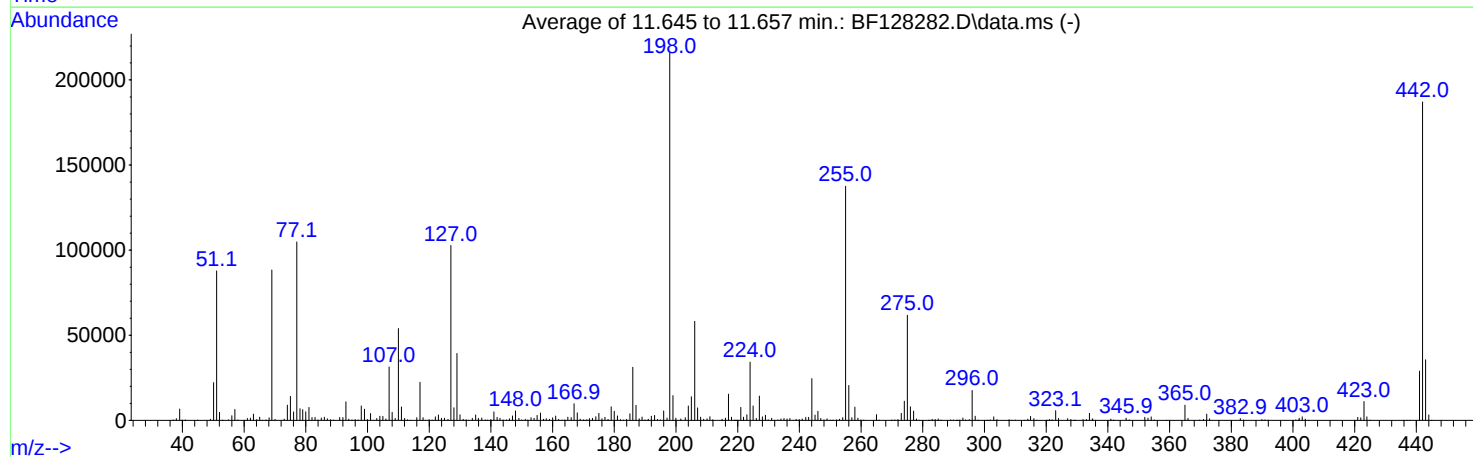


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF051722\
 Data File : BF128282.D
 Acq On : 17 May 2022 10:37
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF050922.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu May 19 06:47:51 2022

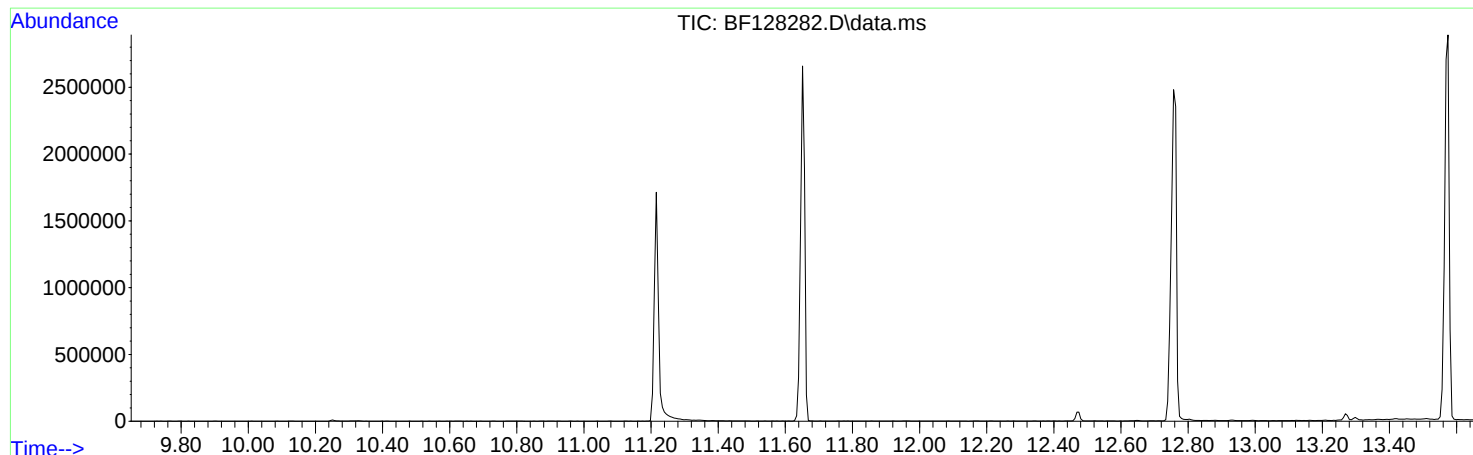




AutoFind: Scans 1591, 1592, 1593; Background Corrected with Scan 1585

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	40.6	87805	PASS
68	69	0.00	2	1.7	1545	PASS
69	198	0.00	100	40.9	88344	PASS
70	69	0.00	2	0.7	604	PASS
127	198	10	80	47.5	102760	PASS
197	198	0.00	2	0.6	1395	PASS
198	198	100	100	100.0	216128	PASS
199	198	5	9	6.7	14542	PASS
275	198	10	60	28.6	61768	PASS
365	198	1	100	4.1	8951	PASS
441	198	0.01	100	13.4	28999	PASS
442	442	50	100	100.0	187099	PASS
443	442	15	24	19.0	35619	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF051722\
 Data File : BF128282.D
 Acq On : 17 May 2022 10:37
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Quant Time: May 18 04:23:09 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF050922.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed May 18 01:31:11 2022
 Response via : Initial Calibration

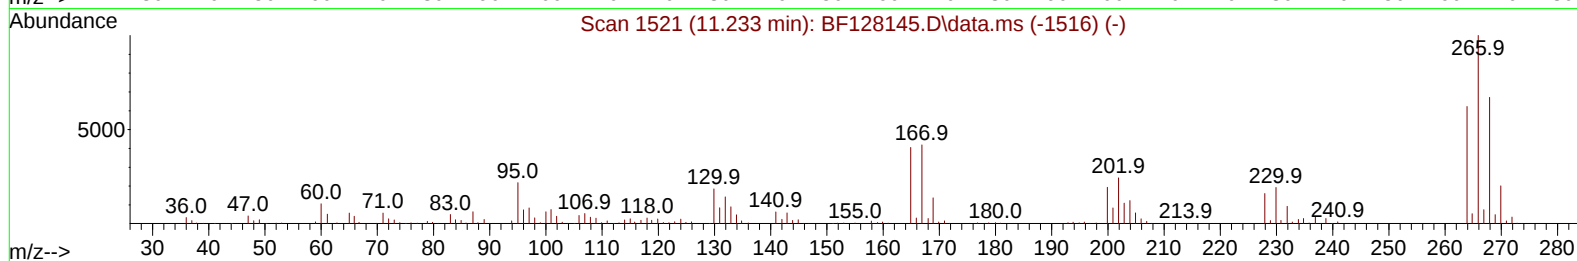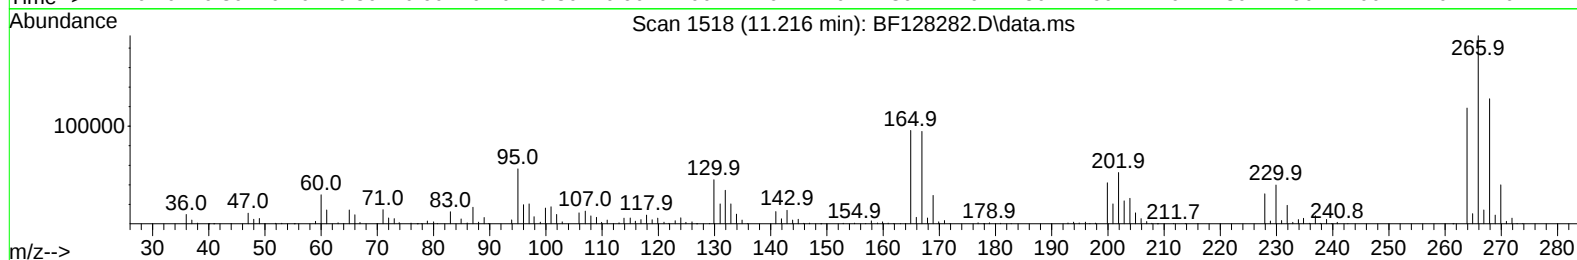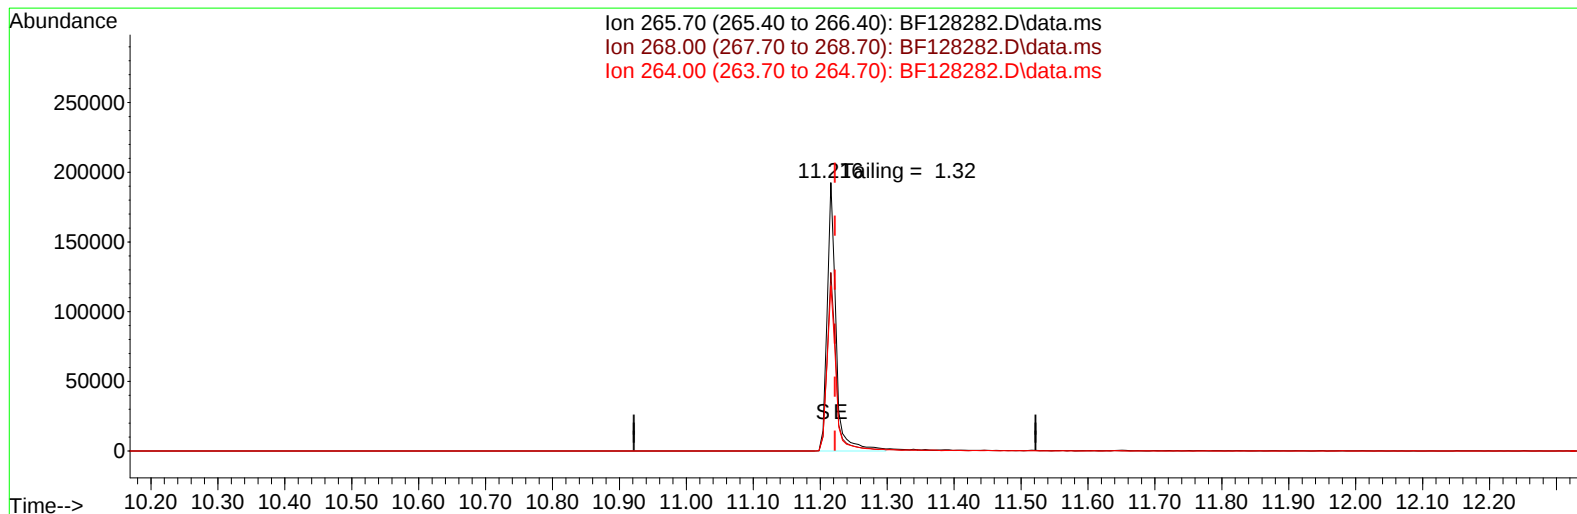

TIC: BF128282.D\data.ms

(70) Pentachlorophenol (C)

11.216min (-0.006) 545717.28 ng




response 180783

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	66.30	66.46
264.00	66.40	61.54
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF051722\
 Data File : BF128282.D
 Acq On : 17 May 2022 10:37
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Quant Time: May 18 04:23:09 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF050922.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed May 18 01:31:11 2022
 Response via : Initial Calibration

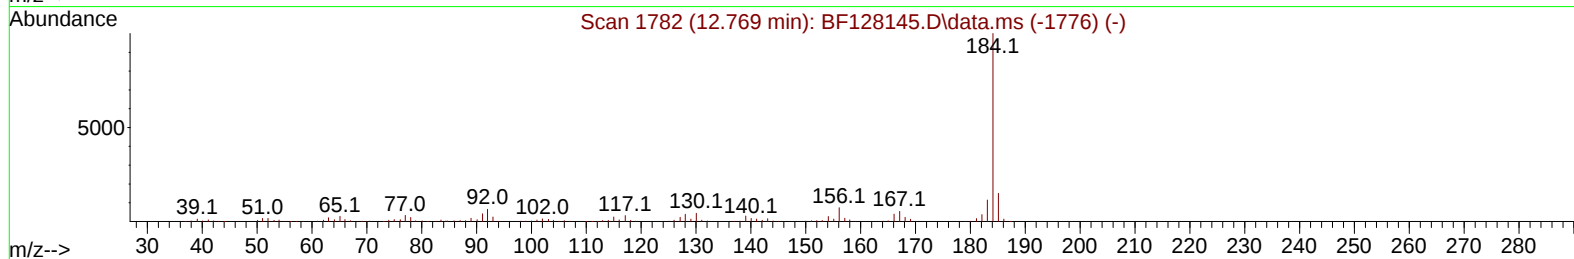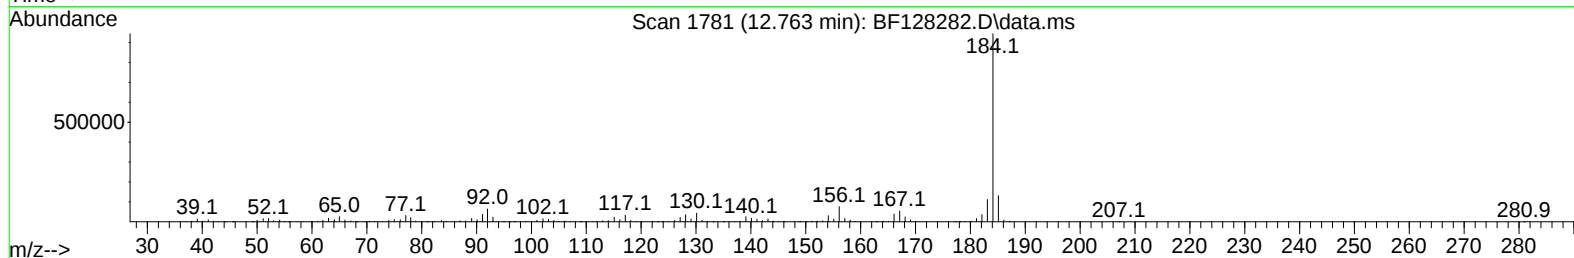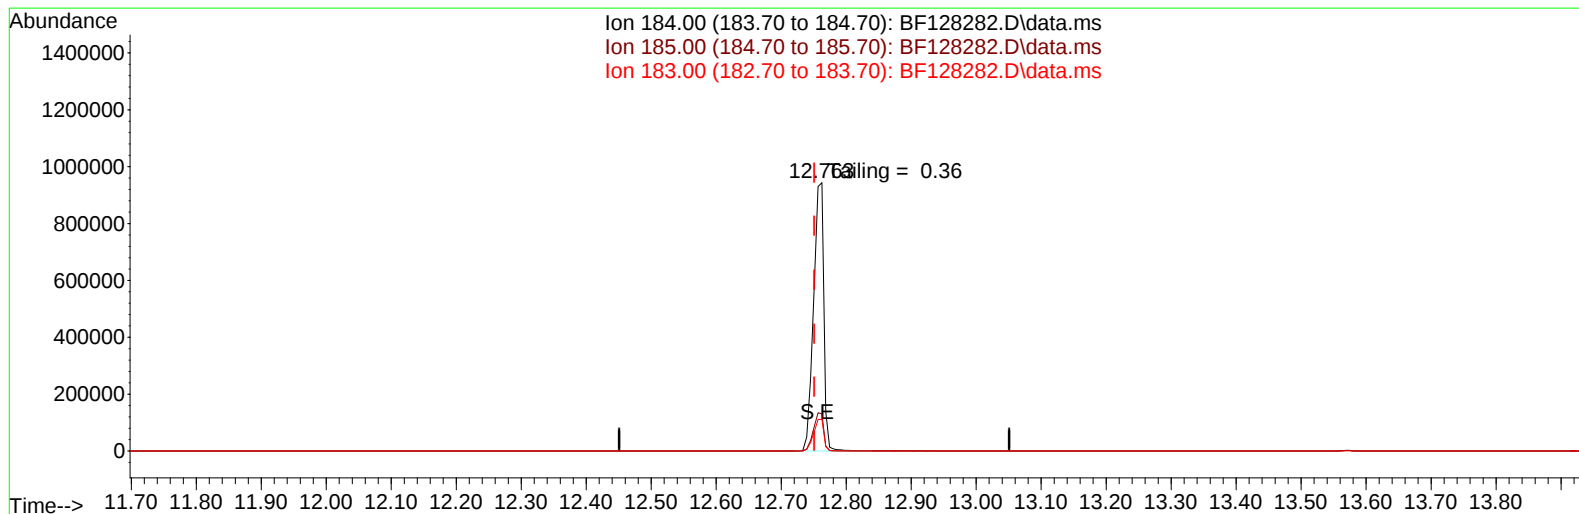

TIC: BF128282.D\data.ms

(77) Benzidine

12.763min (+ 0.012) 106474.37 ng

response 1046949

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.10	13.86
183.00	11.20	11.83
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
5/17/2022	BNA_F	<u>BF128282.D</u>
Compound Name	Response	Retention Time
DDT	516651	13.574
DDD	11952	13.269
DDE	920	12.927
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
12872	529523	2.43

Instrument :
BNA_F
ClientSampleId :
DFTPP