
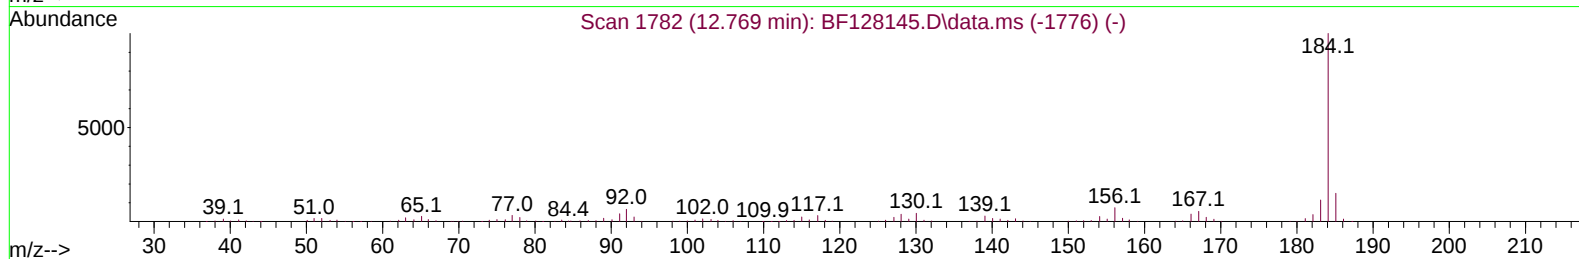
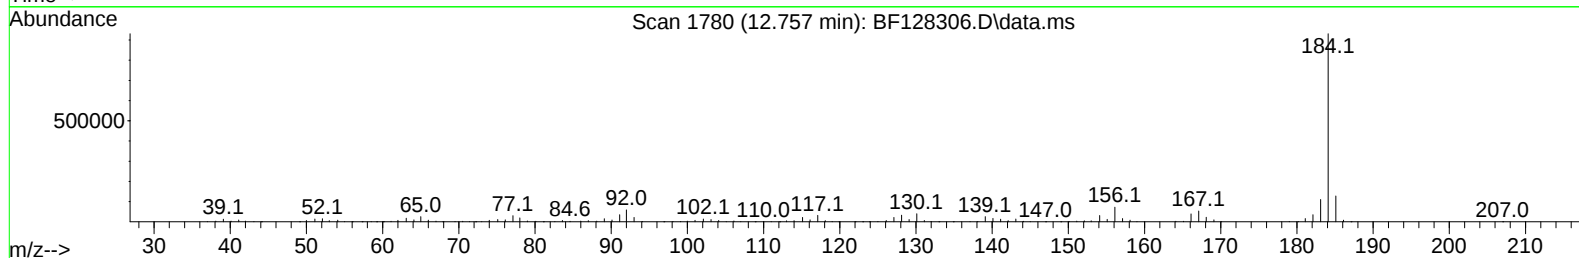


Data Path : Z:\svoasrv\HPCHEM1\BNA\_F\Data\BF051822\  
Data File : BF128306.D  
Acq On : 18 May 2022 12:02  
Operator : CG\JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 18 16:57:03 2022  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_F\Methods\8270-BF050922.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Wed May 18 01:31:11 2022  
Response via : Initial Calibration

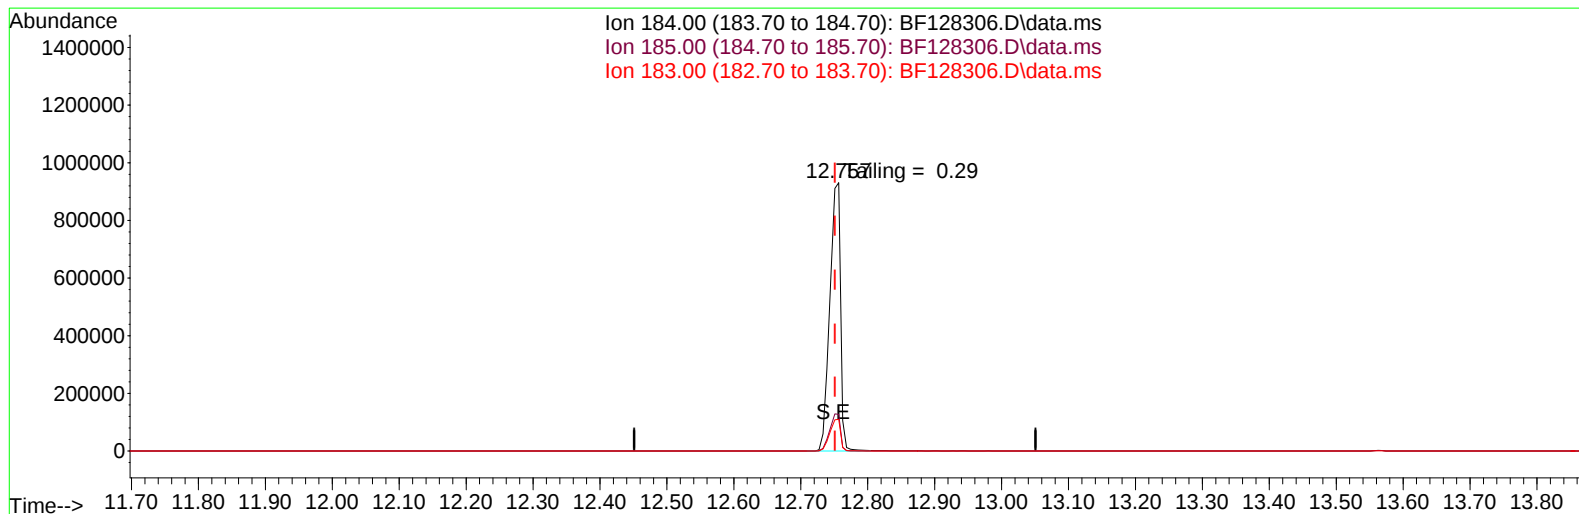

TIC: BF128306.D\data.ms

**(77) Benzidine**

12.757min (+ 0.006) 0.00 ng

response 1039349

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 184.00 | 100.00 | 100.00 |
| 185.00 | 15.10  | 13.69  |
| 183.00 | 11.20  | 11.84  |
| 0.00   | 0.00   | 0.00   |