
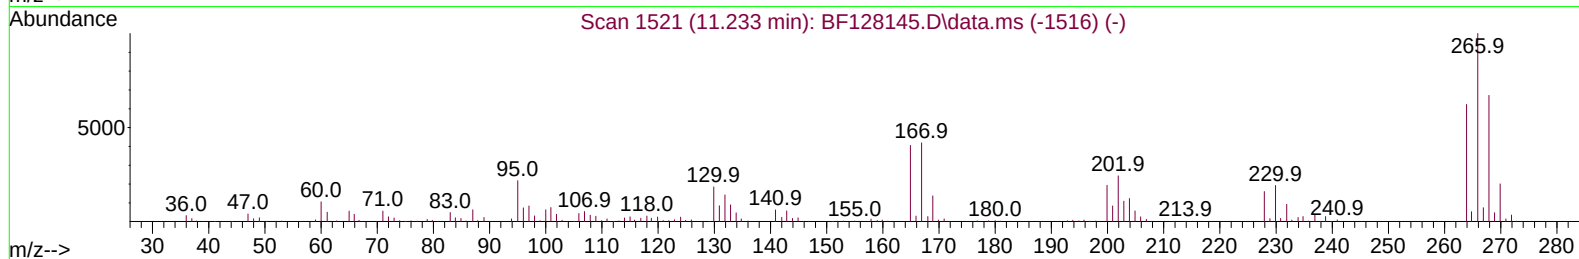
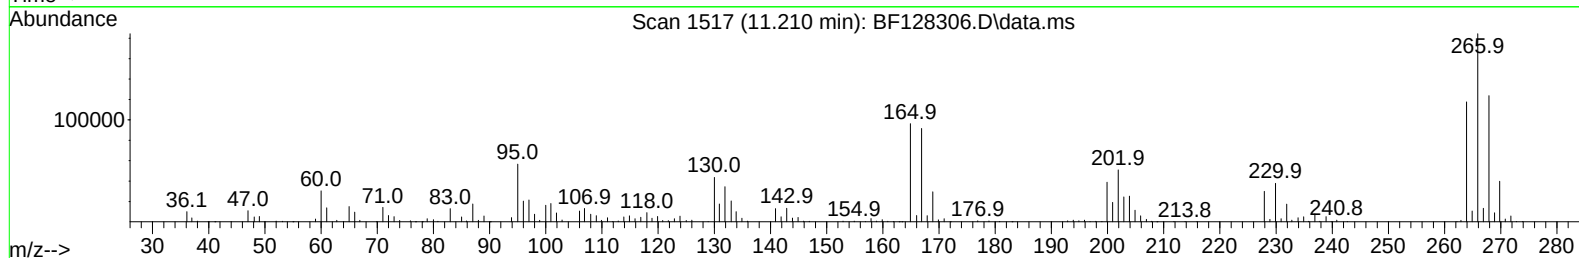


Data Path : Z:\svoasrv\HPCHEM1\BNA\_F\Data\BF051822\  
Data File : BF128306.D  
Acq On : 18 May 2022 12:02  
Operator : CG\JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 18 16:57:03 2022  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_F\Methods\8270-BF050922.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Wed May 18 01:31:11 2022  
Response via : Initial Calibration

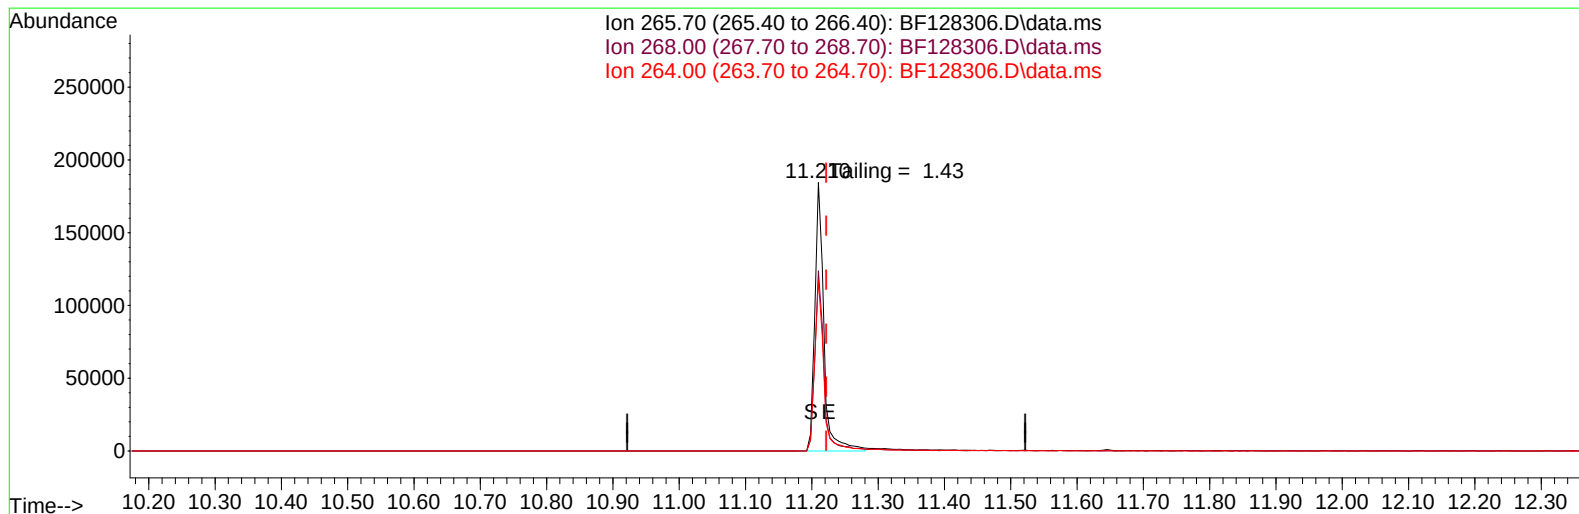

TIC: BF128306.D\data.ms

**(70) Pentachlorophenol (C)**

11.210min (-0.012) 33591.93 ng

response 181121

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 265.70 | 100.00 | 100.00 |
| 268.00 | 66.30  | 67.13  |
| 264.00 | 66.40  | 63.80  |
| 0.00   | 0.00   | 0.00   |