
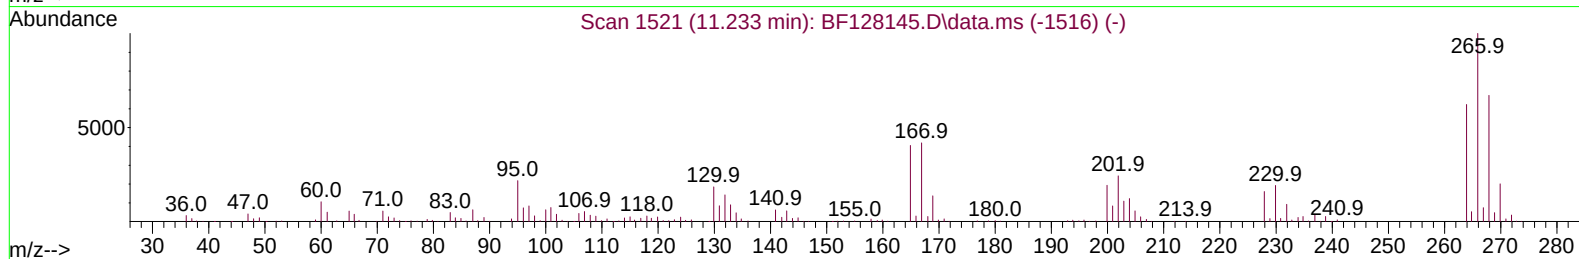
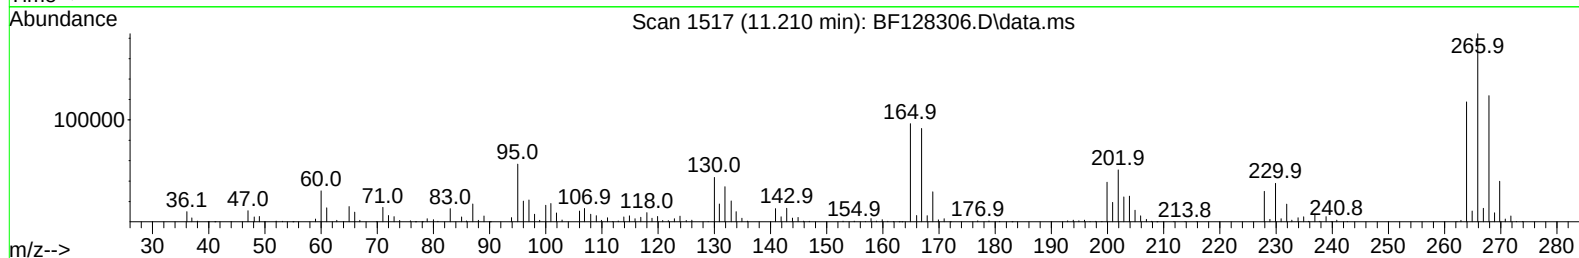


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF051822\
Data File : BF128306.D
Acq On : 18 May 2022 12:02
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 18 16:57:03 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF050922.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed May 18 01:31:11 2022
Response via : Initial Calibration

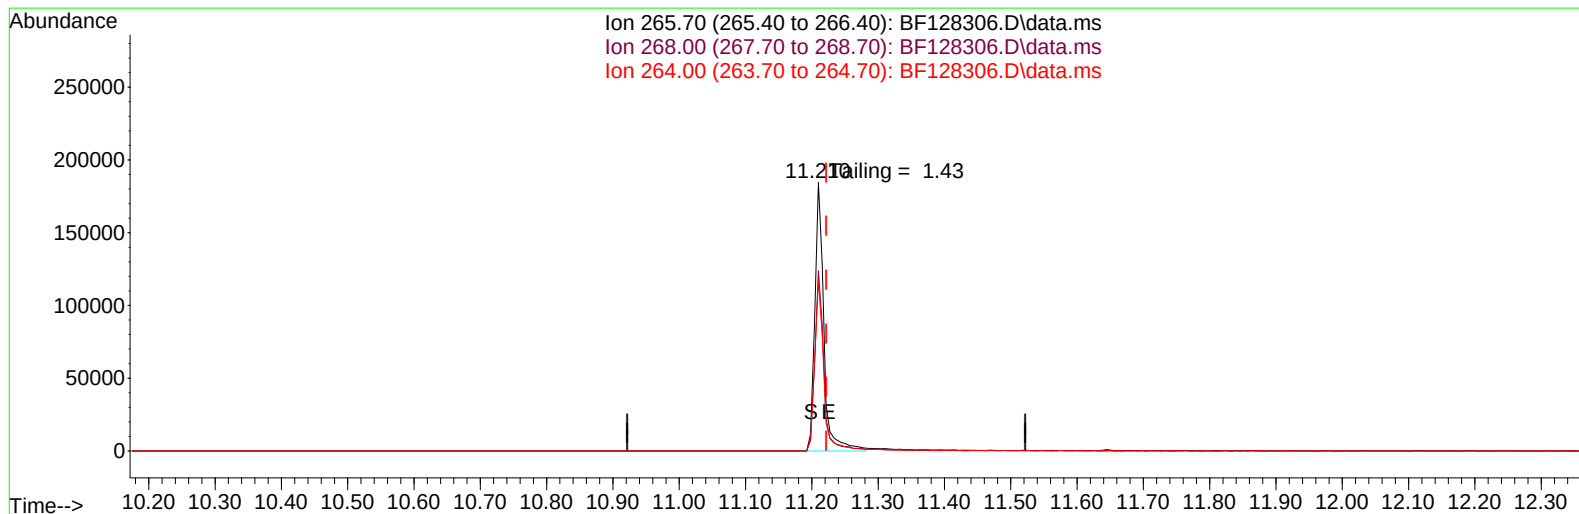




TIC: BF128306.D\data.ms

(70) Pentachlorophenol (C)**11.210min (-0.012) 33591.93 ng****response 181121**

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	66.30	67.13
264.00	66.40	63.80
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF051822\
Data File : BF128306.D
Acq On : 18 May 2022 12:02
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 18 16:57:03 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF050922.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed May 18 01:31:11 2022
Response via : Initial Calibration

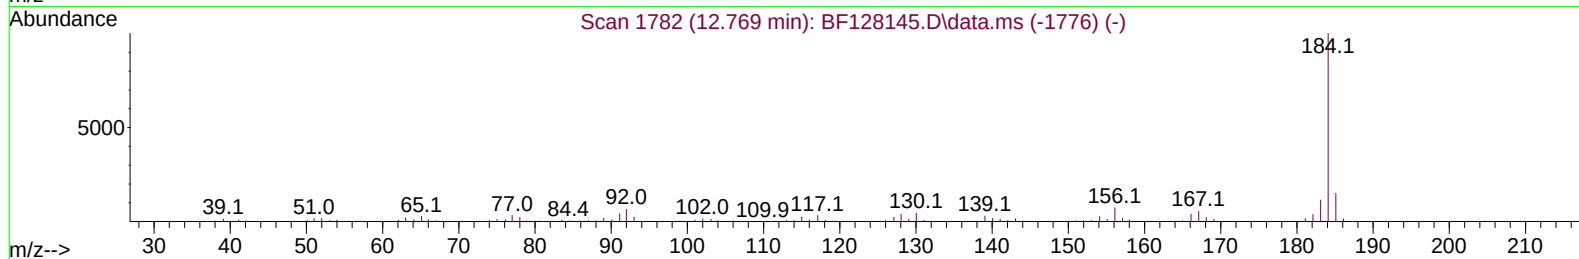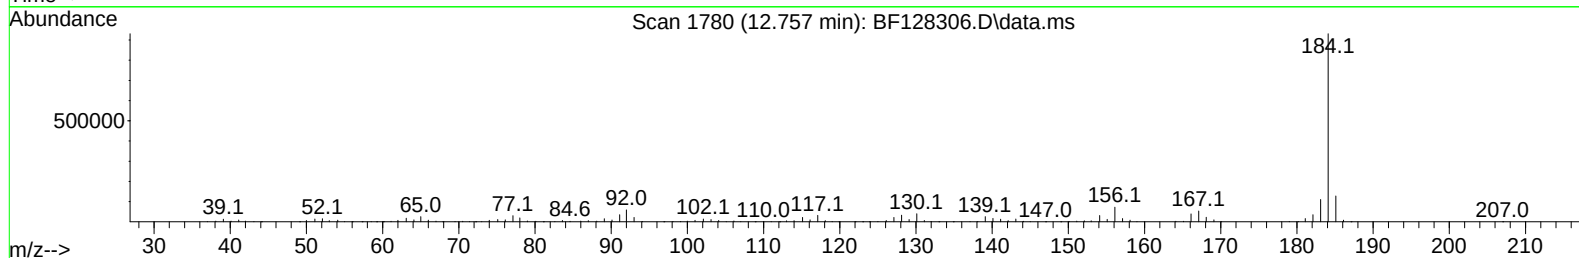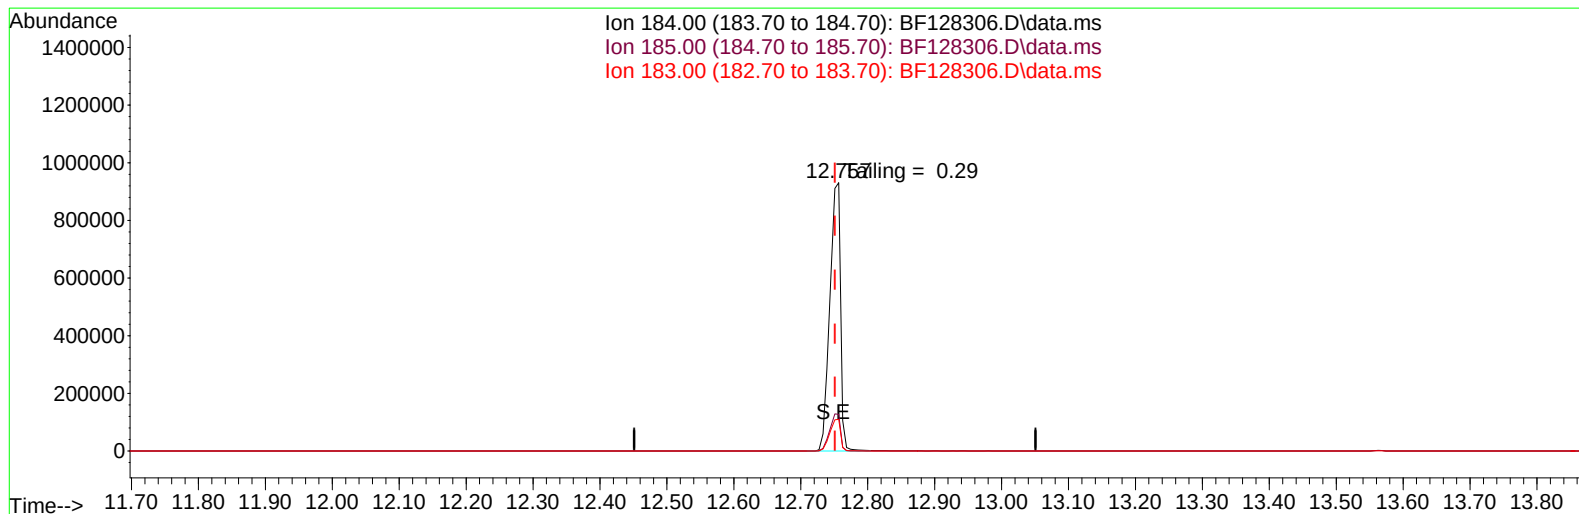

TIC: BF128306.D\data.ms

(77) Benzidine

12.757min (+ 0.006) 0.00 ng

response 1039349

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.10	13.69
183.00	11.20	11.84
0.00	0.00	0.00