

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF051822\
 Data File : BF128313.D
 Acq On : 18 May 2022 16:00
 Operator : CG\JU
 Sample : N2776-05
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 CF-280MER-9-5

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF050922.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF128313.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.493	541	545	557	rBV	1122654	1032598	37.16%	7.117%
2	6.498	713	716	734	rBV	752285	659084	23.72%	4.543%
3	6.869	775	779	786	rBV	674906	532139	19.15%	3.668%
4	7.439	870	876	879	rBV	1628885	1650384	59.39%	11.375%
5	8.151	993	997	1001	rBV	810494	683858	24.61%	4.713%
6	9.228	1175	1180	1183	rBV	3046727	2778718	100.00%	19.152%
7	9.622	1241	1247	1251	rBV	40912	34956	1.26%	0.241%
8	9.910	1292	1296	1299	rBV	956876	785762	28.28%	5.416%
9	10.010	1309	1313	1316	rBV	37464	33879	1.22%	0.234%
10	10.704	1427	1431	1434	rBV	1995057	1741928	62.69%	12.006%
11	11.404	1546	1550	1553	rBV	903678	772909	27.82%	5.327%
12	11.774	1610	1613	1618	rVB	40755	31654	1.14%	0.218%
13	12.992	1815	1820	1823	rBV	2825581	2599919	93.57%	17.920%
14	13.892	1967	1973	1980	rBV8	14304	38150	1.37%	0.263%
15	14.051	1996	2000	2003	rBV	645738	588883	21.19%	4.059%
16	14.139	2011	2015	2019	rBV	62797	60352	2.17%	0.416%
17	15.539	2248	2253	2259	rVB	388738	483667	17.41%	3.334%


Sum of corrected areas: 14508840

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF051822\
Data File : BF128313.D
Acq On : 18 May 2022 16:00
Operator : CG\JU
Sample : N2776-05
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
CF-280MER-9-5

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF050922.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

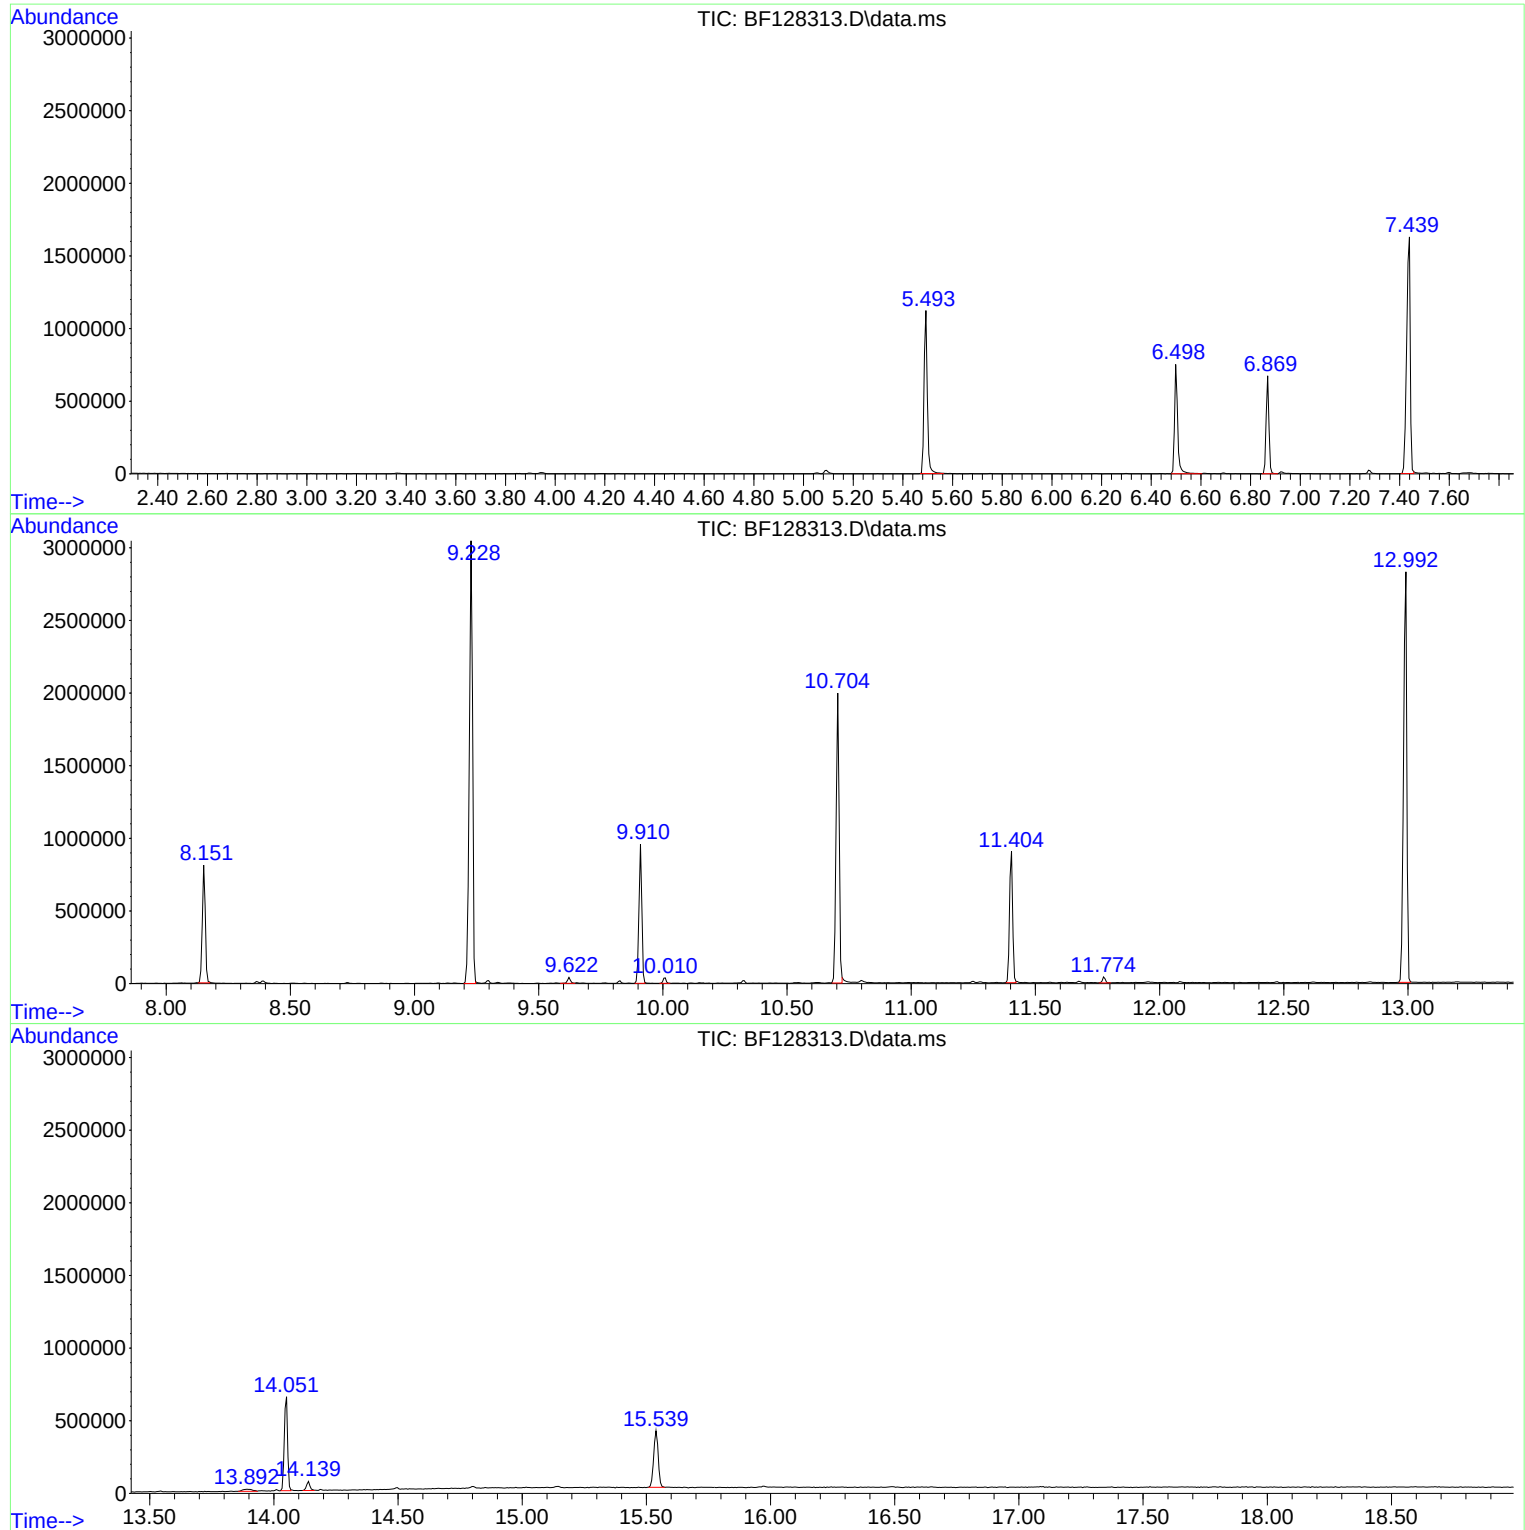

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF051822\
Data File : BF128313.D
Acq On : 18 May 2022 16:00
Operator : CG\JU
Sample : N2776-05
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
CF-280MER-9-5

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF050922.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF051822\
Data File : BF128313.D
Acq On : 18 May 2022 16:00
Operator : CG\JU
Sample : N2776-05
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
CF-280MER-9-5

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF050922.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc