

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF051822\
 Data File : BF128320.D
 Acq On : 18 May 2022 19:26
 Operator : CG\JU
 Sample : N2906-01
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 CDF-1

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF050922.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF128320.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.452	14	28	35	rVB2	18439	42966	1.97%	0.222%
2	3.940	275	281	288	rBV	22757	32594	1.49%	0.169%
3	5.093	473	477	490	rVB	121941	154781	7.08%	0.801%
4	5.493	541	545	561	rVB	1835305	1761905	80.59%	9.121%
5	6.504	712	717	732	rBV	1963909	1911361	87.43%	9.895%
6	6.869	775	779	786	rBV	606854	501743	22.95%	2.597%
7	7.434	871	875	878	rBV	1423207	1277255	58.42%	6.612%
8	8.151	993	997	1000	rBV	797232	662517	30.30%	3.430%
9	9.228	1175	1180	1183	rBV	2649492	2186211	100.00%	11.317%
10	9.292	1186	1191	1195	rVB	38612	33926	1.55%	0.176%
11	9.910	1292	1296	1299	rBV	889463	726573	33.23%	3.761%
12	10.328	1359	1367	1370	rBV4	19859	32680	1.49%	0.169%
13	10.704	1427	1431	1434	rBV	1450553	1326278	60.67%	6.866%
14	10.804	1443	1448	1456	rVB5	21632	46446	2.12%	0.240%
15	11.133	1500	1504	1506	rBV2	24659	28865	1.32%	0.149%
16	11.245	1520	1523	1526	rBV	30874	29559	1.35%	0.153%
17	11.316	1533	1535	1546	rVB	26955	27192	1.24%	0.141%
18	11.398	1546	1549	1552	rBV	828276	748441	34.23%	3.874%
19	11.422	1552	1553	1557	rVB	149747	101745	4.65%	0.527%
20	11.474	1559	1562	1565	rBV	71814	60370	2.76%	0.313%
21	11.645	1585	1591	1594	rBV3	22171	35411	1.62%	0.183%
22	11.904	1632	1635	1637	rBV	58183	56893	2.60%	0.295%
23	11.927	1637	1639	1643	rVV	88134	83000	3.80%	0.430%
24	11.980	1644	1648	1650	rVV	66477	64419	2.95%	0.333%
25	12.016	1650	1654	1656	rVV2	107416	120046	5.49%	0.621%
26	12.033	1656	1657	1663	rVB	50831	44500	2.04%	0.230%
27	12.198	1682	1685	1688	rVB	49643	44867	2.05%	0.232%
28	12.451	1724	1728	1730	rBV	70006	70044	3.20%	0.363%
29	12.492	1730	1735	1737	rVV2	48884	71596	3.27%	0.371%
30	12.533	1740	1742	1748	rVB3	25920	37389	1.71%	0.194%
31	12.616	1752	1756	1760	rBV	572921	478446	21.88%	2.477%
32	12.710	1770	1772	1775	rBV	53621	48530	2.22%	0.251%
33	12.827	1789	1792	1793	rBV	123396	106710	4.88%	0.552%
34	12.845	1793	1795	1798	rVV	432119	378312	17.30%	1.958%
35	12.892	1802	1803	1808	rVB2	53584	56313	2.58%	0.292%
36	12.986	1812	1819	1822	rBV	2134401	1850755	84.66%	9.581%

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF051822\
 Data File : BF128320.D
 Acq On : 18 May 2022 19:26
 Operator : CG\JU
 Sample : N2906-01
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 CDF-1

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF050922.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

37	13.057	1827	1831	1837	rVB3	54291	99324	4.54%	0.514%
38	13.151	1844	1847	1848	rBV2	42338	46390	2.12%	0.240%
39	13.174	1848	1851	1854	rVB2	159075	137860	6.31%	0.714%
40	13.239	1859	1862	1865	rVV	141666	113659	5.20%	0.588%
41	13.280	1865	1869	1872	rVB2	75371	85358	3.90%	0.442%
42	13.374	1881	1885	1887	rBV	34830	37469	1.71%	0.194%
43	13.404	1887	1890	1898	rVB3	51340	80398	3.68%	0.416%
44	13.657	1930	1933	1936	rBV3	38402	41692	1.91%	0.216%
45	13.686	1936	1938	1942	rVB3	30784	37125	1.70%	0.192%
46	13.821	1959	1961	1963	rVB	54425	36557	1.67%	0.189%
47	13.892	1971	1973	1981	rVB5	46856	81754	3.74%	0.423%
48	13.963	1981	1985	1990	rBV4	13829	28844	1.32%	0.149%
49	14.045	1994	1999	2002	rBV2	662243	846548	38.72%	4.382%
50	14.074	2002	2004	2011	rVB	258772	236012	10.80%	1.222%
51	14.133	2011	2014	2016	rBV2	31937	40774	1.87%	0.211%
52	14.198	2022	2025	2028	rVB2	47959	41550	1.90%	0.215%
53	14.398	2056	2059	2060	rBV	25114	26042	1.19%	0.135%
54	14.433	2060	2065	2068	rVV	90260	102879	4.71%	0.533%
55	14.468	2068	2071	2073	rVB	32837	33129	1.52%	0.171%
56	14.533	2079	2082	2084	rBV	30954	31802	1.45%	0.165%
57	14.580	2088	2090	2094	rVB	54889	48289	2.21%	0.250%
58	14.792	2123	2126	2130	rVB5	40904	44659	2.04%	0.231%
59	15.098	2174	2178	2181	rBV	194593	300947	13.77%	1.558%
60	15.210	2193	2197	2202	rBV	65607	70246	3.21%	0.364%
61	15.410	2227	2231	2236	rVB	114968	149788	6.85%	0.775%
62	15.474	2237	2242	2247	rVV	219557	283831	12.98%	1.469%
63	15.539	2248	2253	2256	rVV	422461	531213	24.30%	2.750%
64	15.568	2256	2258	2264	rVB2	54462	76022	3.48%	0.394%
65	16.104	2347	2349	2354	rVB4	18041	26006	1.19%	0.135%
66	17.045	2503	2509	2516	rBV2	85069	167490	7.66%	0.867%
67	17.227	2535	2540	2544	rBV	22583	40248	1.84%	0.208%
68	17.504	2582	2587	2594	rVB	53513	100339	4.59%	0.519%
69	17.751	2625	2629	2638	rVB3	23134	52340	2.39%	0.271%




Sum of corrected areas: 19317223

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF051822\
Data File : BF128320.D
Acq On : 18 May 2022 19:26
Operator : CG\JU
Sample : N2906-01
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
CDF-1

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF050922.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

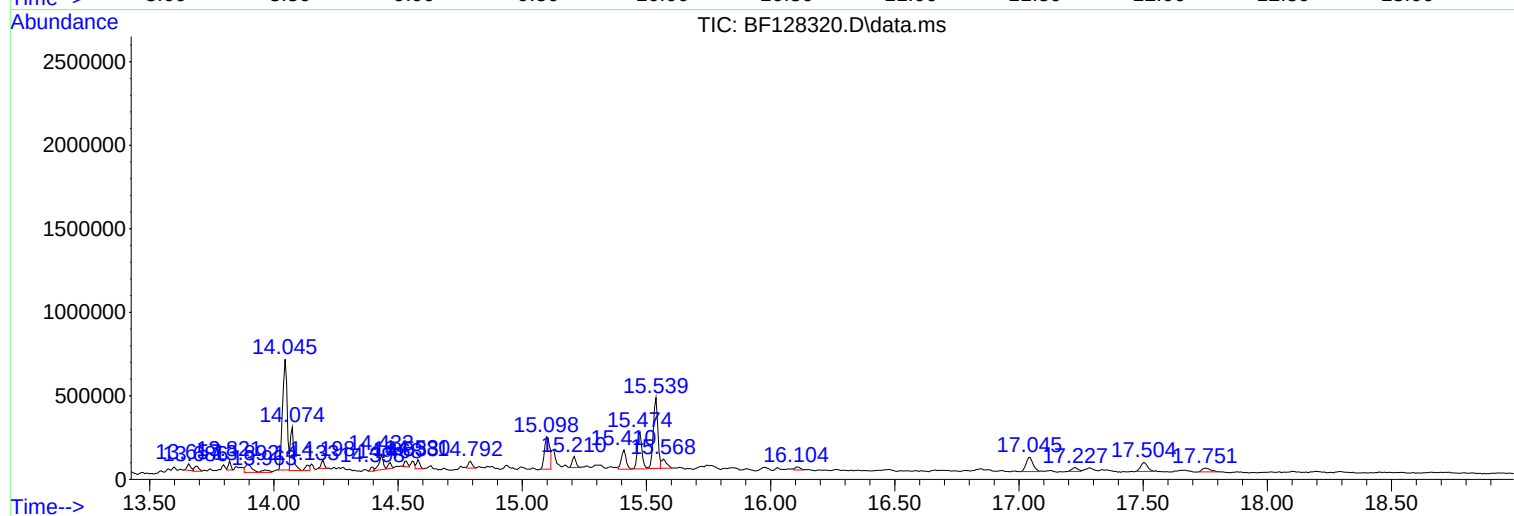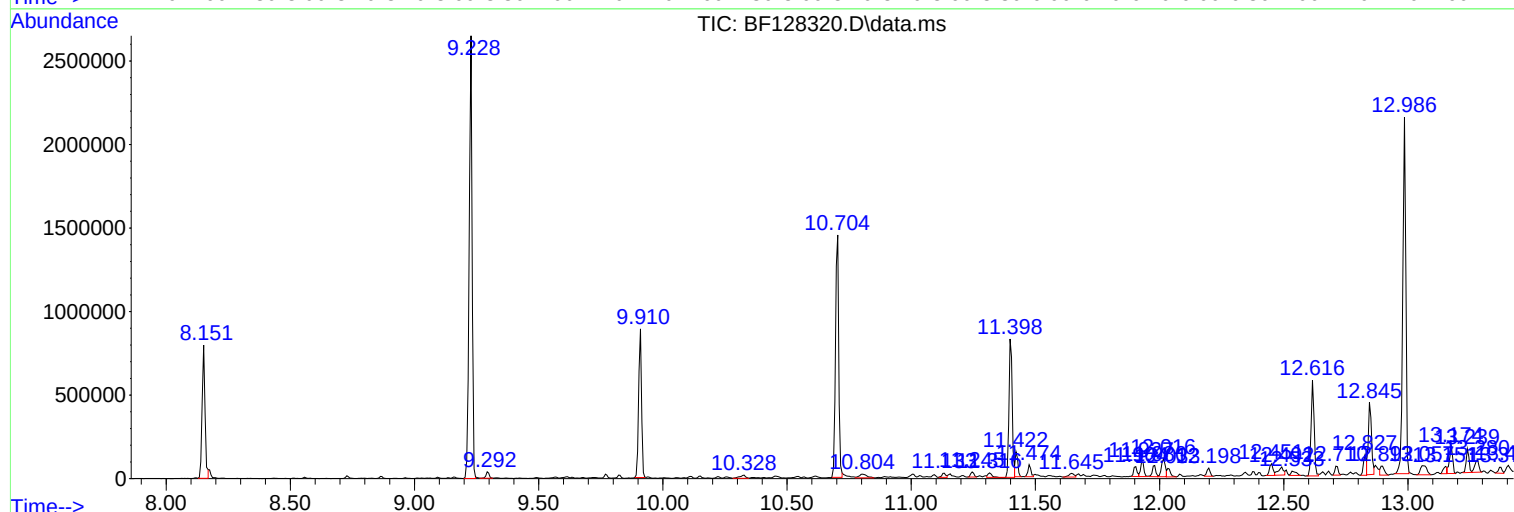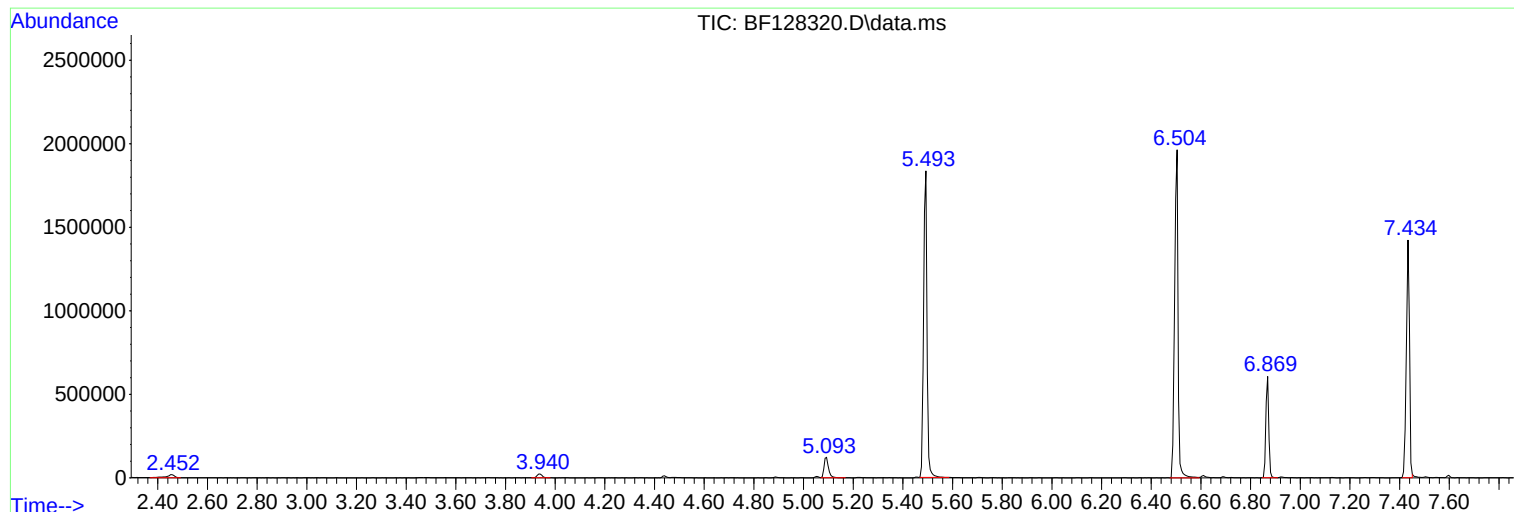

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF051822\
Data File : BF128320.D
Acq On : 18 May 2022 19:26
Operator : CG\JU
Sample : N2906-01
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
CDF-1










Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF050922.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 2-Pentanone, 4-hydroxy-4-me... Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
5.093	6.17 ng	154781	1,4-Dichlorobenzene-d4	6.869

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1	2-Pentanone, 4-hydroxy-4-methyl-	116	C6H12O2	000123-42-2	45		
2	Acetic acid, cyano-, 1,1-dimethy...	141	C7H11NO2	001116-98-9	25		
3	Butane, 1-ethoxy-	102	C6H14O	000628-81-9	9		
4	Morpholine, 4-methyl-	101	C5H11NO	000109-02-4	9		
5	2,3-Butanedione, monooxime	101	C4H7NO2	000057-71-6	9		

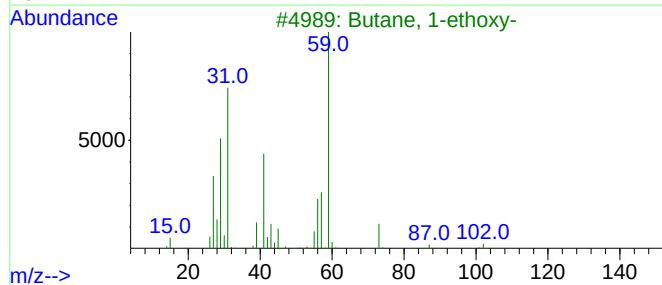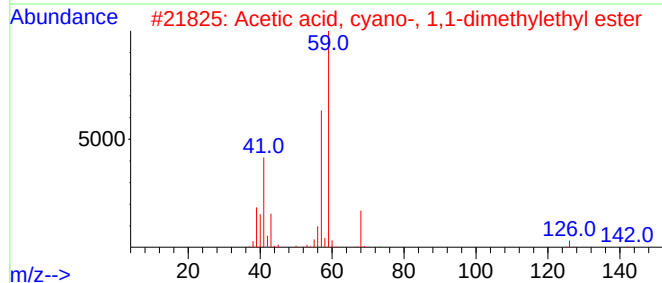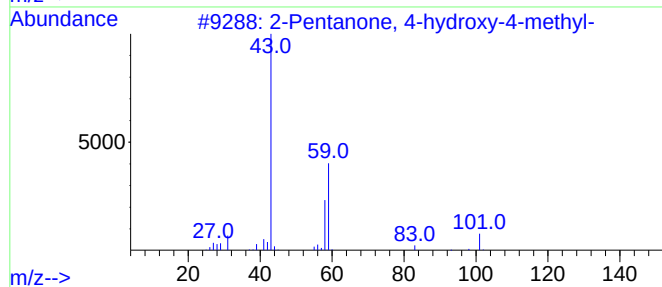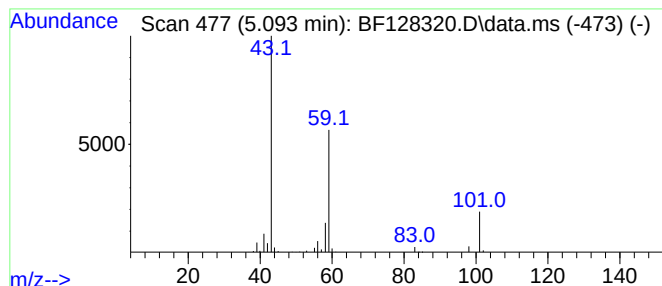

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF051822\
Data File : BF128320.D
Acq On : 18 May 2022 19:26
Operator : CG\JU
Sample : N2906-01
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
CDF-1










Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF050922.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 2 1H-Cyclopropa[l]phenanthren... Concentration Rank 9

R.T.	EstConc	Area	Relative to ISTD	R.T.
11.927	2.22 ng	83000	Phenanthrene-d10	11.398

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			1H-Cyclopropa[l]phenanthrene,1a,...	192	C15H12	000949-41-7	95
2			Phenanthrene, 1-methyl-	192	C15H12	000832-69-9	93
3			Phenanthrene, 4-methyl-	192	C15H12	000832-64-4	93
4			5H-Dibenzo[a,d]cycloheptene	192	C15H12	000256-81-5	93
5			Anthracene, 2-methyl-	192	C15H12	000613-12-7	91

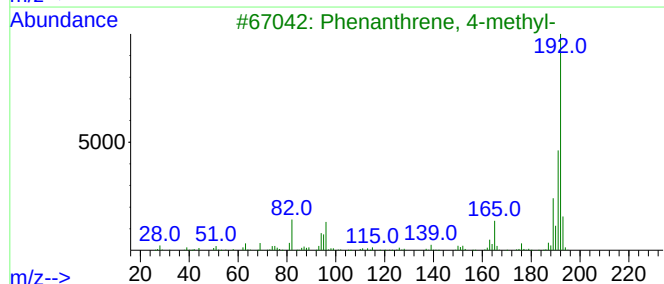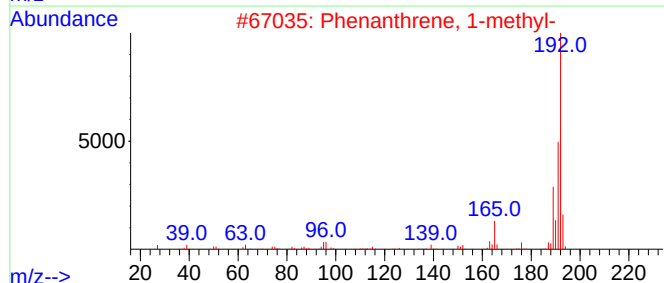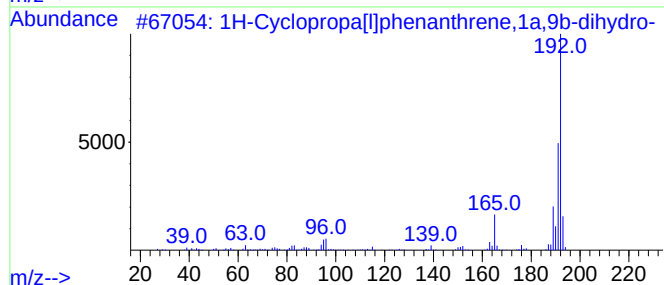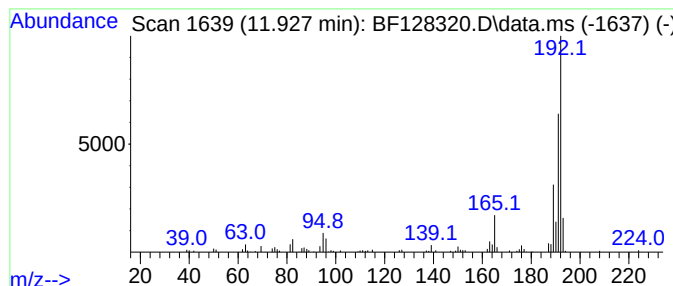

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF051822\
Data File : BF128320.D
Acq On : 18 May 2022 19:26
Operator : CG\JU
Sample : N2906-01
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
CDF-1










Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF050922.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 3 4H-Cyclopenta[def]phenanthrene Concentration Rank 4

R.T.	EstConc	Area	Relative to ISTD	R.T.
12.016	3.21 ng	120046	Phenanthrene-d10	11.398

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			4H-Cyclopenta[def]phenanthrene	190	C15H10	000203-64-5	58
2			6H-Cyclobuta[jk]phenanthrene	190	C15H10	083469-43-6	53
3			Thiophene-3-carboxaldehyde, 5-ch...	190	C5H4BClO3S	036155-87-0	50
4			4,6-Dichloro-2-ethylpyrimidin-5-...	191	C6H7Cl2N3	006237-96-3	43
5			Methyl diselenide	190	C2H6Se2	007101-31-7	38

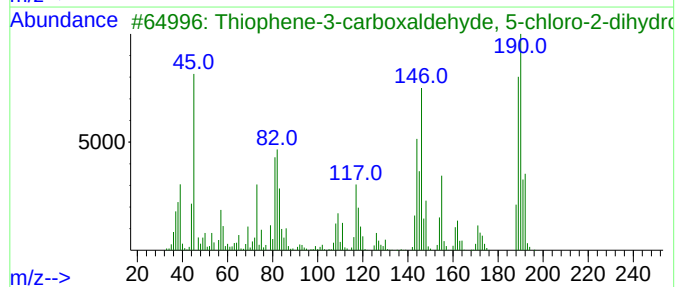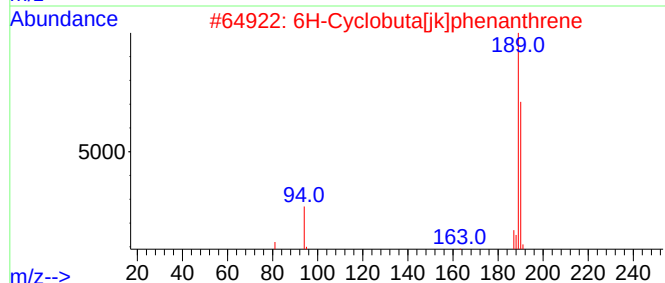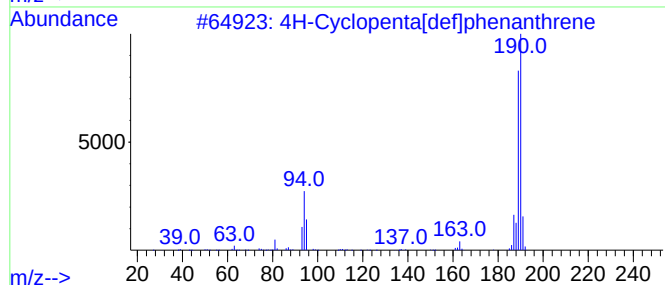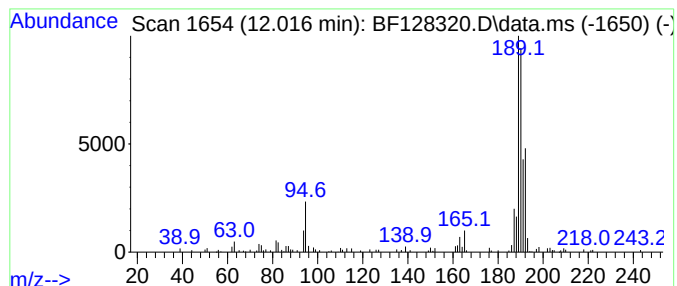

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF051822\
Data File : BF128320.D
Acq On : 18 May 2022 19:26
Operator : CG\JU
Sample : N2906-01
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
CDF-1










Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF050922.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 4 Pyrene, 1-methyl- Concentration Rank 8

R.T.	EstConc	Area	Relative to ISTD	R.T.
13.057	2.35 ng	99324	Chrysene-d12	14.045

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Pyrene, 1-methyl-	216	C17H12	002381-21-7	90
2			11H-Benzo[b]fluorene	216	C17H12	000243-17-4	50
3			Benzo[b]naphtho[2,3-d]furan	218	C16H10O	000243-42-5	49
4			Fluoranthene, 2-methyl-	216	C17H12	033543-31-6	49
5			Pyrene, 2-methyl-	216	C17H12	003442-78-2	45

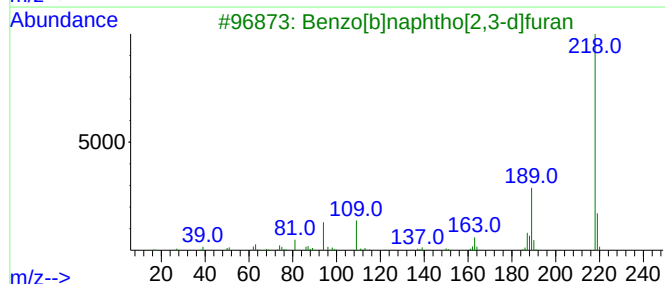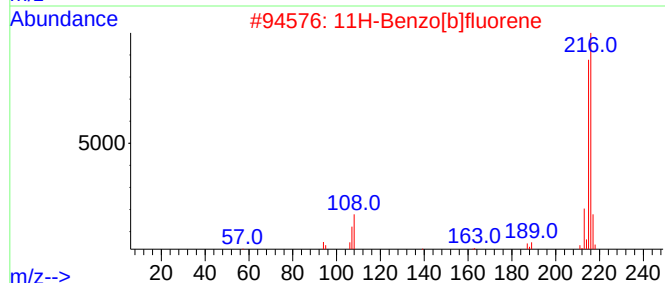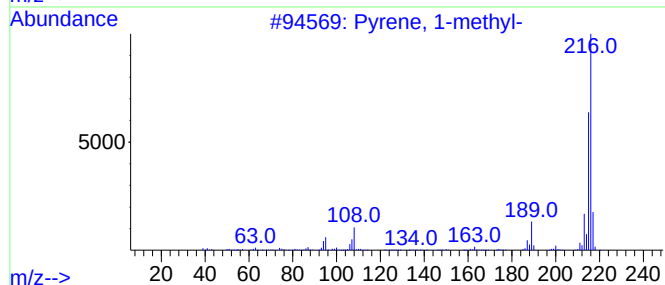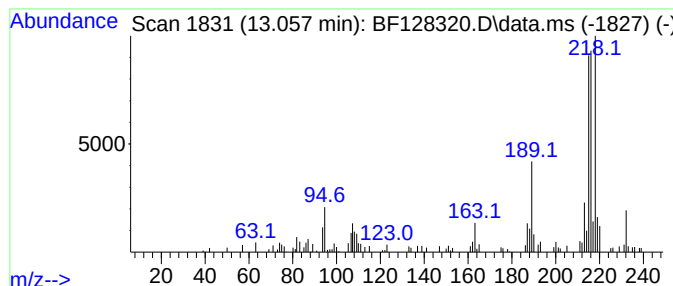

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF051822\
Data File : BF128320.D
Acq On : 18 May 2022 19:26
Operator : CG\JU
Sample : N2906-01
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
CDF-1










Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF050922.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 5 11H-Benzo[a]fluorene Concentration Rank 3

R.T.	EstConc	Area	Relative to ISTD	R.T.
13.174	3.26 ng	137860	Chrysene-d12	14.045

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			11H-Benzo[a]fluorene	216	C17H12	000238-84-6	95
2			11H-Benzo[b]fluorene	216	C17H12	000243-17-4	93
3			Pyrene, 1-methyl-	216	C17H12	002381-21-7	93
4			Fluoranthene, 2-methyl-	216	C17H12	033543-31-6	91
5			Pyrene, 2-methyl-	216	C17H12	003442-78-2	90

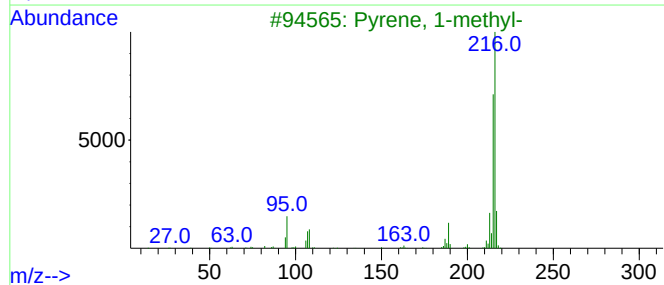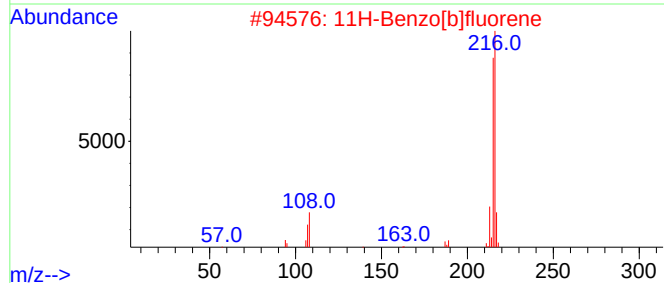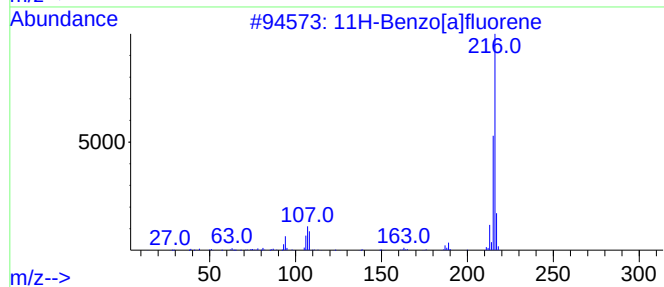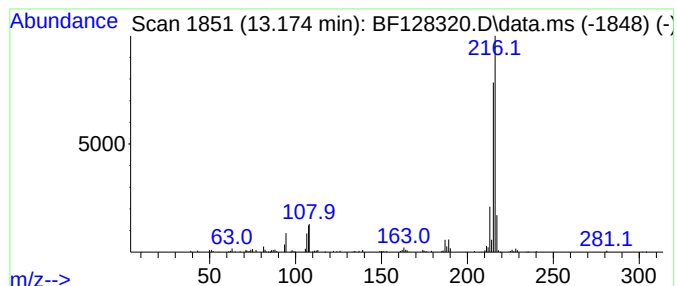

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF051822\
Data File : BF128320.D
Acq On : 18 May 2022 19:26
Operator : CG\JU
Sample : N2906-01
Misc :
ALS Vial : 15 Sample Multiplier: 1










Instrument :
BNA_F
ClientSampleId :
CDF-1

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF050922.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 6 11H-Benzo[b]fluorene Concentration Rank 5

R.T.	EstConc	Area	Relative to ISTD	R.T.	
13.239	2.69 ng	113659	Chrysene-d12	14.045	
Hit# of 5	Tentative ID	MW	MolForm	CAS#	Qual
1	Pyrene, 1-methyl-	216	C17H12	002381-21-7	93
2	11H-Benzo[b]fluorene	216	C17H12	000243-17-4	91
3	11H-Benzo[a]fluorene	216	C17H12	000238-84-6	90
4	Fluoranthene, 2-methyl-	216	C17H12	033543-31-6	90
5	7H-Benzo[c]fluorene	216	C17H12	000205-12-9	74

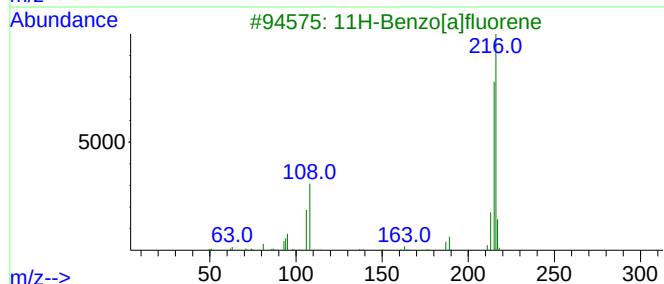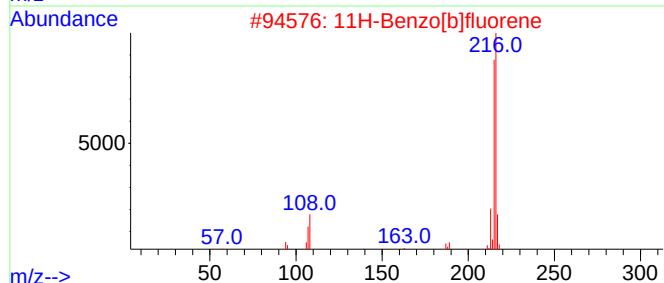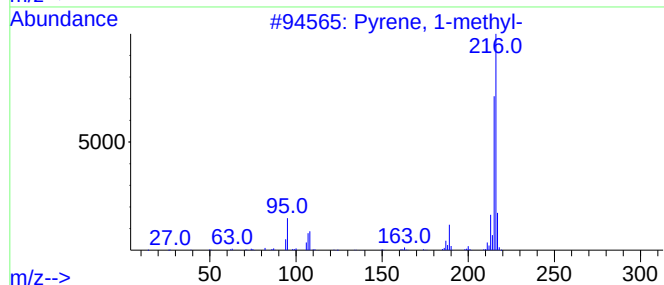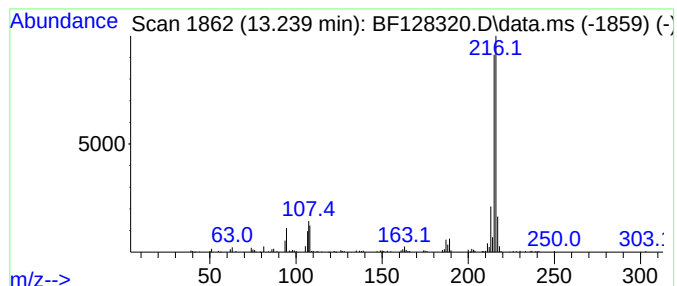

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF051822\
Data File : BF128320.D
Acq On : 18 May 2022 19:26
Operator : CG\JU
Sample : N2906-01
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
CDF-1










Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF050922.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 7 Pyrene, 2-methyl- Concentration Rank 10

R.T.	EstConc	Area	Relative to ISTD	R.T.
13.280	2.02 ng	85358	Chrysene-d12	14.045

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1	Pyrene, 1-methyl-			216	C17H12	002381-21-7	95
2	Pyrene, 2-methyl-			216	C17H12	003442-78-2	90
3	Pyrene, 4-methyl-			216	C17H12	003353-12-6	83
4	11H-Benzo[a]fluorene			216	C17H12	000238-84-6	70
5	Fluoranthene, 2-methyl-			216	C17H12	033543-31-6	64

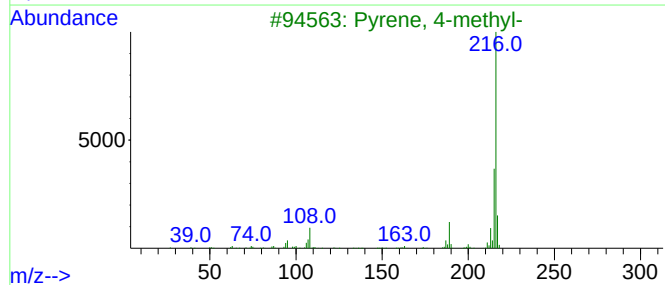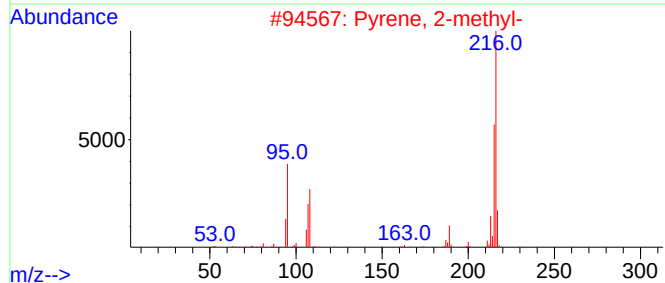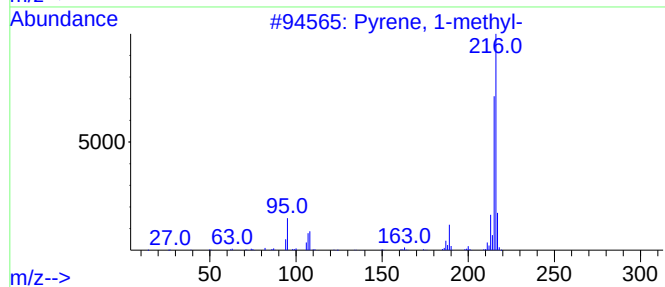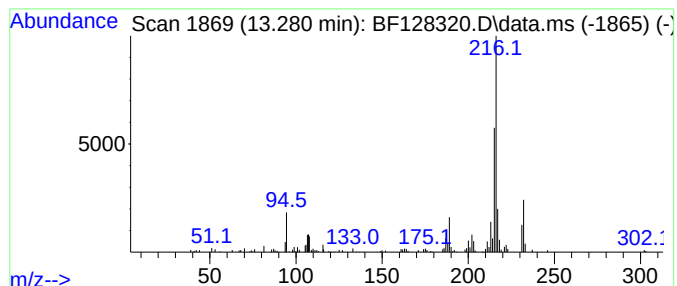

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF051822\
Data File : BF128320.D
Acq On : 18 May 2022 19:26
Operator : CG\JU
Sample : N2906-01
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
CDF-1










Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF050922.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 8 2-Methylchrysene Concentration Rank 7

R.T.	EstConc	Area	Relative to ISTD	R.T.
14.433	2.43 ng	102879	Chrysene-d12	14.045

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			2-Methylchrysene	242	C19H14	003351-32-4	93
2			Triphenylene, 2-methyl-	242	C19H14	001705-84-6	91
3			Chrysene, 1-methyl-	242	C19H14	003351-28-8	90
4			Chrysene, 5-methyl-	242	C19H14	003697-24-3	90
5			Benz[a]anthracene, 2-methyl-	242	C19H14	002498-76-2	90

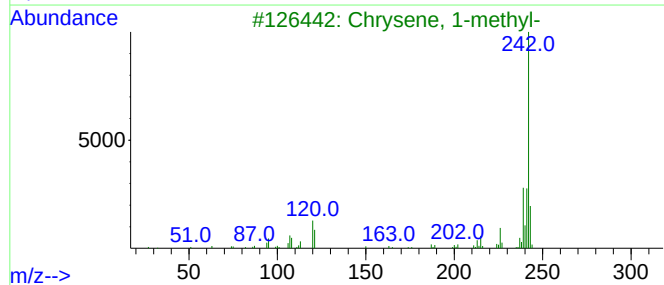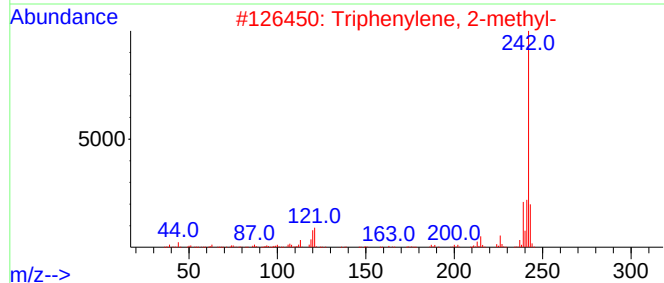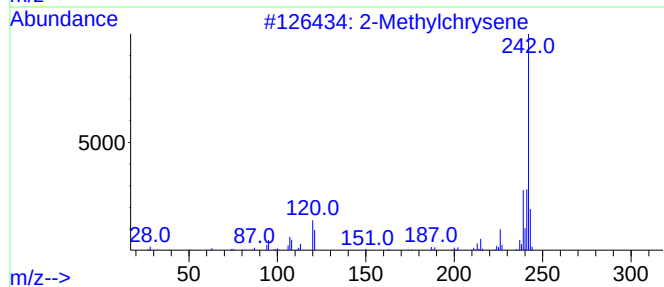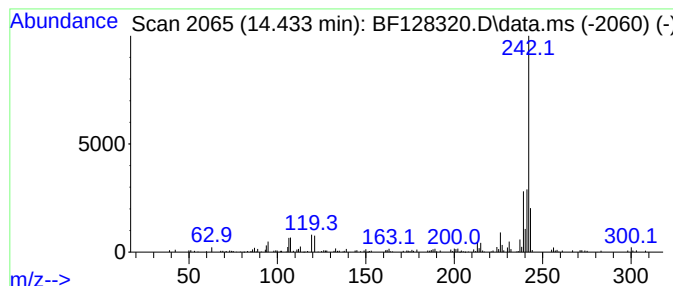

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF051822\
Data File : BF128320.D
Acq On : 18 May 2022 19:26
Operator : CG\JU
Sample : N2906-01
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
CDF-1










Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF050922.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 9 Benzo[e]pyrene Concentration Rank 6

R.T.	EstConc	Area	Relative to ISTD	R.T.
15.210	2.64 ng	70246	Perylene-d12	15.539

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Benzo[e]pyrene	252	C20H12	000192-97-2	95
2			Benzo[a]pyrene	252	C20H12	000050-32-8	91
3			Benzo[b]fluoranthene	252	C20H12	000205-99-2	90
4			Benzo[k]fluoranthene	252	C20H12	000207-08-9	89
5			Perylene	252	C20H12	000198-55-0	81

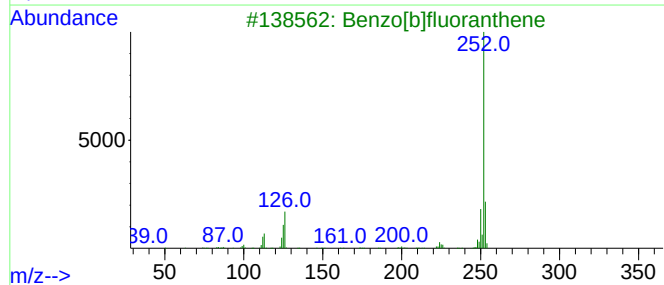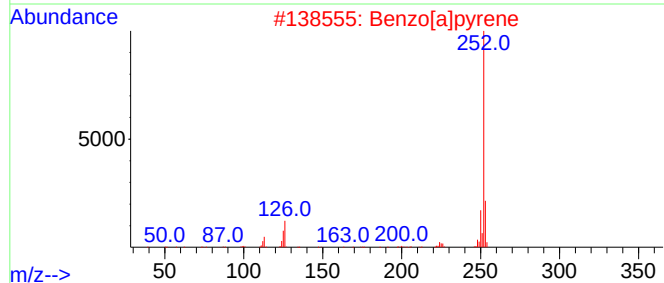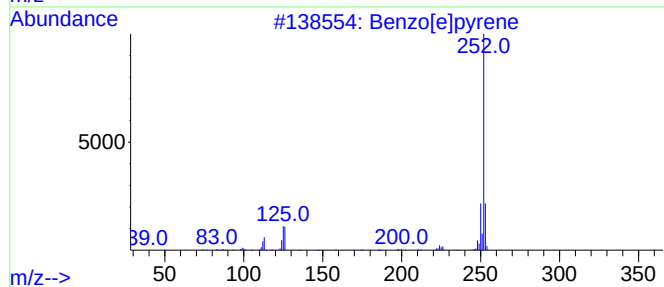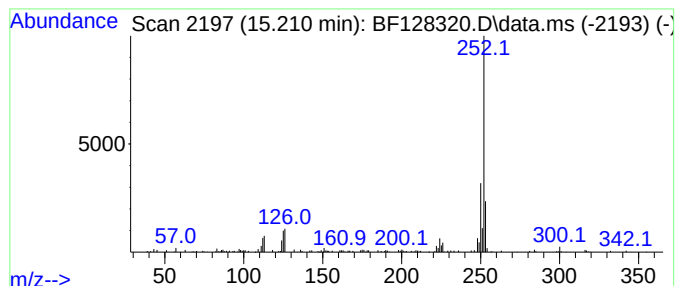

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF051822\
Data File : BF128320.D
Acq On : 18 May 2022 19:26
Operator : CG\JU
Sample : N2906-01
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
CDF-1










Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF050922.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 10 Benzo[j]fluoranthene Concentration Rank 2

R.T.	EstConc	Area	Relative to ISTD	R.T.
15.410	5.64 ng	149788	Perylene-d12	15.539

Hit#	of 5	Tentative ID	MW	MolForm	CAS#	Qual
1		Benzo[e]pyrene	252	C20H12	000192-97-2	98
2		Benzo[k]fluoranthene	252	C20H12	000207-08-9	97
3		Benzo[b]fluoranthene	252	C20H12	000205-99-2	95
4		Benzo[j]fluoranthene	252	C20H12	000205-82-3	95
5		Benzo[a]pyrene	252	C20H12	000050-32-8	95

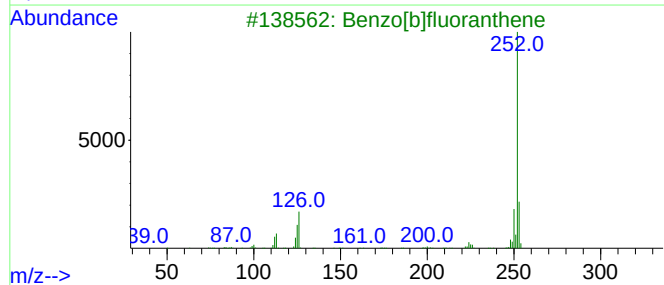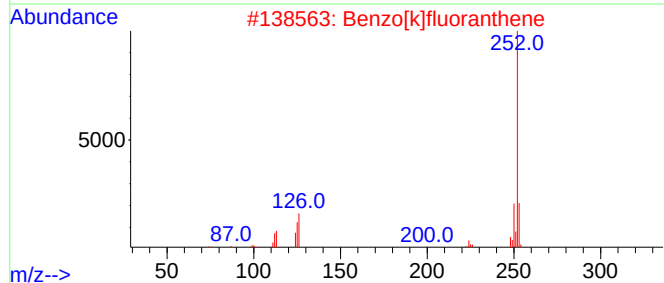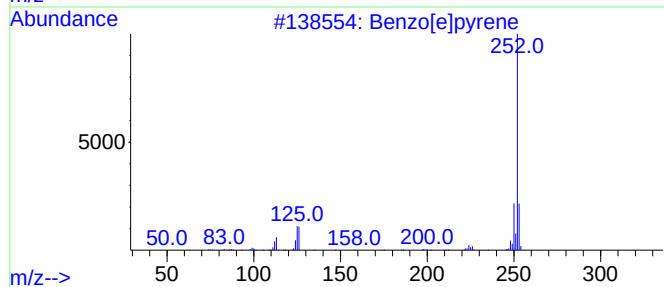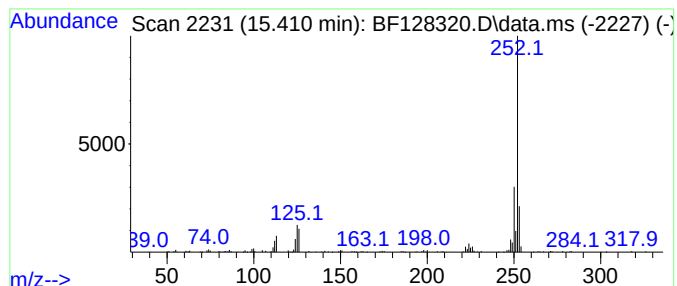

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF051822\
Data File : BF128320.D
Acq On : 18 May 2022 19:26
Operator : CG\JU
Sample : N2906-01
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
CDF-1

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF050922.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
2-Pentanone, 4-...	5.093	6.2	ng	154781	1	6.869	501743	20.0
1H-Cyclopropa[1...	11.927	2.2	ng	83000	4	11.398	748441	20.0
4H-Cyclopenta[d...	12.016	3.2	ng	120046	4	11.398	748441	20.0
Pyrene, 1-methyl-	13.057	2.4	ng	99324	5	14.045	846548	20.0
11H-Benzo[a]flu...	13.174	3.3	ng	137860	5	14.045	846548	20.0
11H-Benzo[b]flu...	13.239	2.7	ng	113659	5	14.045	846548	20.0
Pyrene, 2-methyl-	13.280	2.0	ng	85358	5	14.045	846548	20.0
2-Methylchrysene	14.433	2.4	ng	102879	5	14.045	846548	20.0
Benzo[e]pyrene	15.210	2.6	ng	70246	6	15.539	531213	20.0
Benzo[j]fluoran...	15.410	5.6	ng	149788	6	15.539	531213	20.0