

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF051822\
 Data File : BF128326.D
 Acq On : 18 May 2022 22:23
 Operator : CG\JU
 Sample : N2864-12 10X
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 P011-SS005-0006-01

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF050922.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF128326.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.487	541	544	555	rBV	76356	92817	11.71%	1.999%
2	6.504	714	717	727	rBV	77483	97603	12.32%	2.102%
3	6.869	775	779	790	rBV	654553	568183	71.69%	12.236%
4	7.434	871	875	885	rBV	69525	67557	8.52%	1.455%
5	8.151	993	997	1010	rBV	906931	730575	92.19%	15.734%
6	9.222	1176	1179	1186	rBV	157634	130927	16.52%	2.820%
7	9.486	1221	1224	1227	rBV	29410	24138	3.05%	0.520%
8	9.910	1292	1296	1299	rBV	1007416	792501	100.00%	17.067%
9	10.698	1427	1430	1439	rVB	63933	62939	7.94%	1.355%
10	10.992	1477	1480	1483	rVB2	15490	11643	1.47%	0.251%
11	11.398	1546	1549	1553	rBV	845470	764742	96.50%	16.470%
12	12.980	1815	1818	1823	rVB	148727	122319	15.43%	2.634%
13	13.898	1972	1974	1979	rBV6	11173	13851	1.75%	0.298%
14	14.045	1995	1999	2003	rBV	674506	644847	81.37%	13.888%
15	14.139	2012	2015	2018	rVB	22252	21758	2.75%	0.469%
16	15.539	2248	2253	2259	rVB	393710	496952	62.71%	10.702%




Sum of corrected areas: 4643352

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF051822\
Data File : BF128326.D
Acq On : 18 May 2022 22:23
Operator : CG\JU
Sample : N2864-12 10X
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
P011-SS005-0006-01

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF050922.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

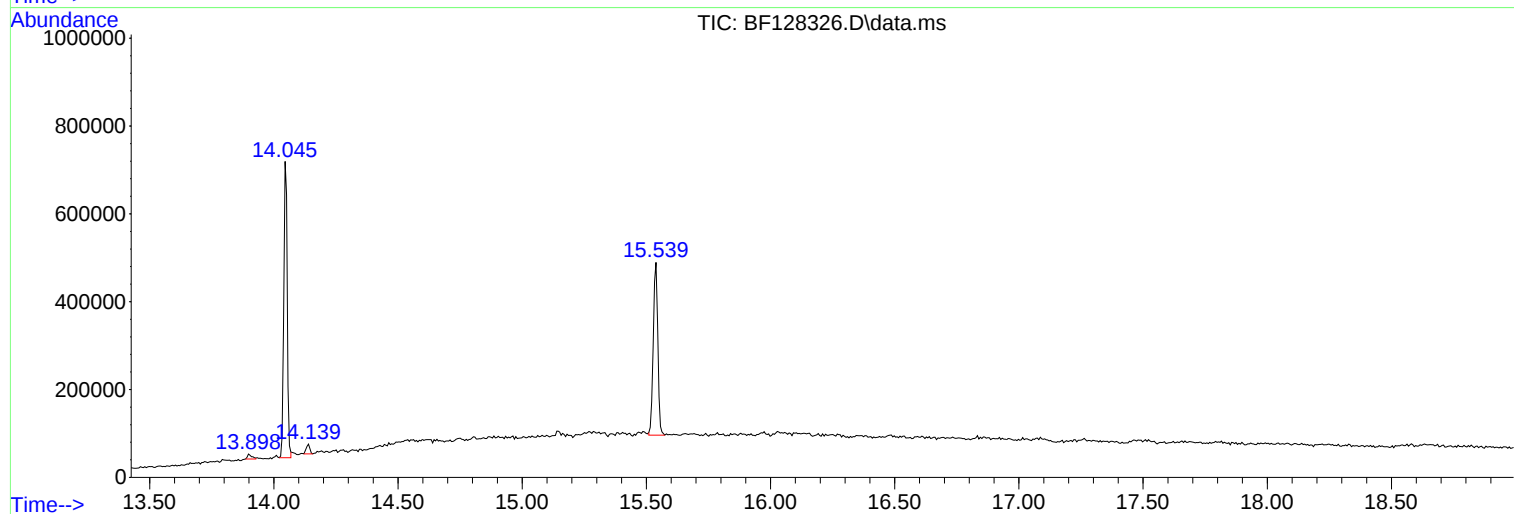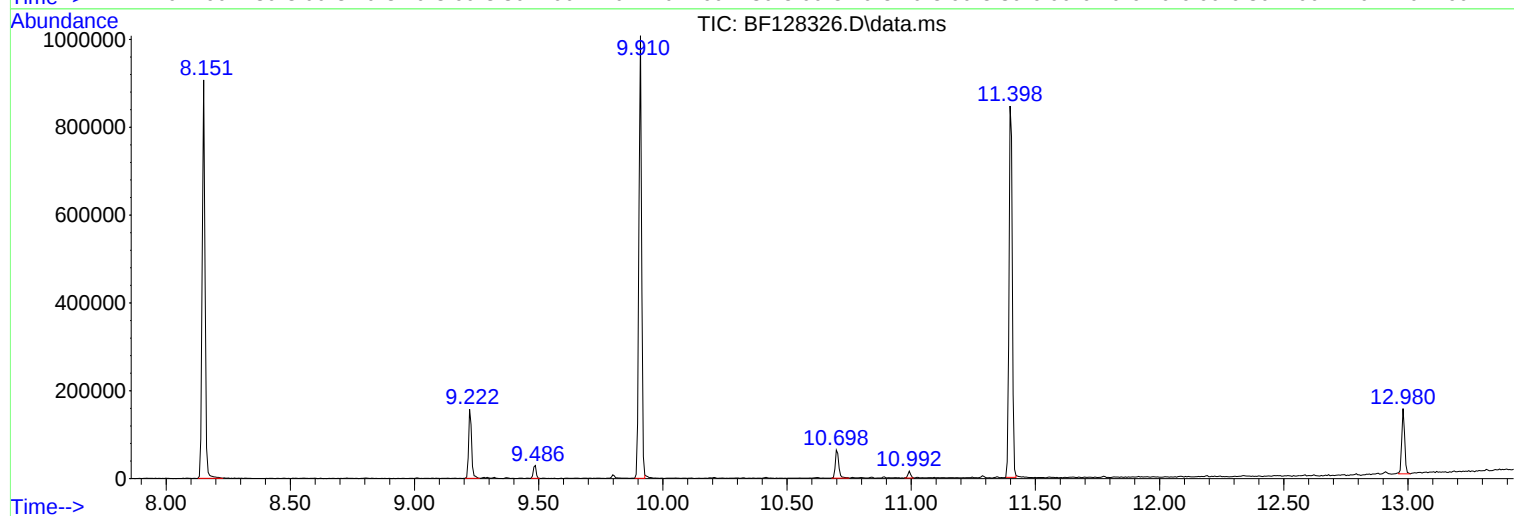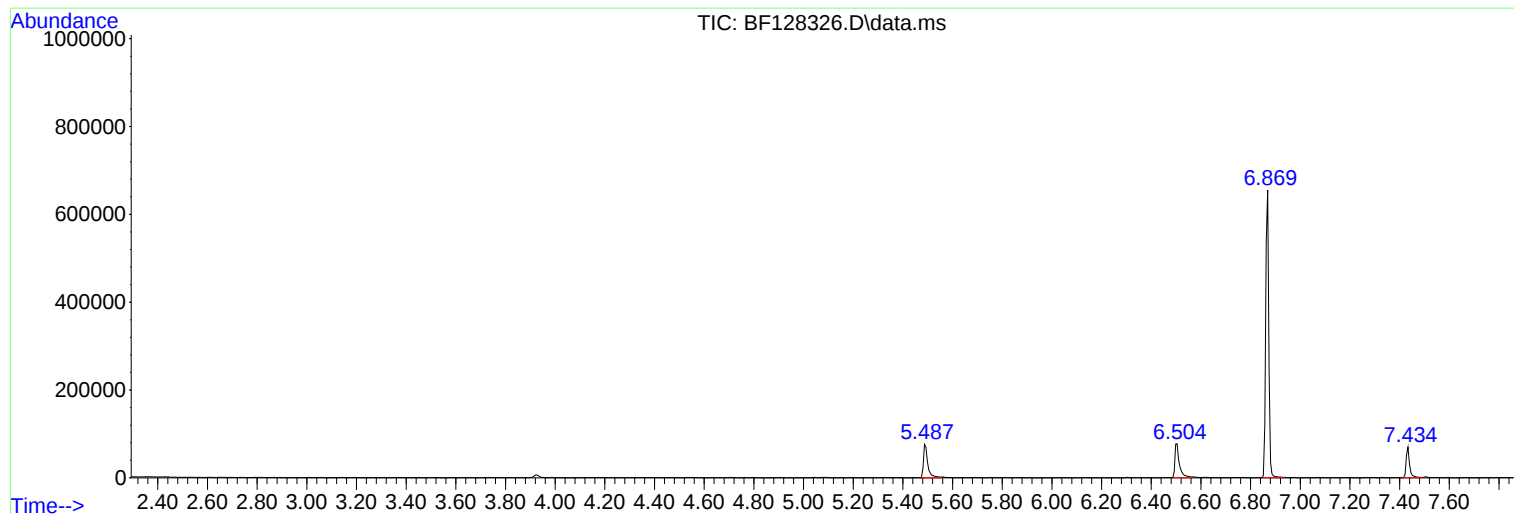

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF051822\
Data File : BF128326.D
Acq On : 18 May 2022 22:23
Operator : CG\JU
Sample : N2864-12 10X
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
P011-SS005-0006-01

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF050922.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF051822\
Data File : BF128326.D
Acq On : 18 May 2022 22:23
Operator : CG\JU
Sample : N2864-12 10X
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
P011-SS005-0006-01

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF050922.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------