


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF051822\
 Data File : BF128306.D
 Acq On : 18 May 2022 12:02
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF050922.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu May 19 06:47:51 2022

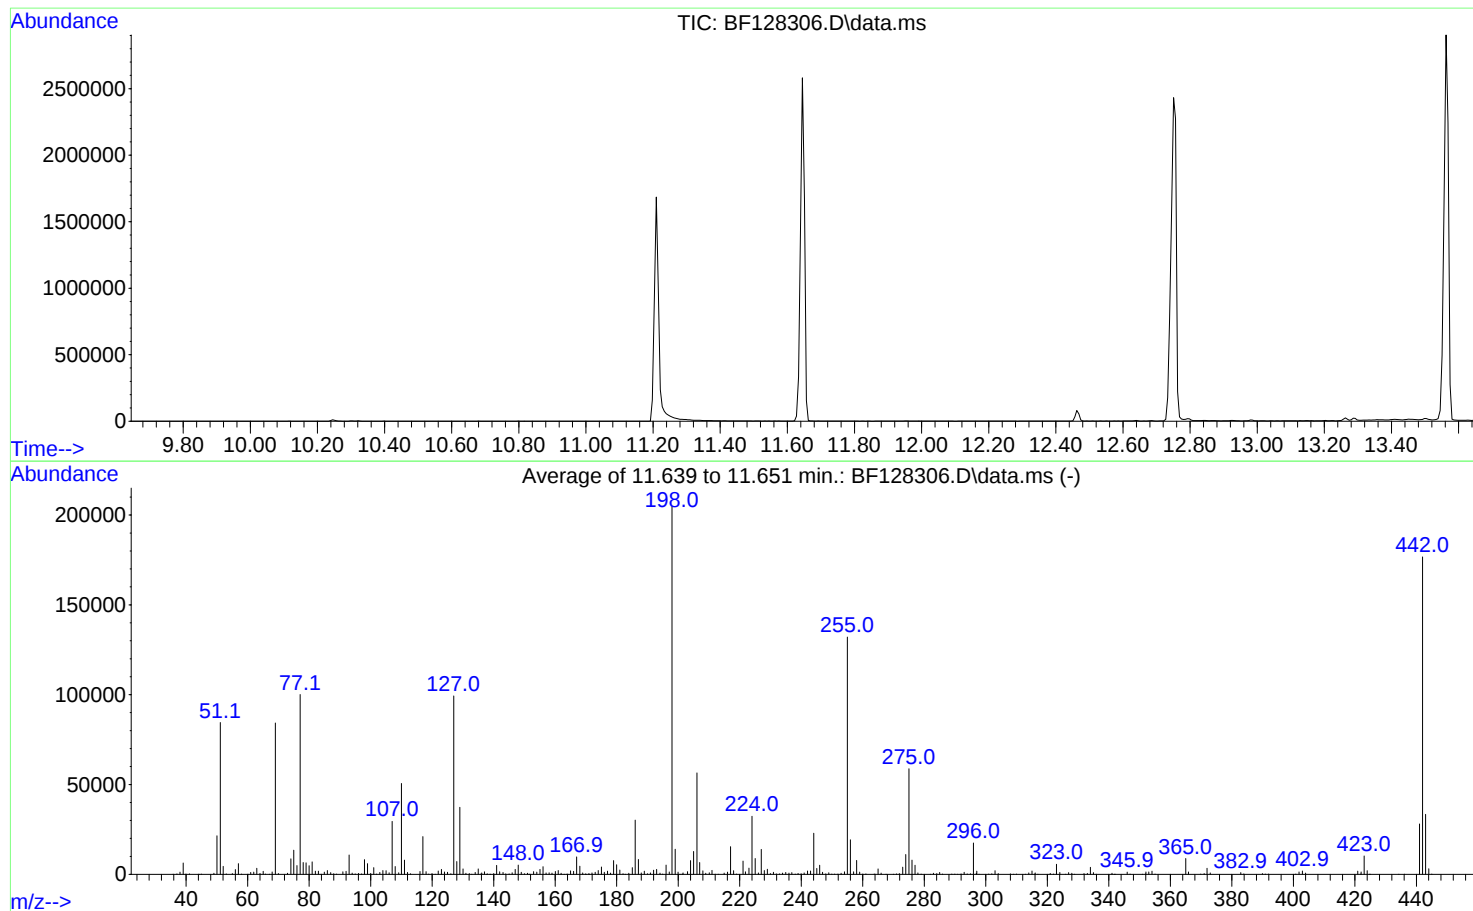




AutoFind: Scans 1590, 1591, 1592; Background Corrected with Scan 1584

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	41.3	84525	PASS
68	69	0.00	2	1.6	1337	PASS
69	198	0.00	100	41.2	84293	PASS
70	69	0.00	2	0.5	419	PASS
127	198	10	80	48.5	99315	PASS
197	198	0.00	2	0.7	1368	PASS
198	198	100	100	100.0	204757	PASS
199	198	5	9	6.8	13974	PASS
275	198	10	60	28.7	58744	PASS
365	198	1	100	4.3	8823	PASS
441	198	0.01	100	13.7	28047	PASS
442	442	50	100	100.0	176669	PASS
443	442	15	24	18.9	33428	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF051822\
Data File : BF128306.D
Acq On : 18 May 2022 12:02
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: May 18 16:57:03 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF050922.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed May 18 01:31:11 2022
Response via : Initial Calibration

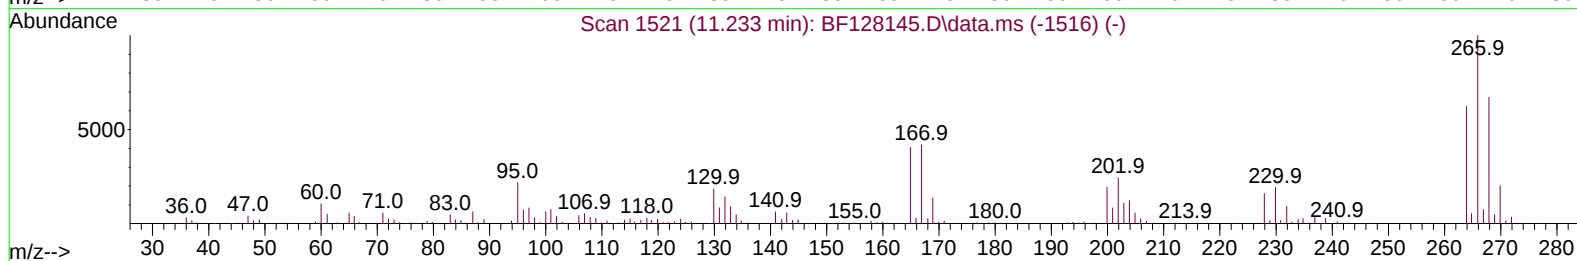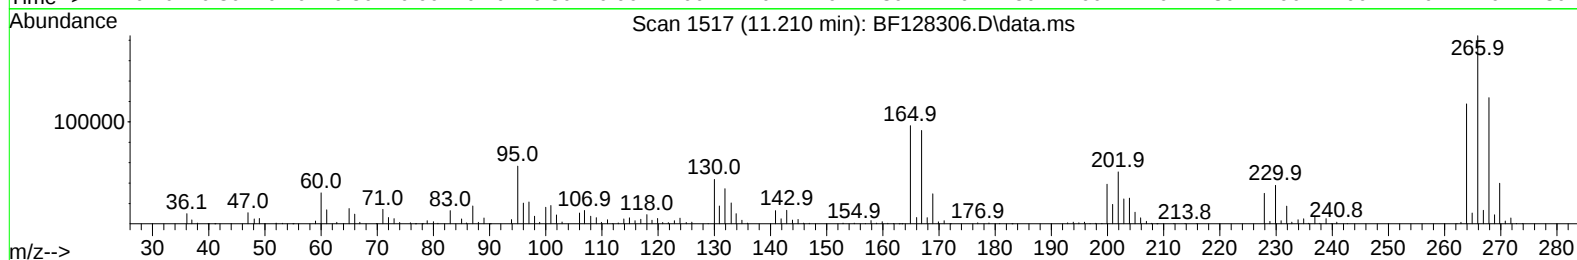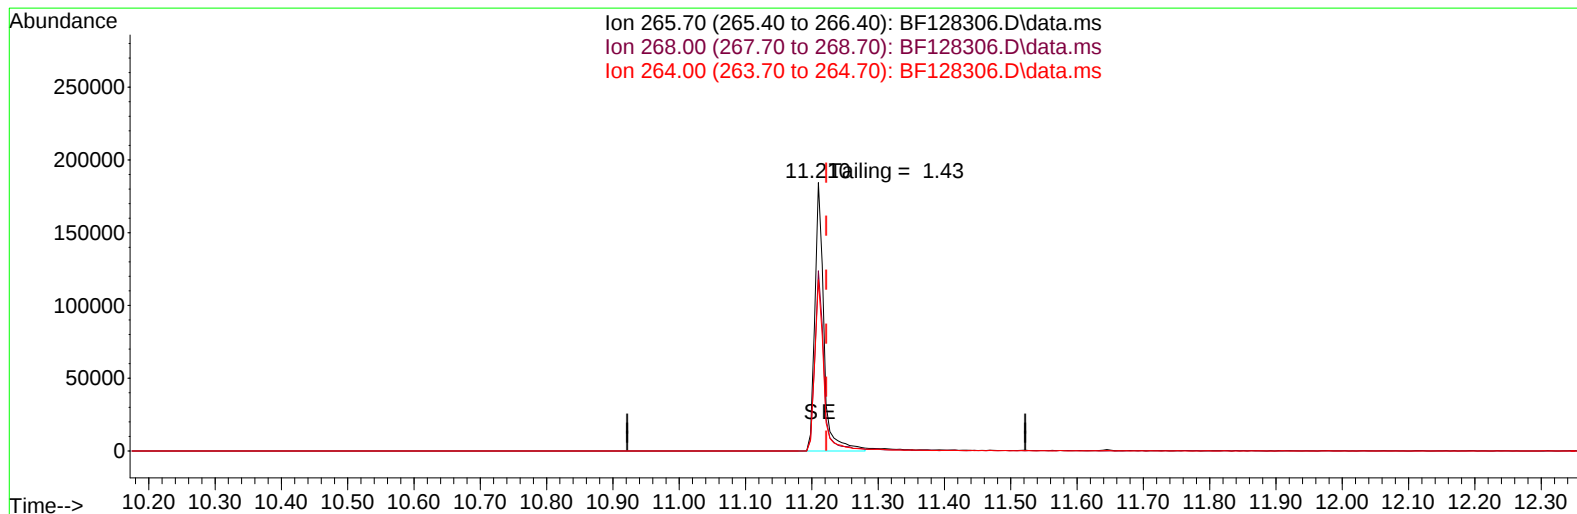

TIC: BF128306.D\data.ms

(70) Pentachlorophenol (C)

11.210min (-0.012) 33591.93 ng




response 181121

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	66.30	67.13
264.00	66.40	63.80
0.00	0.00	0.00

```
Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF051822\  
Data File : BF128306.D  
Acq On    : 18 May 2022  12:02  
Operator  : CG\JU  
Sample    : DFTPP  
Misc      :  
ALS Vial  : 1    Sample Multiplier: 1
```

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: May 18 16:57:03 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF050922.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed May 18 01:31:11 2022
Response via : Initial Calibration

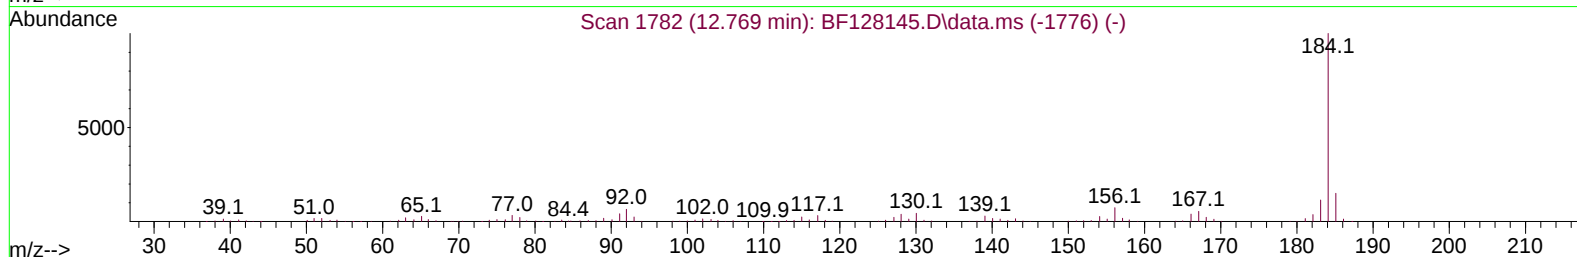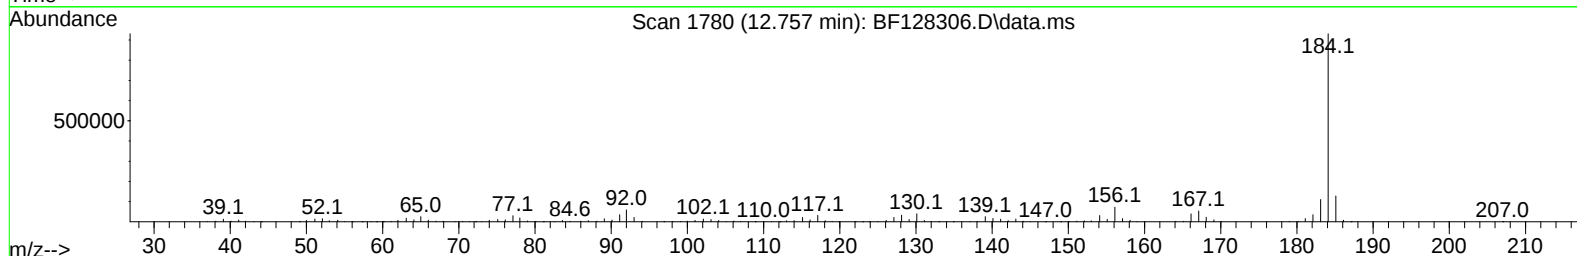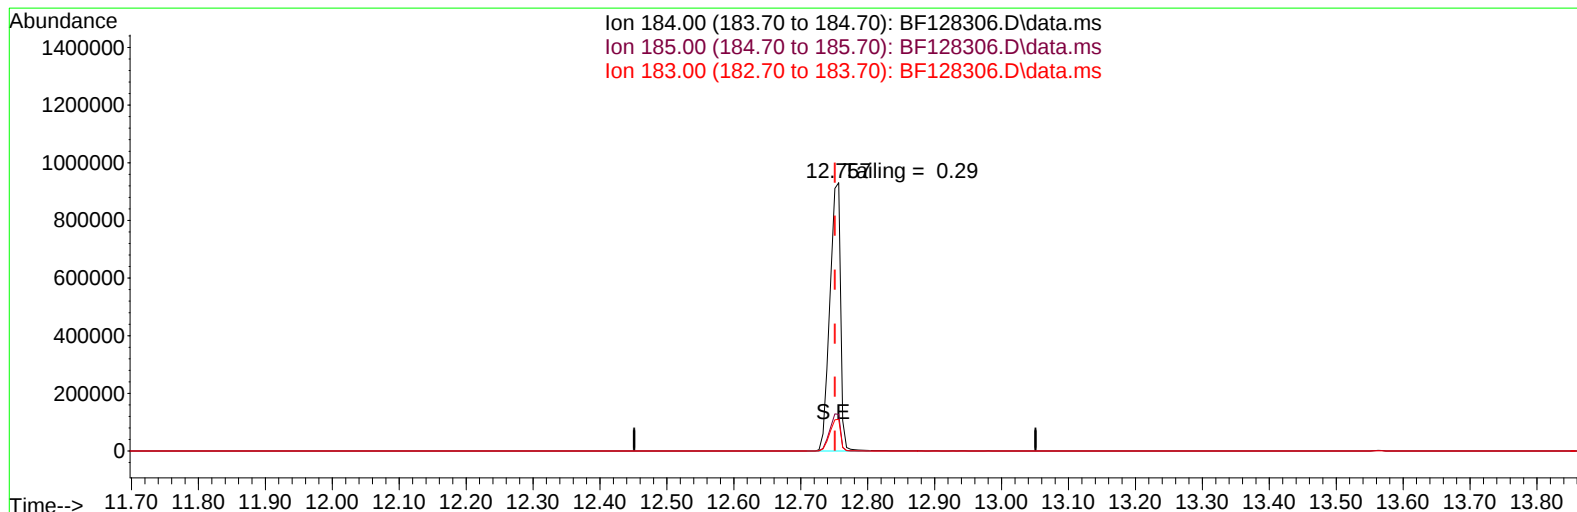

TIC: BF128306.D\data.ms

(77) Benzidine

12.757min (+ 0.006) 0.00 ng

response **1039349**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.10	13.69
183.00	11.20	11.84
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
5/18/2022	BNA_F	<u>BF128306.D</u>
Compound Name	Response	Retention Time
DDT	510873	13.56
DDD	3607	20.47
DDE	787	19.97
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
4394	515267	0.85

Instrument :
BNA_F
ClientSampleId :
DFTPP