

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF052422\
 Data File : BF128439.D
 Acq On : 24 May 2022 17:15
 Operator : CG\JU
 Sample : N2874-10
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 P007-SS002-2430-01

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF052022.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF128439.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.081	471	475	485	rBV	14432	21766	1.17%	0.168%
2	5.469	537	541	571	rBV	1835240	1773422	95.25%	13.709%
3	6.481	709	713	730	rBV	1833514	1770514	95.09%	13.687%
4	6.845	771	775	783	rBV	632785	547212	29.39%	4.230%
5	7.410	867	871	882	rBV	1321100	1187743	63.79%	9.182%
6	8.128	989	993	1006	rBV	759960	690573	37.09%	5.338%
7	9.198	1171	1175	1179	rBV	2097130	1861947	100.00%	14.394%
8	9.881	1288	1291	1295	rBV	839360	713436	38.32%	5.515%
9	10.675	1423	1426	1435	rBV	1078256	960669	51.59%	7.426%
10	11.375	1541	1545	1549	rBV	772339	623545	33.49%	4.820%
11	12.957	1810	1814	1818	rBV	1655390	1407771	75.61%	10.883%
12	13.898	1967	1974	1985	rBV10	24826	73949	3.97%	0.572%
13	14.021	1991	1995	1999	rBV	590519	571142	30.67%	4.415%
14	14.116	2007	2011	2015	rBV	43550	50811	2.73%	0.393%
15	14.669	2096	2105	2109	rBV	23165	64654	3.47%	0.500%
16	14.769	2119	2122	2127	rBV5	19969	23813	1.28%	0.184%
17	14.845	2132	2135	2141	rVB	41536	46419	2.49%	0.359%
18	15.110	2177	2180	2184	rBV2	22695	24015	1.29%	0.186%
19	15.504	2242	2247	2252	rBV	395500	522479	28.06%	4.039%




Sum of corrected areas: 12935880

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF052422\
Data File : BF128439.D
Acq On : 24 May 2022 17:15
Operator : CG\JU
Sample : N2874-10
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
P007-SS002-2430-01

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF052022.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

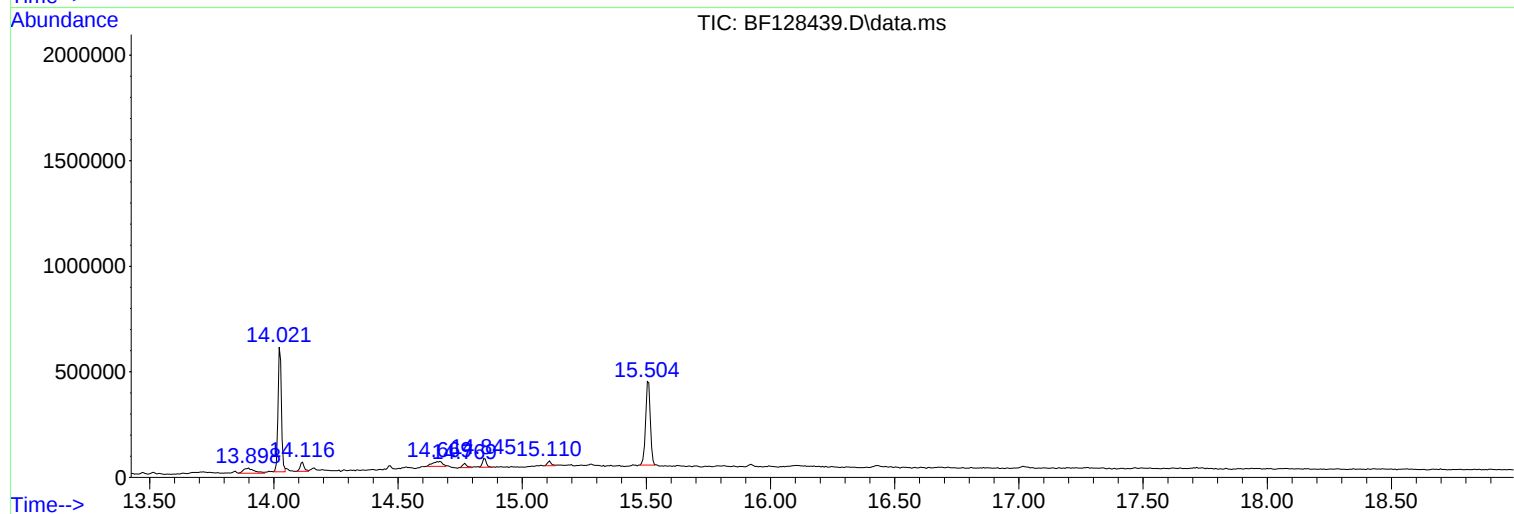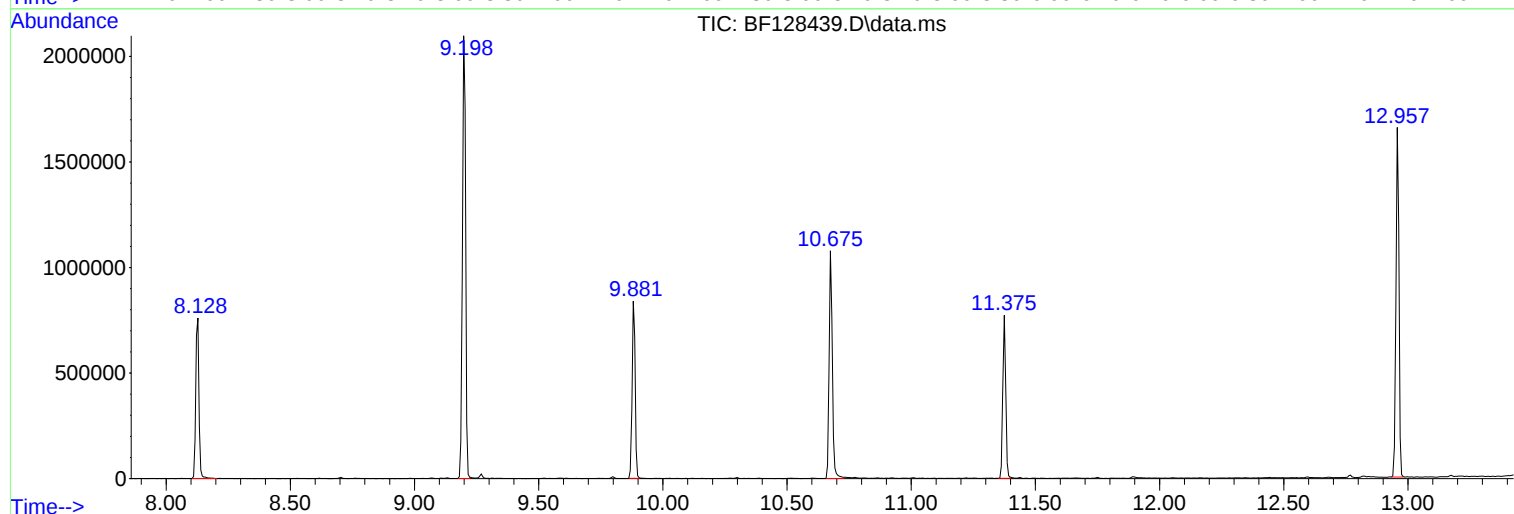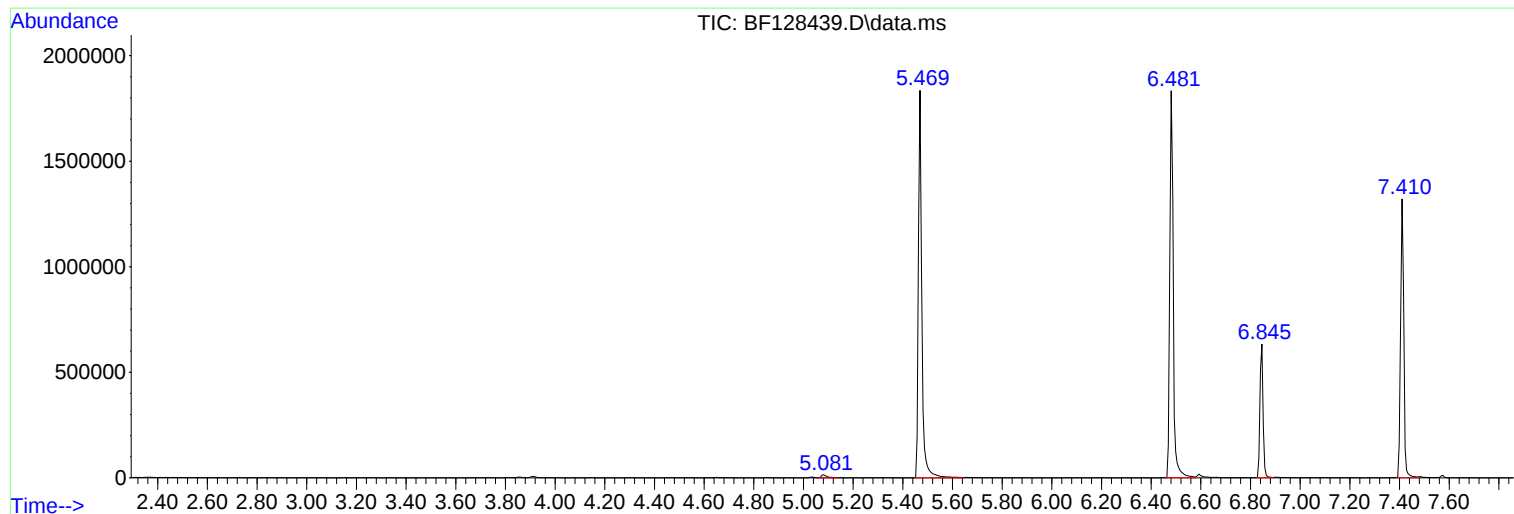

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF052422\
Data File : BF128439.D
Acq On : 24 May 2022 17:15
Operator : CG\JU
Sample : N2874-10
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
P007-SS002-2430-01

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF052022.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF052422\
Data File : BF128439.D
Acq On : 24 May 2022 17:15
Operator : CG\JU
Sample : N2874-10
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
P007-SS002-2430-01

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF052022.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc