

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF052422\
 Data File : BF128448.D
 Acq On : 24 May 2022 21:39
 Operator : CG\JU
 Sample : N2897-06 5X
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 P042-SS001-0006-01

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF052022.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF128448.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.887	268	272	280	rBV	7095	10771	1.39%	0.195%
2	5.469	538	541	560	rBV	267263	306905	39.67%	5.556%
3	6.487	711	714	730	rBV	275654	321718	41.58%	5.824%
4	6.845	771	775	785	rBV	721879	616360	79.67%	11.158%
5	7.410	868	871	881	rBV	235164	202437	26.17%	3.665%
6	8.128	989	993	997	rBV	950908	768775	99.37%	13.917%
7	9.198	1172	1175	1179	rBV	442234	365897	47.29%	6.624%
8	9.886	1288	1292	1295	rBV	969336	773687	100.00%	14.006%
9	10.680	1423	1427	1437	rBV	155619	147521	19.07%	2.671%
10	11.374	1542	1545	1549	rBV	731289	685471	88.60%	12.409%
11	11.751	1607	1609	1612	rBV	19371	16877	2.18%	0.306%
12	11.992	1646	1650	1653	rVB5	12609	12909	1.67%	0.234%
13	12.957	1811	1814	1818	rVB	350274	296281	38.29%	5.364%
14	14.027	1992	1996	2000	rBV	611214	574757	74.29%	10.405%
15	14.115	2009	2011	2014	rBV	32126	30234	3.91%	0.547%
16	15.509	2244	2248	2254	rVB	310725	393221	50.82%	7.119%




Sum of corrected areas: 5523821

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF052422\
Data File : BF128448.D
Acq On : 24 May 2022 21:39
Operator : CG\JU
Sample : N2897-06 5X
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
P042-SS001-0006-01

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF052022.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

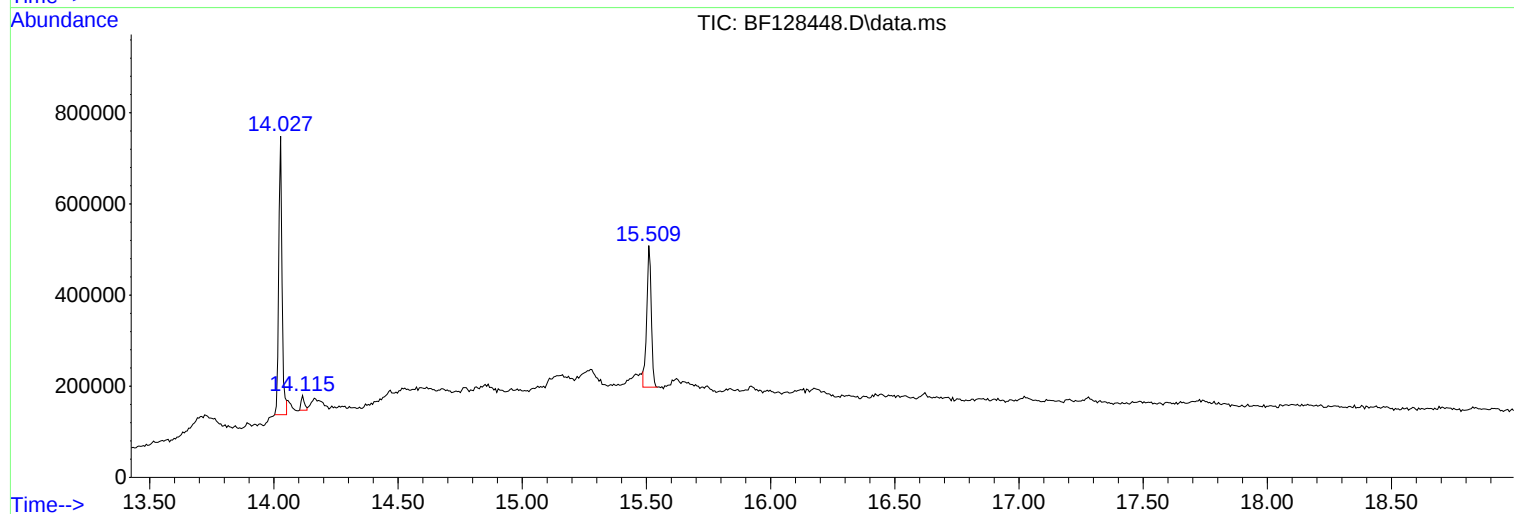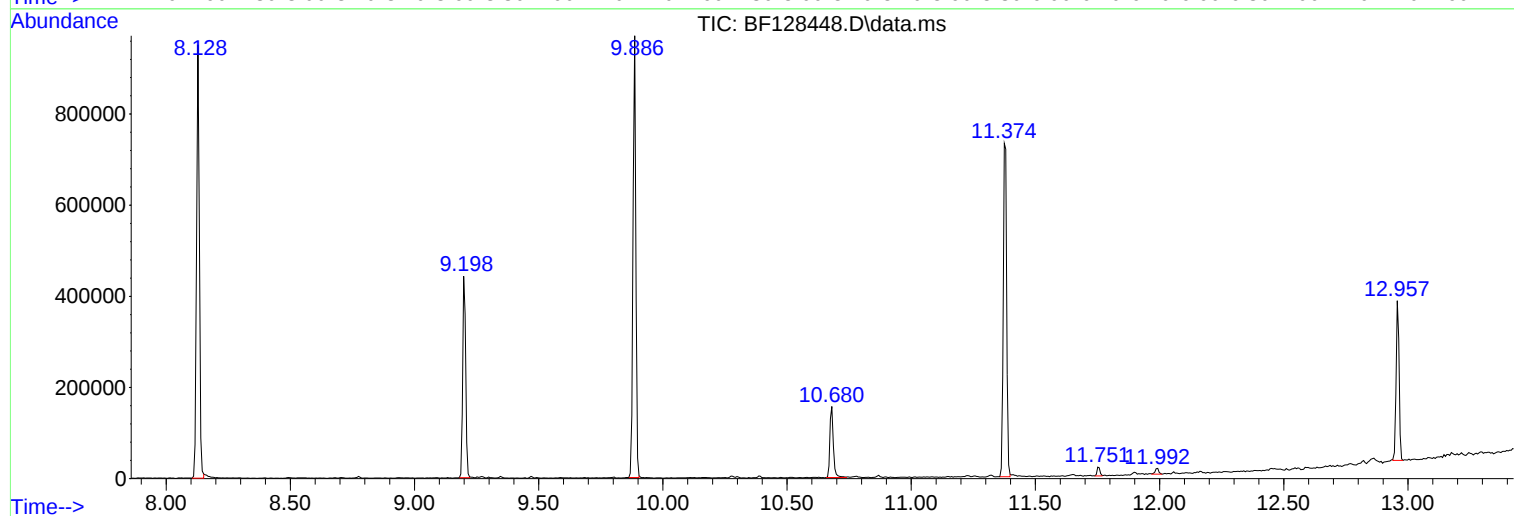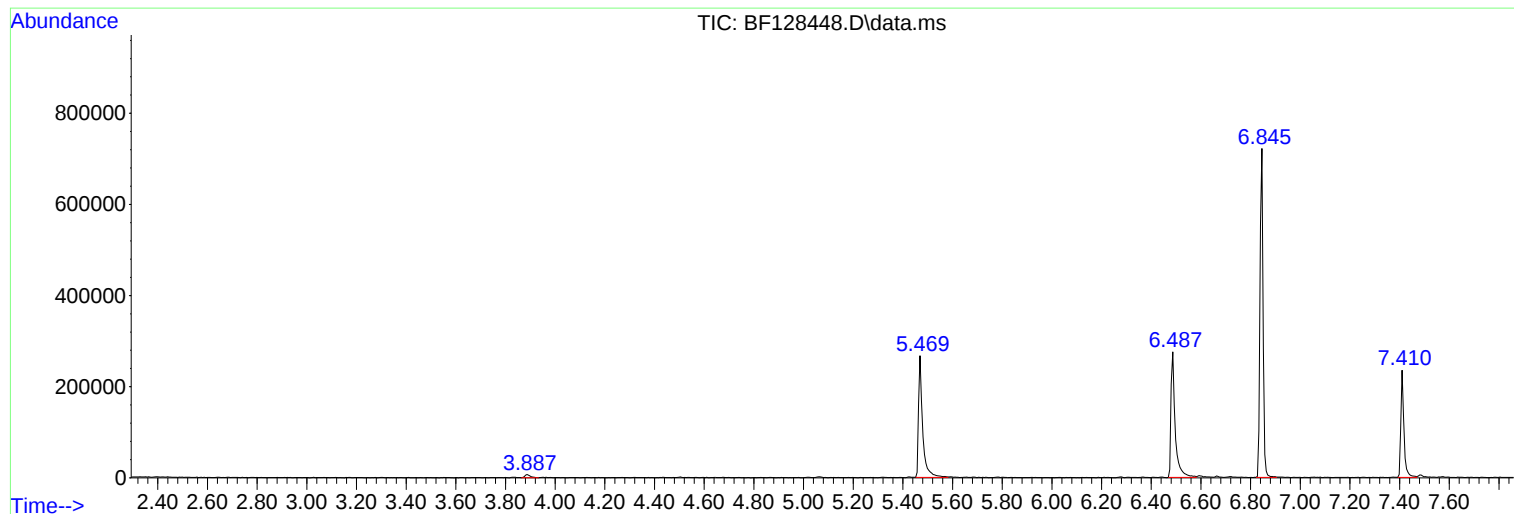

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF052422\
Data File : BF128448.D
Acq On : 24 May 2022 21:39
Operator : CG\JU
Sample : N2897-06 5X
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
P042-SS001-0006-01

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF052022.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF052422\
Data File : BF128448.D
Acq On : 24 May 2022 21:39
Operator : CG\JU
Sample : N2897-06 5X
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
P042-SS001-0006-01

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF052022.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
