

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF052422\
 Data File : BF128449.D
 Acq On : 24 May 2022 22:08
 Operator : CG\JU
 Sample : N2896-14 5X
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 P039-SS001-1218-01

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF052022.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF128449.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.893	268	273	279	rBV2	6582	10027	1.28%	0.173%
2	5.469	538	541	559	rBV	326626	375170	47.98%	6.457%
3	6.487	710	714	731	rBV	327230	390095	49.89%	6.714%
4	6.846	771	775	784	rBV	735278	621978	79.55%	10.705%
5	7.410	868	871	882	rBV	290310	248710	31.81%	4.281%
6	8.128	989	993	997	rBV	980946	773819	98.96%	13.318%
7	9.198	1172	1175	1179	rBV	539605	443405	56.71%	7.632%
8	9.886	1288	1292	1295	rBV	936847	781912	100.00%	13.458%
9	10.681	1423	1427	1435	rBV	184712	173209	22.15%	2.981%
10	11.375	1542	1545	1549	rBV	768470	710136	90.82%	12.222%
11	12.957	1811	1814	1818	rBV	431580	349835	44.74%	6.021%
12	14.027	1992	1996	1999	rBV	566287	517280	66.16%	8.903%
13	14.116	2008	2011	2014	rVB	33135	27710	3.54%	0.477%
14	15.510	2244	2248	2253	rVB2	303894	386854	49.48%	6.658%




Sum of corrected areas: 5810140

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF052422\
Data File : BF128449.D
Acq On : 24 May 2022 22:08
Operator : CG\JU
Sample : N2896-14 5X
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
P039-SS001-1218-01

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF052022.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

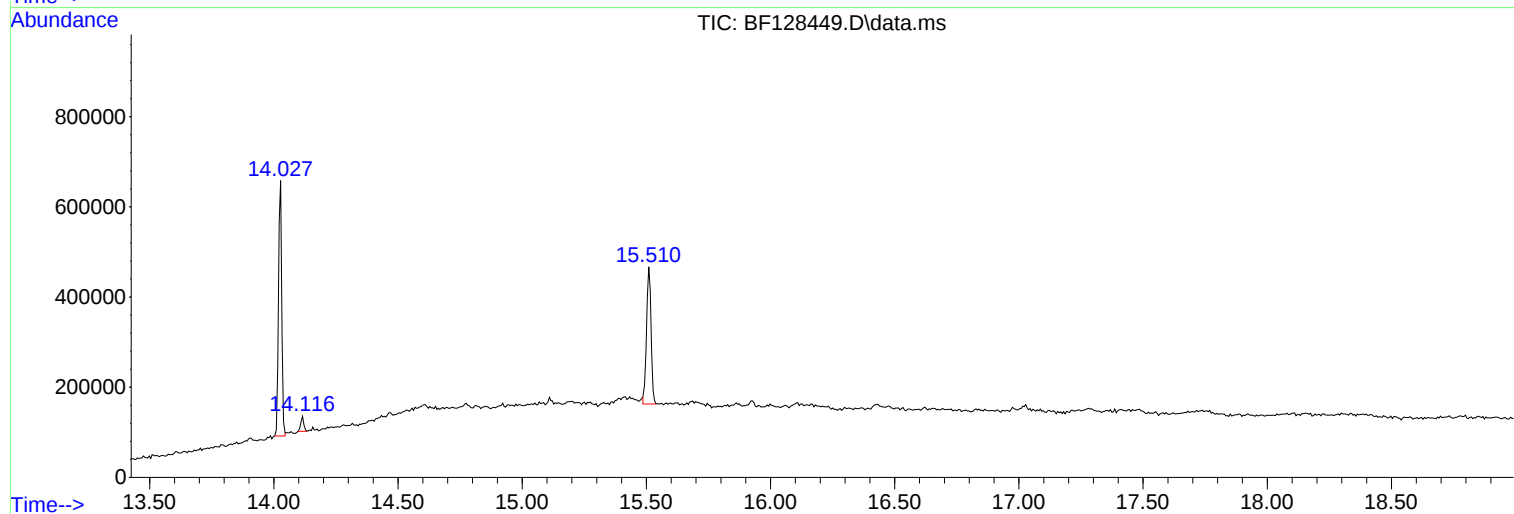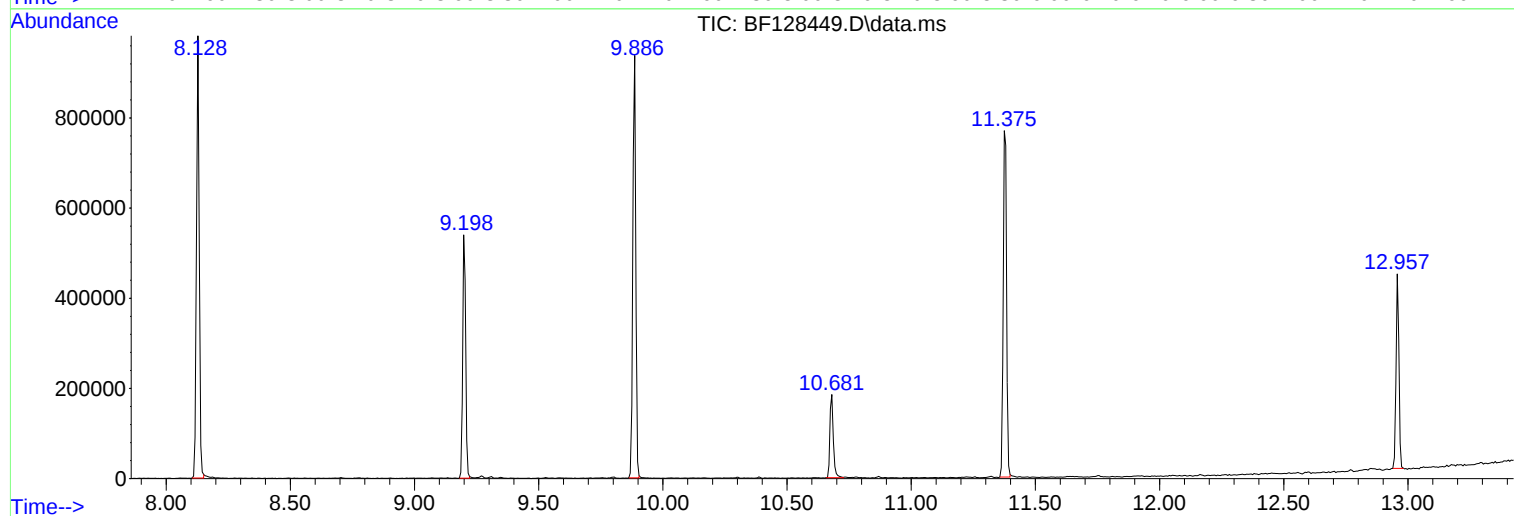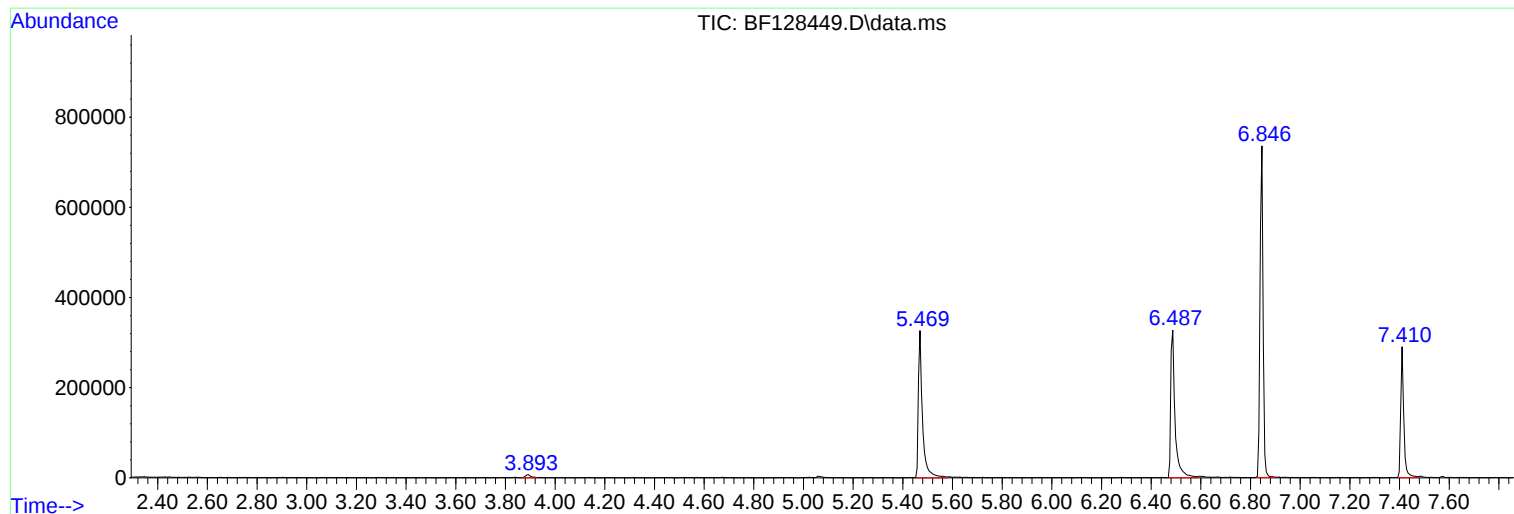

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF052422\
Data File : BF128449.D
Acq On : 24 May 2022 22:08
Operator : CG\JU
Sample : N2896-14 5X
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
P039-SS001-1218-01

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF052022.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF052422\
Data File : BF128449.D
Acq On : 24 May 2022 22:08
Operator : CG\JU
Sample : N2896-14 5X
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
P039-SS001-1218-01

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF052022.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------