

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF052422\
 Data File : BF128450.D
 Acq On : 24 May 2022 22:37
 Operator : CG\JU
 Sample : N2896-12 10X
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 P039-SS001-0006-01

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF052022.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF128450.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.887	268	272	279	rBV2	6617	10542	1.37%	0.228%
2	5.475	538	542	557	rBV	114559	155184	20.20%	3.354%
3	6.487	712	714	730	rBV	124330	166003	21.61%	3.588%
4	6.845	771	775	786	rBV	723804	604078	78.64%	13.057%
5	7.410	868	871	877	rBV	112261	103570	13.48%	2.239%
6	8.051	976	980	985	rBV	27556	28609	3.72%	0.618%
7	8.128	989	993	997	rBV	968124	755586	98.36%	16.332%
8	9.198	1172	1175	1179	rBV	256662	197718	25.74%	4.274%
9	9.886	1288	1292	1295	rBV	949647	768200	100.00%	16.605%
10	10.681	1424	1427	1434	rVB	78435	69485	9.05%	1.502%
11	11.375	1542	1545	1549	rBV	775939	677178	88.15%	14.637%
12	12.957	1811	1814	1818	rBV	199689	163541	21.29%	3.535%
13	14.027	1992	1996	1999	rBV	584647	524184	68.24%	11.330%
14	14.116	2009	2011	2014	rVB	33270	24156	3.14%	0.522%
15	15.510	2244	2248	2256	rVB	301666	378368	49.25%	8.178%




Sum of corrected areas: 4626402

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF052422\
Data File : BF128450.D
Acq On : 24 May 2022 22:37
Operator : CG\JU
Sample : N2896-12 10X
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
P039-SS001-0006-01

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF052022.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

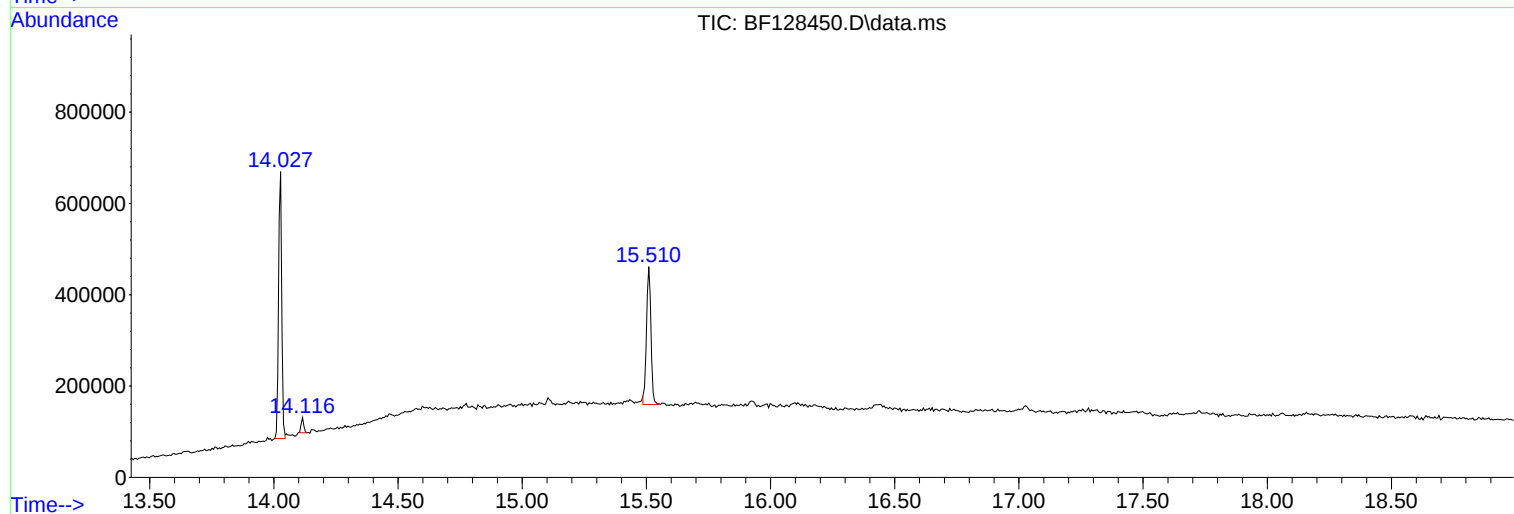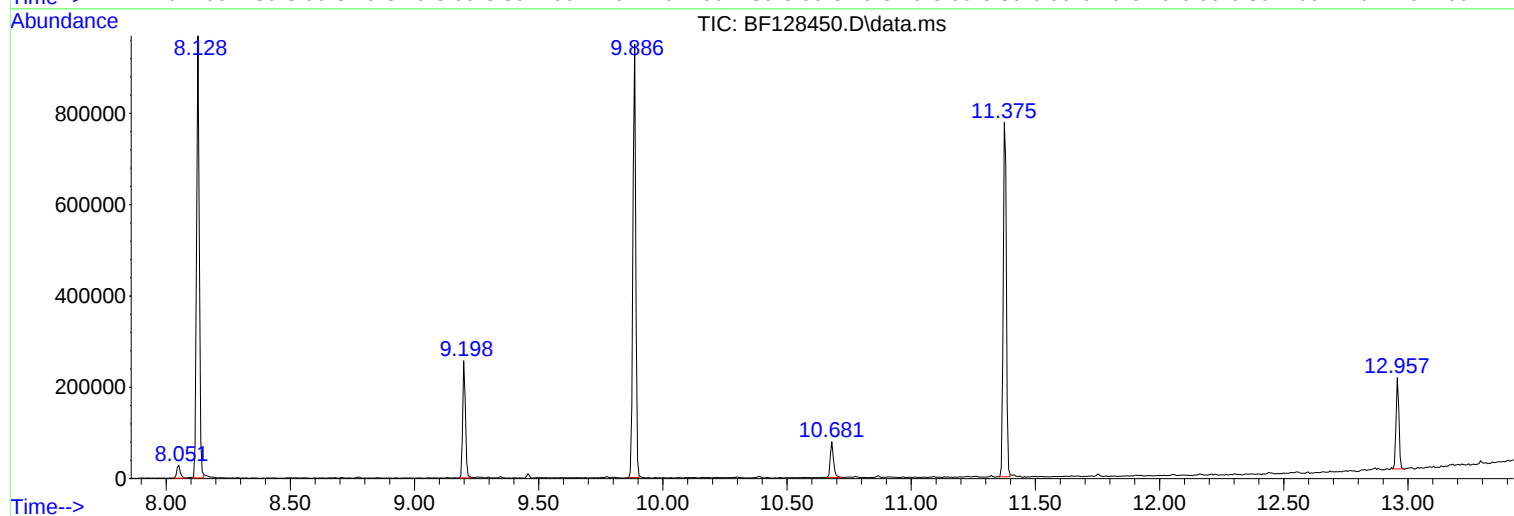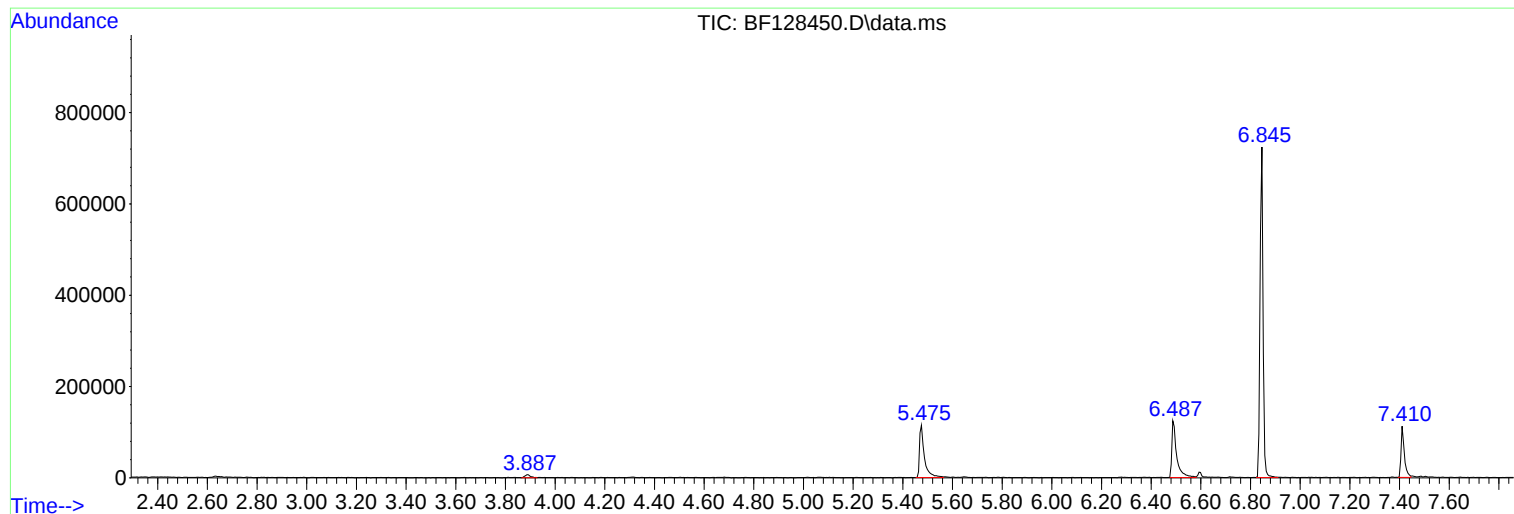

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF052422\
Data File : BF128450.D
Acq On : 24 May 2022 22:37
Operator : CG\JU
Sample : N2896-12 10X
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
P039-SS001-0006-01

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF052022.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF052422\
Data File : BF128450.D
Acq On : 24 May 2022 22:37
Operator : CG\JU
Sample : N2896-12 10X
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
P039-SS001-0006-01

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF052022.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------