
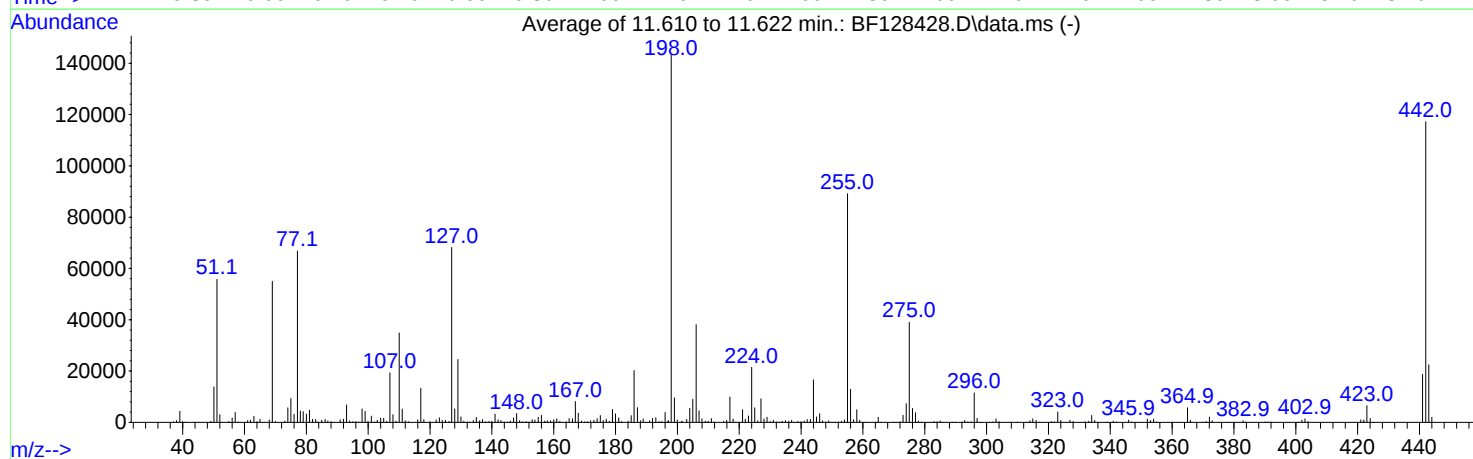


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF052422\
 Data File : BF128428.D
 Acq On : 24 May 2022 11:18
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF052022.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed May 25 12:38:46 2022

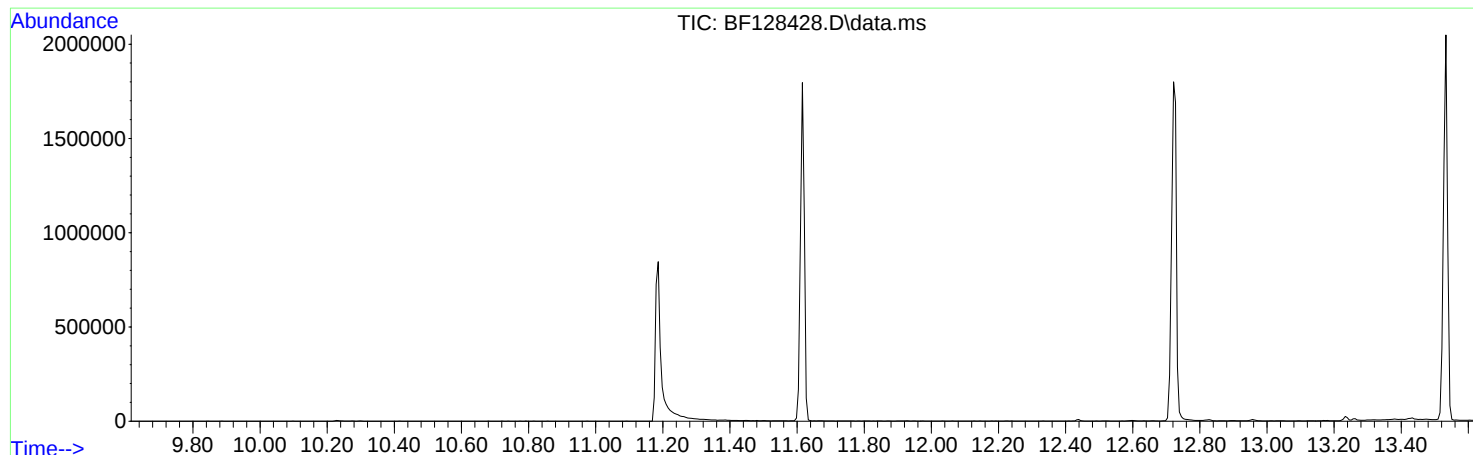




AutoFind: Scans 1585, 1586, 1587; Background Corrected with Scan 1579

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	38.9	55805	PASS
68	69	0.00	2	1.7	951	PASS
69	198	0.00	100	38.4	55051	PASS
70	69	0.00	2	0.5	299	PASS
127	198	10	80	47.6	68211	PASS
197	198	0.00	2	0.5	670	PASS
198	198	100	100	100.0	143421	PASS
199	198	5	9	6.7	9570	PASS
275	198	10	60	27.2	39019	PASS
365	198	1	100	4.0	5686	PASS
441	198	0.01	100	13.1	18750	PASS
442	442	50	100	100.0	117216	PASS
443	442	15	24	19.2	22474	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF052422\
Data File : BF128428.D
Acq On : 24 May 2022 11:18
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: May 25 07:33:27 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF052022.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed May 25 03:52:53 2022
Response via : Initial Calibration

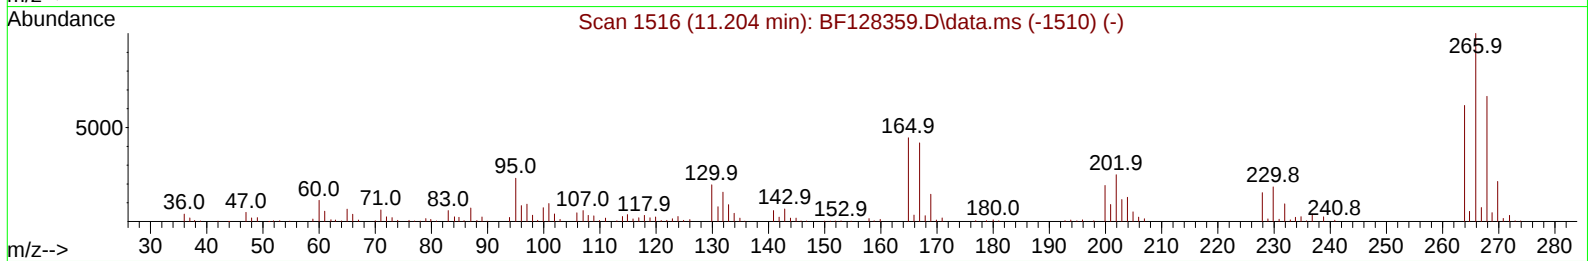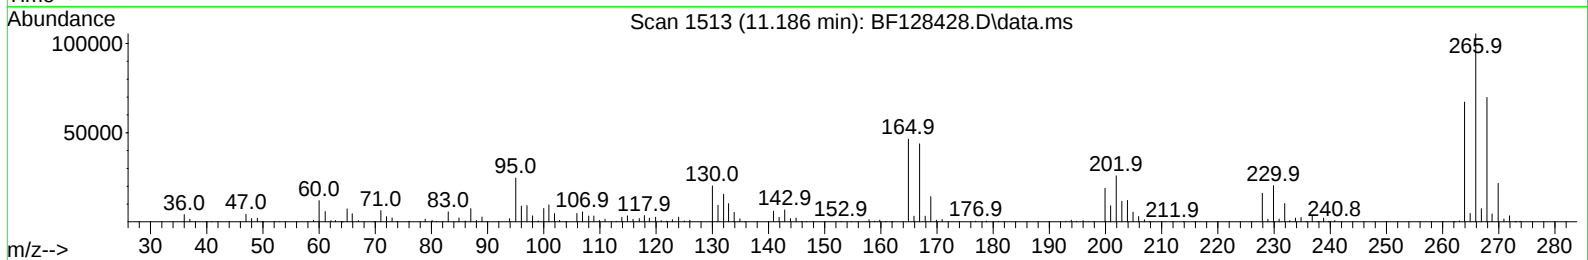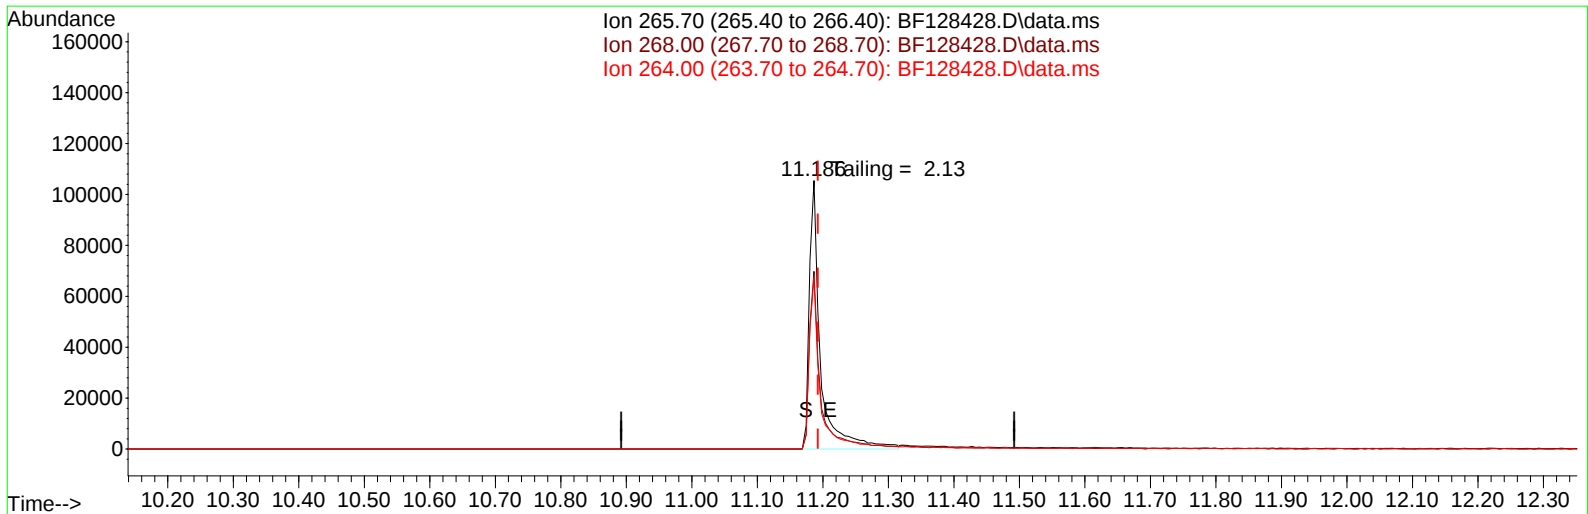

TIC: BF128428.D\data.ms

(70) Pentachlorophenol (C)

11.186min (-0.006) 63259.70 ng




response 128753

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	66.30	66.19
264.00	66.40	63.70
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF052422\
 Data File : BF128428.D
 Acq On : 24 May 2022 11:18
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Quant Time: May 25 07:33:27 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF052022.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed May 25 03:52:53 2022
 Response via : Initial Calibration

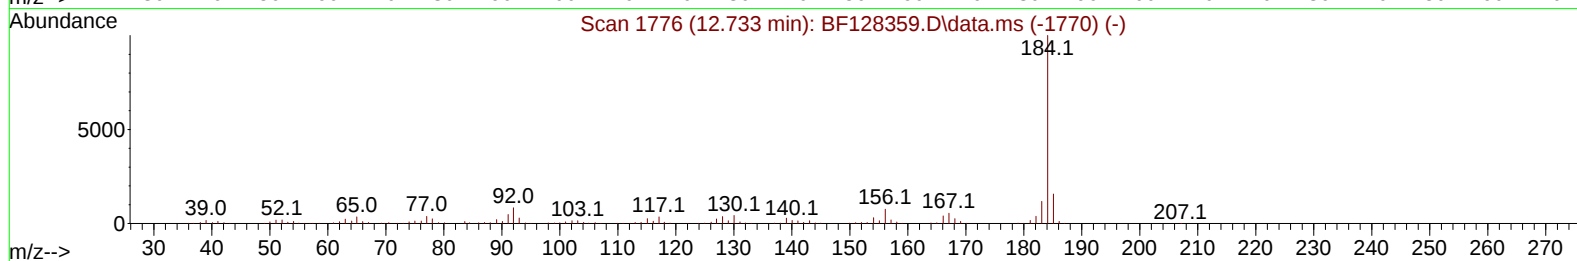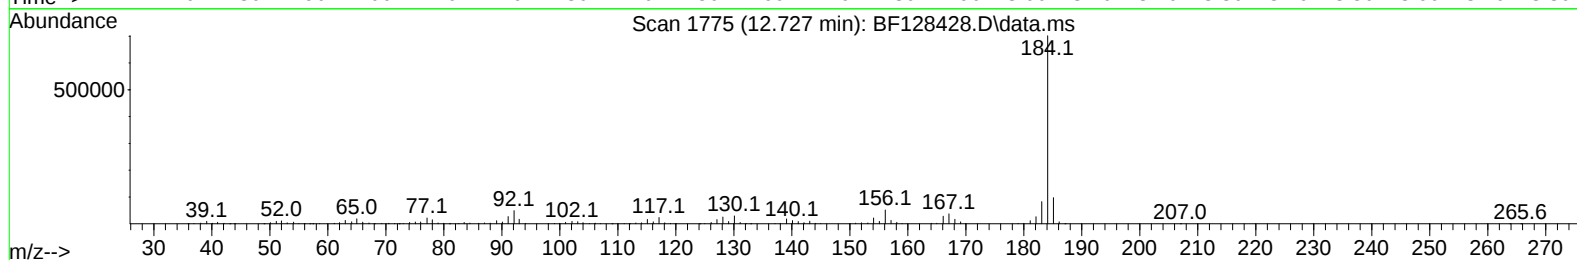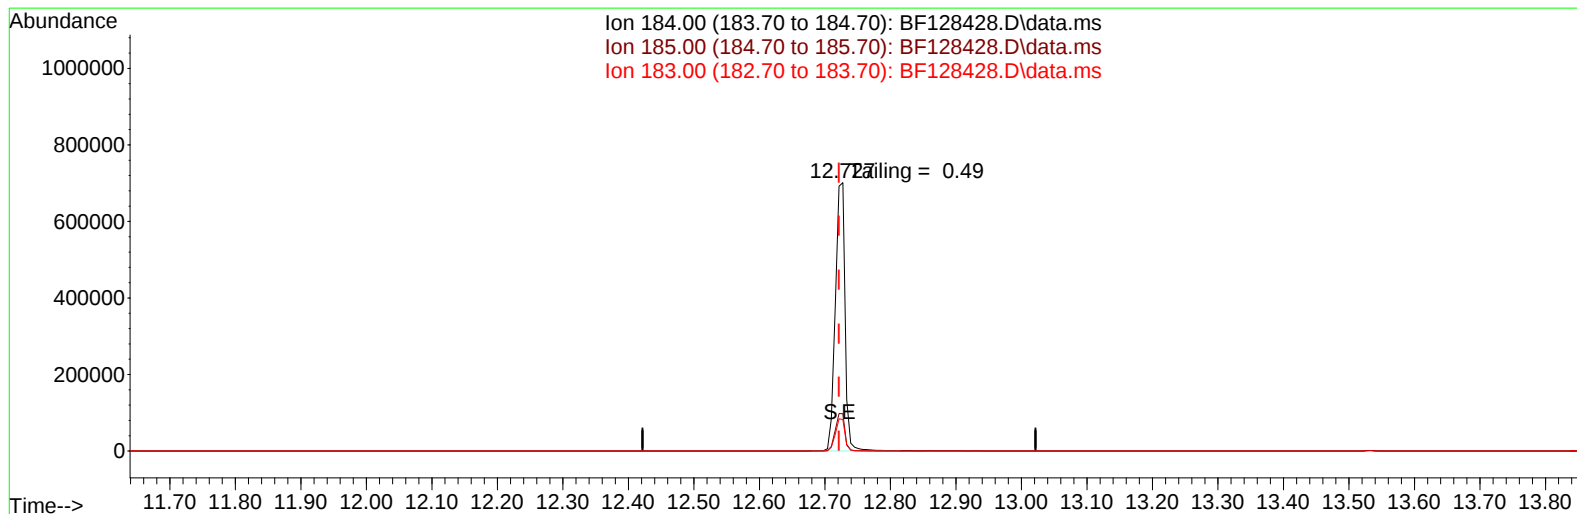

TIC: BF128428.D\data.ms

(77) Benzidine

12.727min (+ 0.006) 44273.37 ng

response 727453

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.10	13.93
183.00	11.20	11.74
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
5/24/2022	BNA_F	<u>BF128428.D</u>
Compound Name	Response	Retention Time
DDT	332889	13.533
DDD	7116	13.233
DDE	822	12.892
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
7938	340827	2.33

Instrument :
BNA_F
ClientSampleId :
DFTPP