
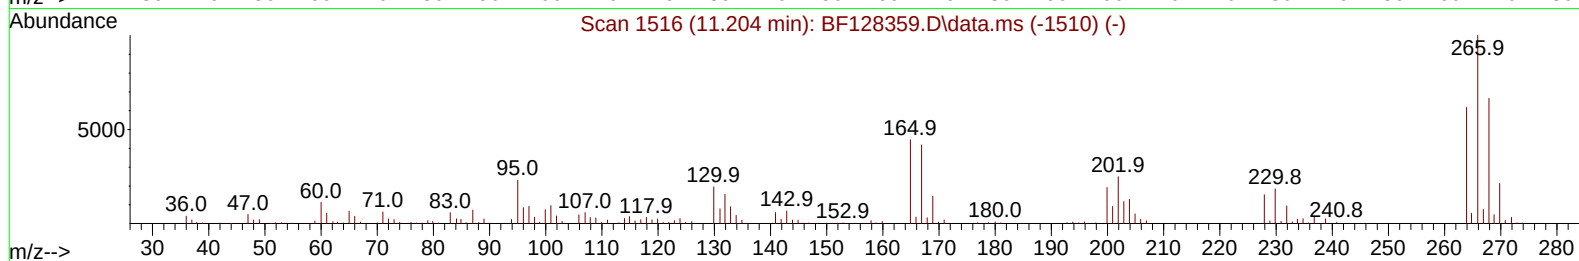
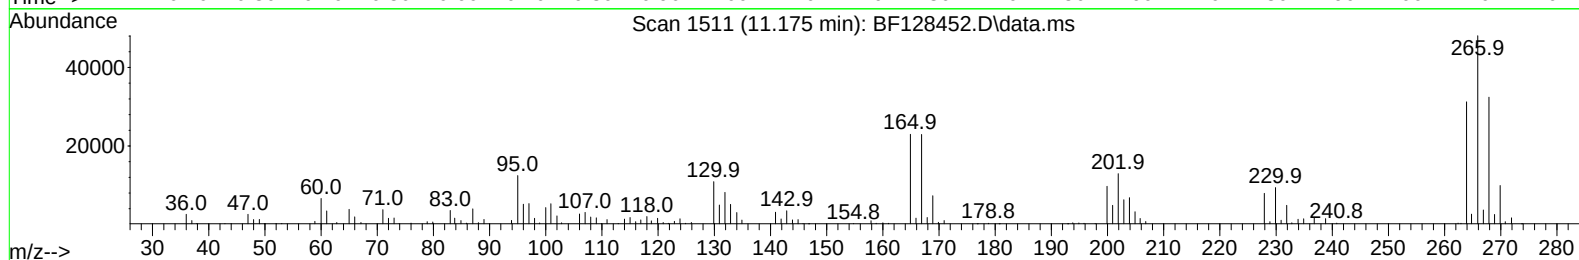


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF052522\
Data File : BF128452.D
Acq On : 25 May 2022 10:44
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 26 06:01:11 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF052022.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu May 26 06:01:06 2022
Response via : Initial Calibration

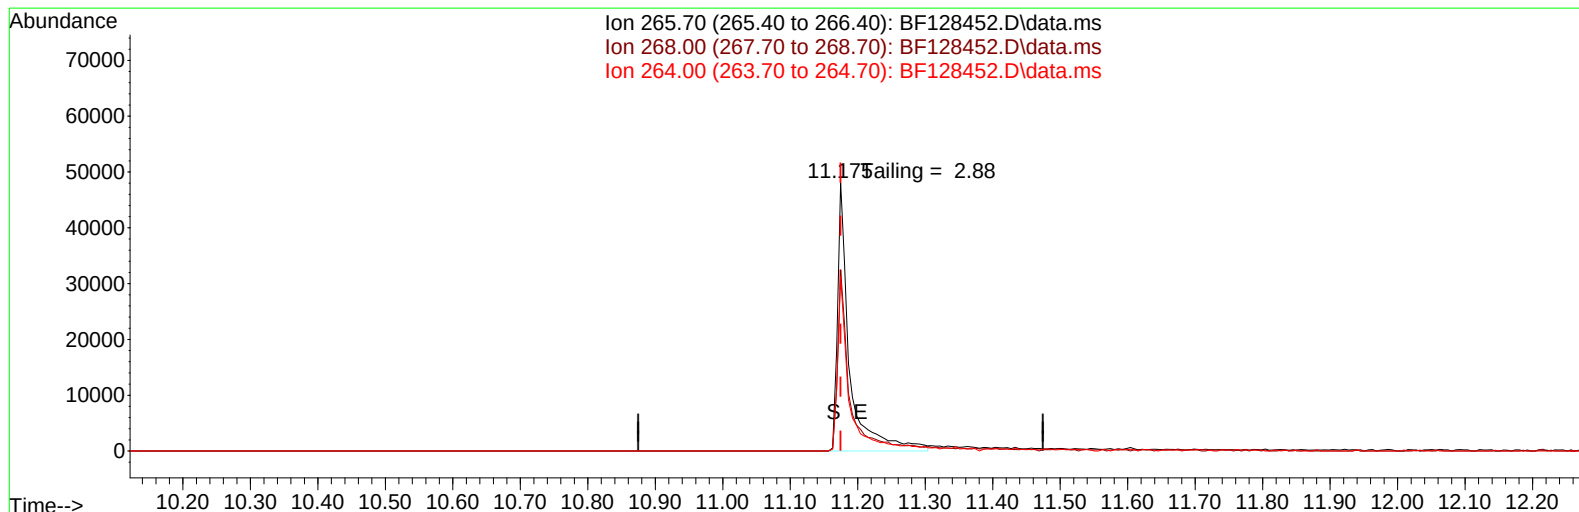

TIC: BF128452.D\data.ms

(70) Pentachlorophenol (C)




11.175min (0.000) 43187.79 ng

response 58070

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	66.30	67.47
264.00	66.40	64.95
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF052522\
Data File : BF128452.D
Acq On : 25 May 2022 10:44
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 26 06:01:11 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF052022.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu May 26 06:01:06 2022
Response via : Initial Calibration

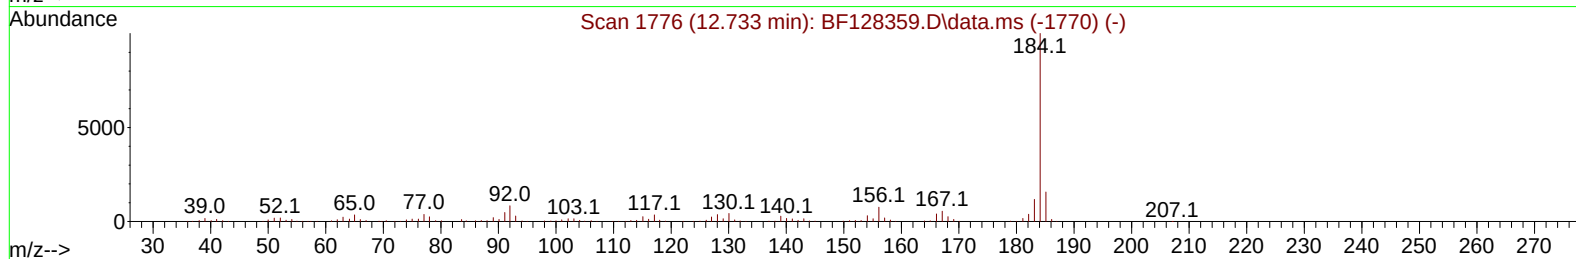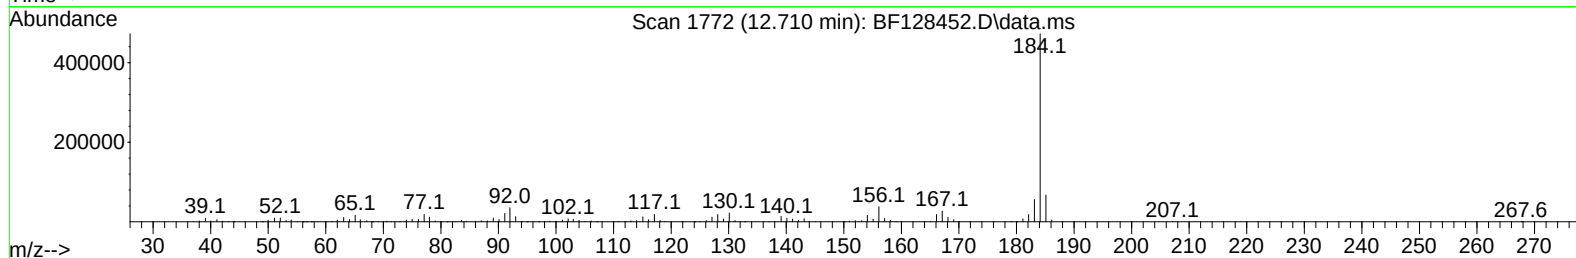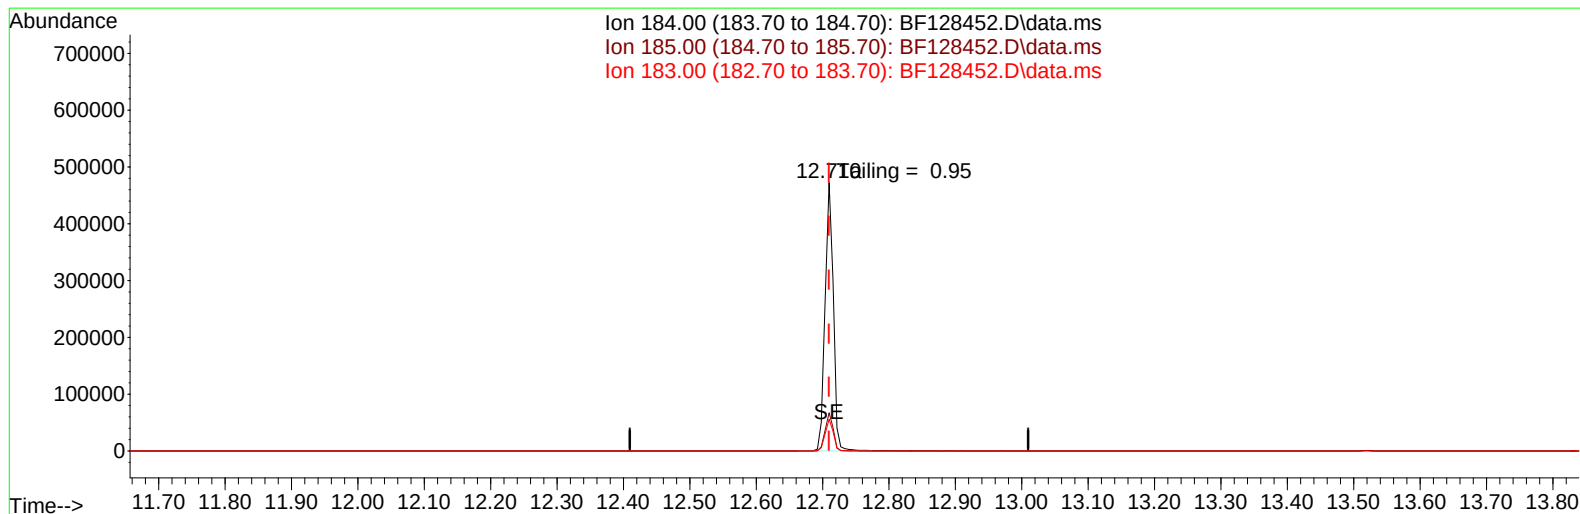

TIC: BF128452.D\data.ms

(77) Benzidine

12.710min (0.000) 58763.38 ng

response 410659

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.10	14.25
183.00	11.20	11.85
0.00	0.00	0.00