

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF052522\
 Data File : BF128463.D
 Acq On : 25 May 2022 16:54
 Operator : CG\JU
 Sample : N2897-09
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 P042-SS001-1824-01

Quant Time: May 26 01:01:11 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF052022.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed May 25 12:38:46 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	6.810	152	86737	20.000	ng	0.00
21) Naphthalene-d8	8.092	136	296167	20.000	ng	0.00
39) Acenaphthene-d10	9.845	164	136042	20.000	ng	0.00
64) Phenanthrene-d10	11.339	188	210470	20.000	ng	0.00
76) Chrysene-d12	13.986	240	171898	20.000	ng	# 0.00
86) Perylene-d12	15.457	264	126379	20.000	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.434	112	445968	81.822	ng	0.00
7) Phenol-d6	6.451	99	554251	77.225	ng	0.00
23) Nitrobenzene-d5	7.375	82	370013	55.977	ng	0.00
42) 2,4,6-Tribromophenol	10.639	330	97281	69.338	ng	0.00
45) 2-Fluorobiphenyl	9.163	172	535006	64.312	ng	0.00
79) Terphenyl-d14	12.921	244	479256	53.821	ng	0.00


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF052522\
Data File : BF128463.D
Acq On : 25 May 2022 16:54
Operator : CG\JU
Sample : N2897-09
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
P042-SS001-1824-01

Quant Time: May 26 01:01:11 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF052022.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed May 25 12:38:46 2022
Response via : Initial Calibration




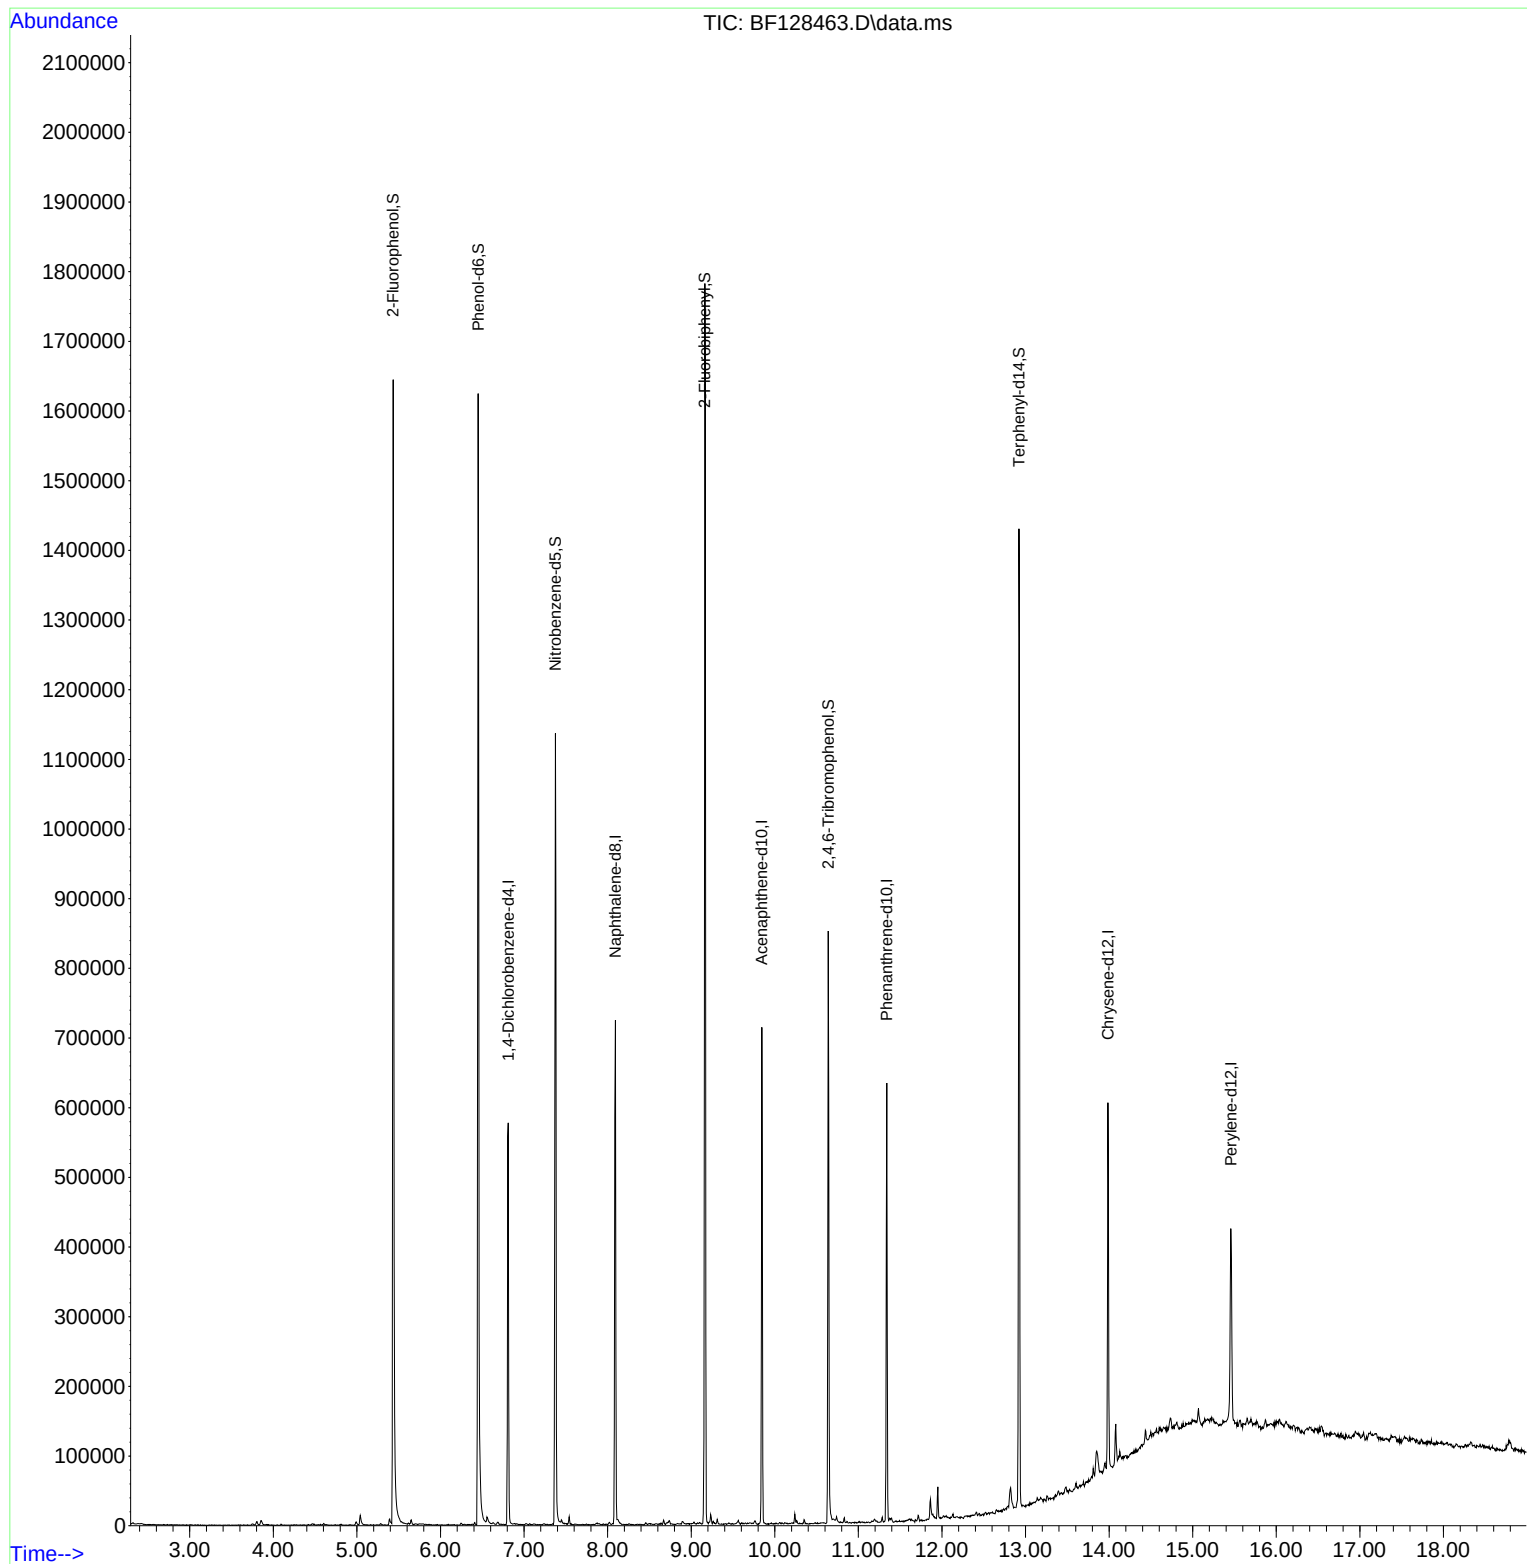


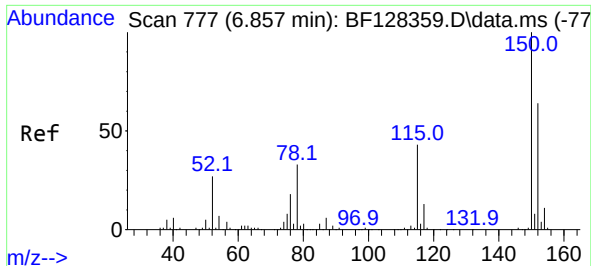

#1
1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 6.810 min Scan# 70
Delta R.T. 0.000 min
Lab File: BF128463.D
Acq: 25 May 2022 16:54




Instrument :
BNA_F
ClientSampleId :
P042-SS001-1824-01


Tgt Ion:152 Resp: 86737
Ion Ratio Lower Upper
152 100
150 152.3 125.3 187.9
115 62.0 48.8 73.2

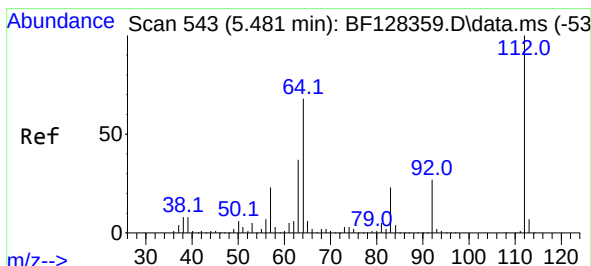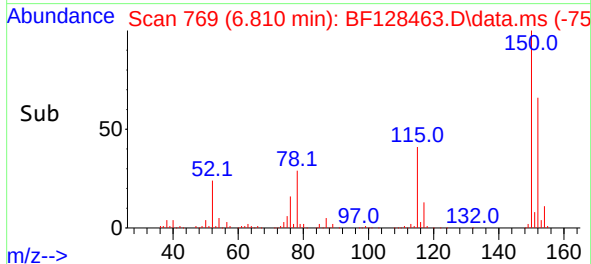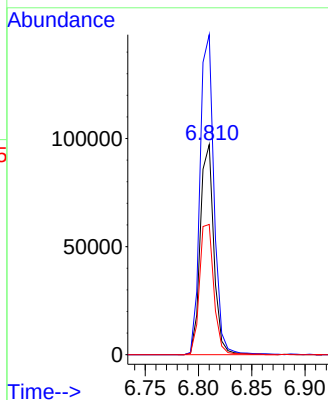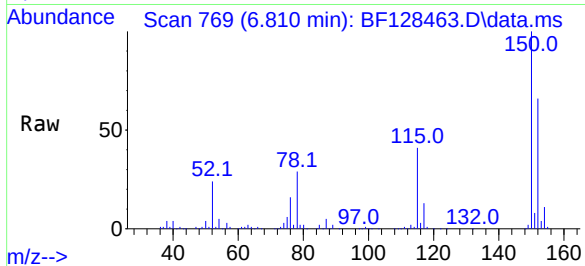

#5
2-Fluorophenol
Concen: 81.822 ng
RT: 5.434 min Scan# 535
Delta R.T. -0.000 min
Lab File: BF128463.D
Acq: 25 May 2022 16:54

Tgt Ion:112 Resp: 445968
Ion Ratio Lower Upper
112 100
64 65.2 49.5 74.3
63 35.4 26.3 39.5


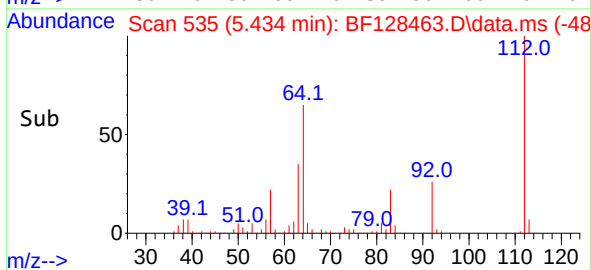
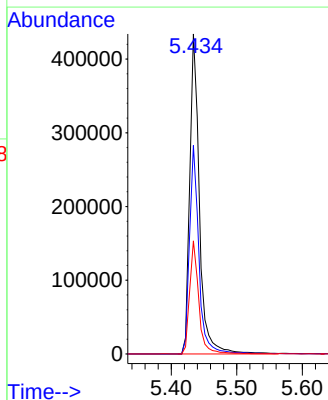
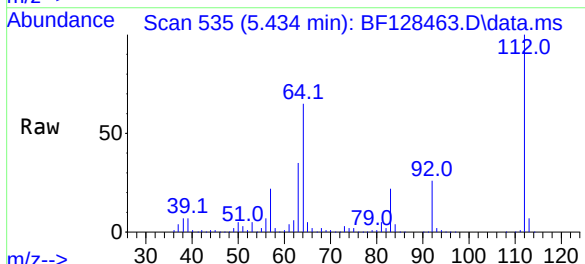


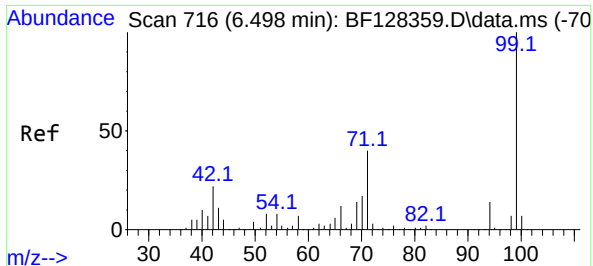

#7
Phenol-d6
Concen: 77.225 ng
RT: 6.451 min Scan# 70
Delta R.T. -0.006 min
Lab File: BF128463.D
Acq: 25 May 2022 16:54




Instrument :
BNA_F
ClientSampleId :
P042-SS001-1824-01


Tgt Ion: 99 Resp: 554251
Ion Ratio Lower Upper
99 100
42 21.1 16.6 24.8
71 38.9 30.0 45.0

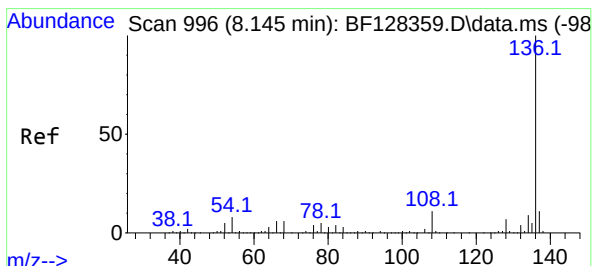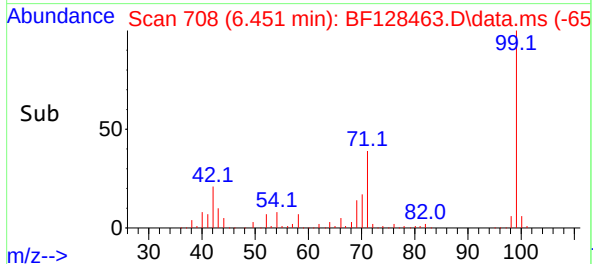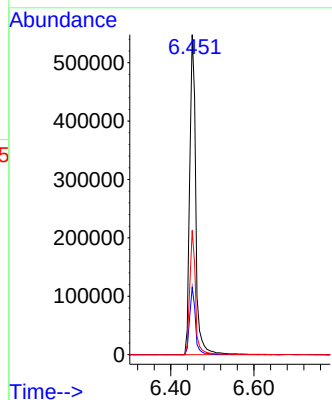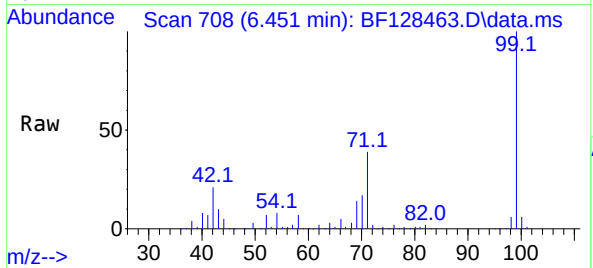

#21
Naphthalene-d8
Concen: 20.000 ng
RT: 8.092 min Scan# 987
Delta R.T. -0.000 min
Lab File: BF128463.D
Acq: 25 May 2022 16:54

Tgt Ion: 136 Resp: 296167
Ion Ratio Lower Upper
136 100
137 10.8 8.6 13.0
54 7.7 6.8 10.2
68 6.0 5.1 7.7


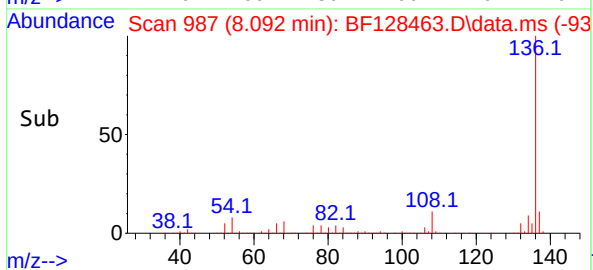
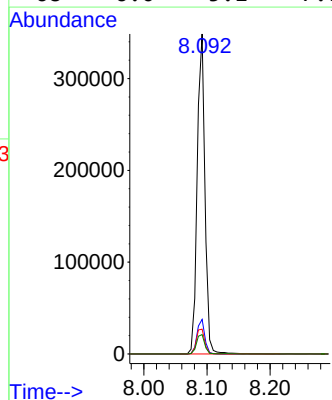
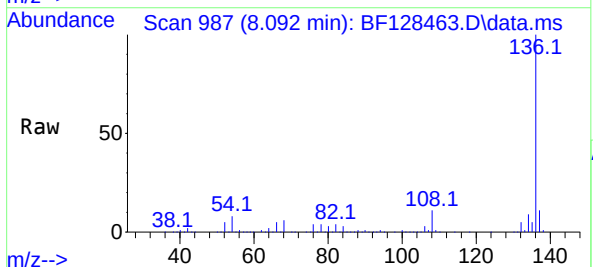


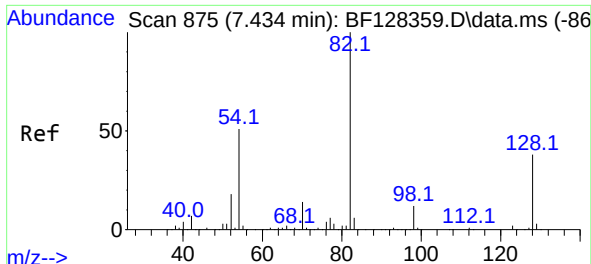

#23
Nitrobenzene-d5
Concen: 55.977 ng
RT: 7.375 min Scan# 80
Delta R.T. -0.006 min
Lab File: BF128463.D
Acq: 25 May 2022 16:54




Instrument :
BNA_F
ClientSampleId :
P042-SS001-1824-01


Tgt Ion: 82 Resp: 370013
Ion Ratio Lower Upper
82 100
128 38.3 30.0 45.0
54 52.0 41.3 61.9

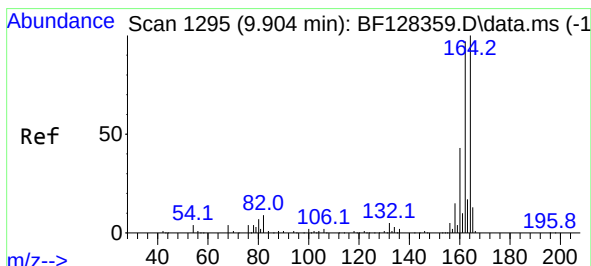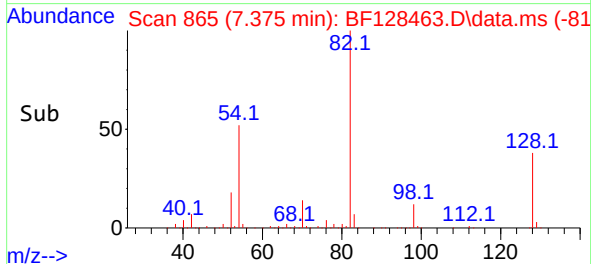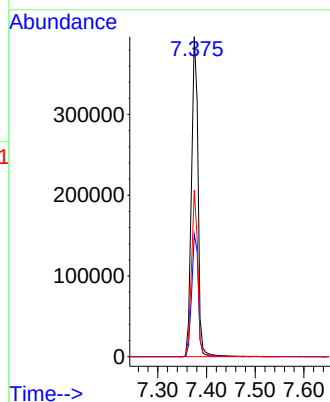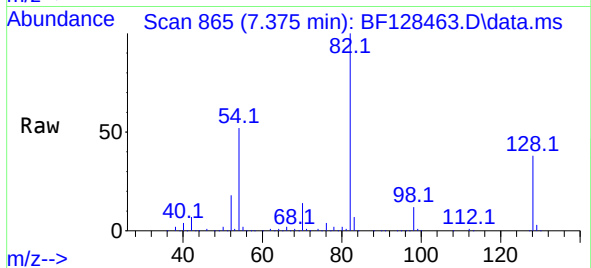

#39
Acenaphthene-d10
Concen: 20.000 ng
RT: 9.845 min Scan# 1285
Delta R.T. -0.006 min
Lab File: BF128463.D
Acq: 25 May 2022 16:54


Tgt Ion:164 Resp: 136042
Ion Ratio Lower Upper
164 100
162 95.2 76.0 114.0
160 42.8 34.8 52.2

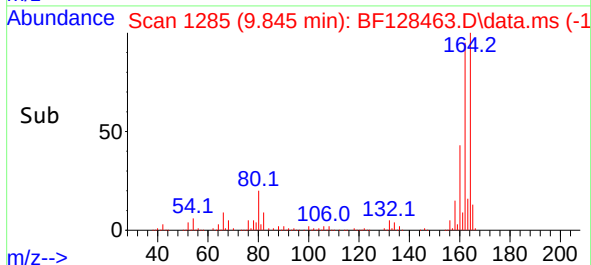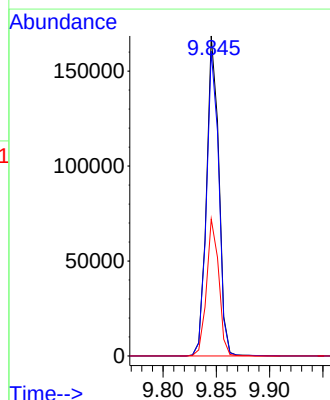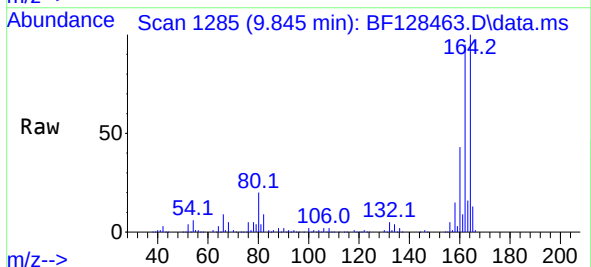



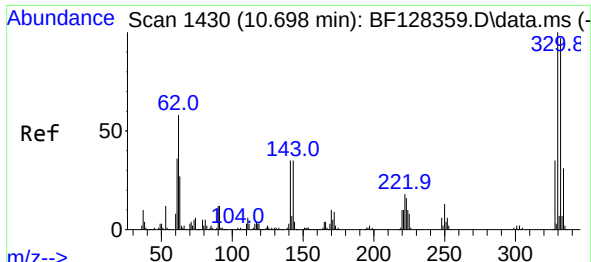


#42
2,4,6-Tribromophenol
Concen: 69.338 ng
RT: 10.639 min Scan# 14
Delta R.T. -0.006 min
Lab File: BF128463.D
Acq: 25 May 2022 16:54

Instrument :
BNA_F
ClientSampleId :
P042-SS001-1824-01



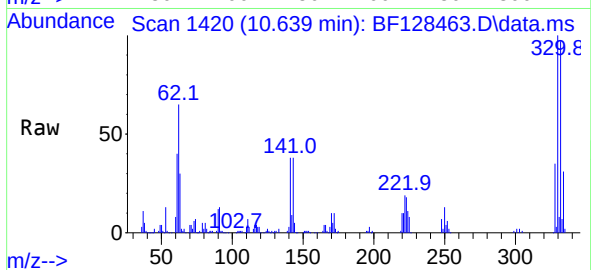



Tgt Ion:330 Resp: 97281
Ion Ratio Lower Upper
330 100
332 95.5 79.0 118.4
141 33.1 28.9 43.3

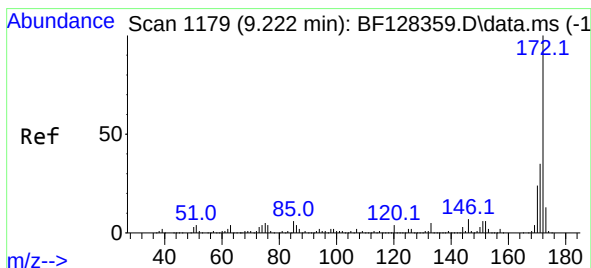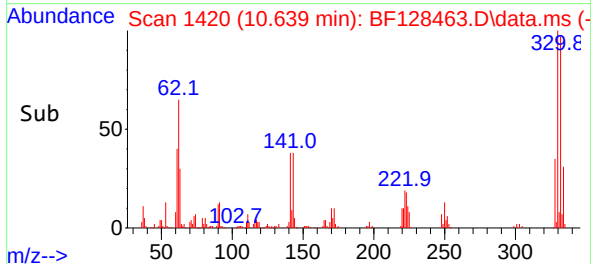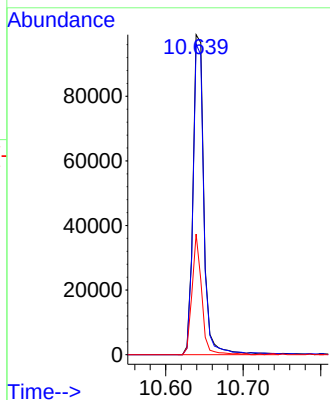

#45
2-Fluorobiphenyl
Concen: 64.312 ng
RT: 9.163 min Scan# 1169
Delta R.T. -0.006 min
Lab File: BF128463.D
Acq: 25 May 2022 16:54

Tgt Ion:172 Resp: 535006
Ion Ratio Lower Upper
172 100
171 35.2 28.6 42.8
170 24.3 19.1 28.7


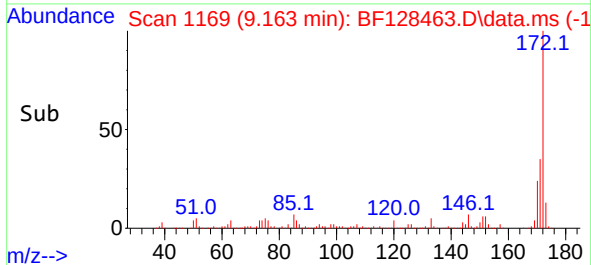
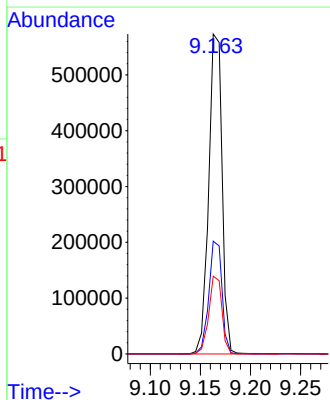
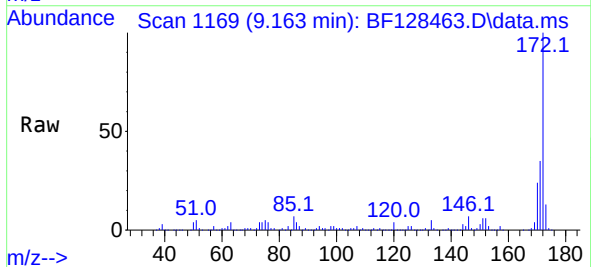


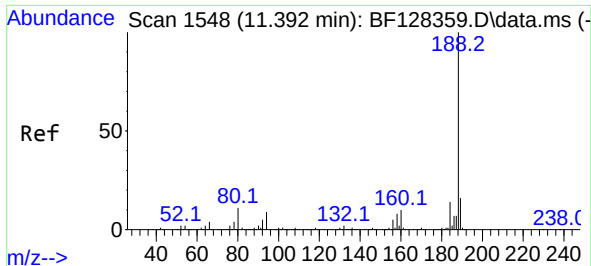

#64
Phenanthrene-d10
Concen: 20.000 ng
RT: 11.339 min Scan# 11
Delta R.T. -0.000 min
Lab File: BF128463.D
Acq: 25 May 2022 16:54




Instrument :
BNA_F
ClientSampleId :
P042-SS001-1824-01


Tgt Ion:188 Resp: 210470
Ion Ratio Lower Upper
188 100
94 8.6 8.0 12.0
80 9.8 8.9 13.3

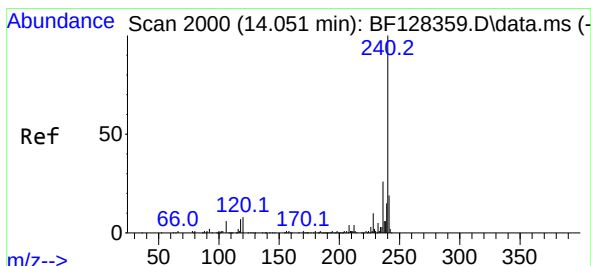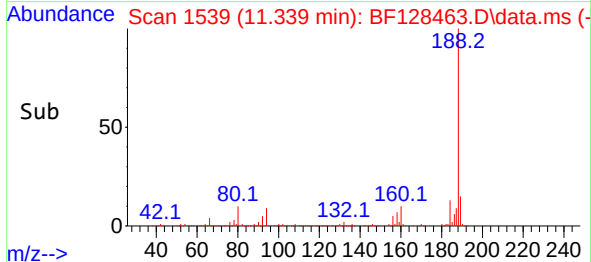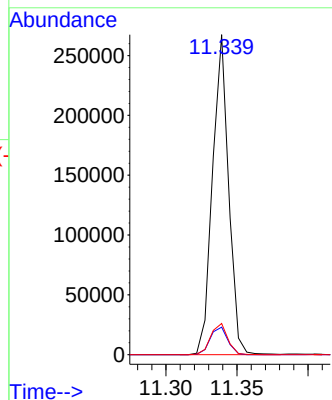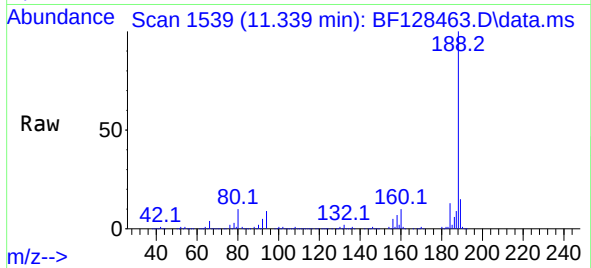

#76
Chrysene-d12
Concen: 20.000 ng
RT: 13.986 min Scan# 1989
Delta R.T. -0.006 min
Lab File: BF128463.D
Acq: 25 May 2022 16:54


Tgt Ion:240 Resp: 171898
Ion Ratio Lower Upper
240 100
120 11.1 7.0 10.6#
236 26.0 20.3 30.5

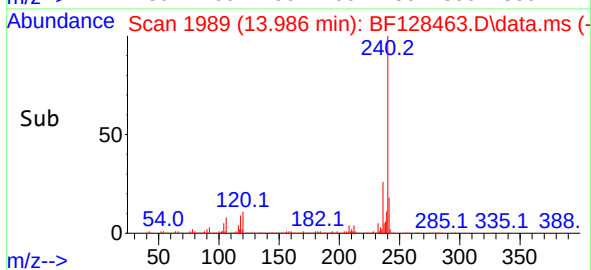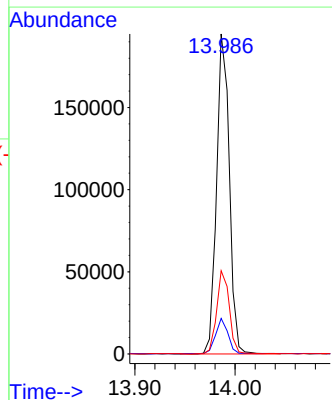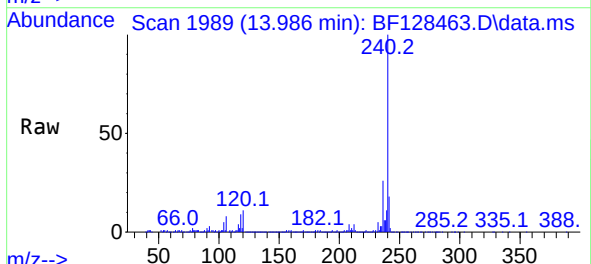



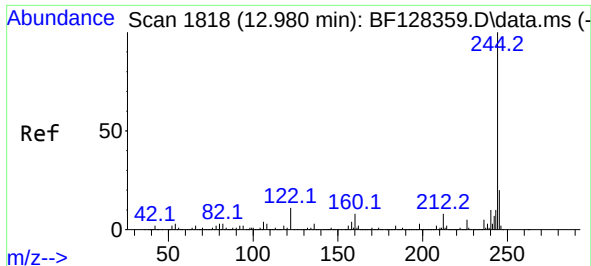


#79
Terphenyl-d14
Concen: 53.821 ng
RT: 12.921 min Scan# 1808
Delta R.T. -0.006 min
Lab File: BF128463.D
Acq: 25 May 2022 16:54

Instrument :
BNA_F
ClientSampleId :
P042-SS001-1824-01

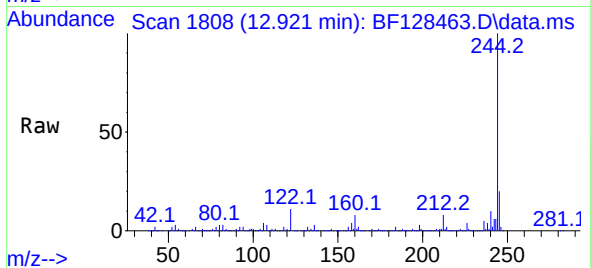

Tgt Ion:244 Resp: 479256
Ion Ratio Lower Upper
244 100
212 7.6 6.2 9.4
122 11.1 8.6 12.8

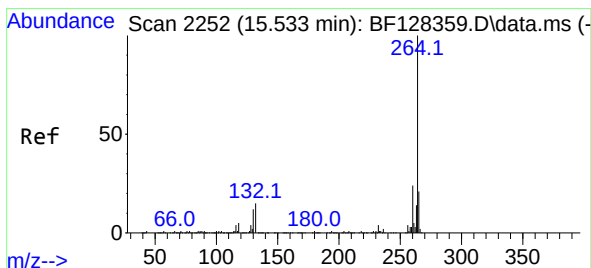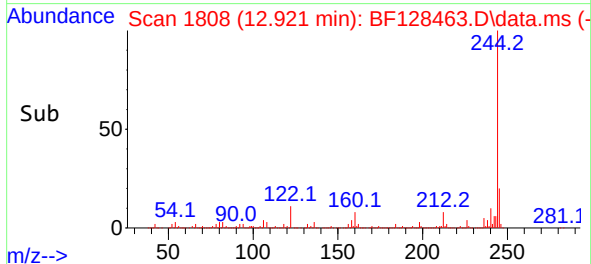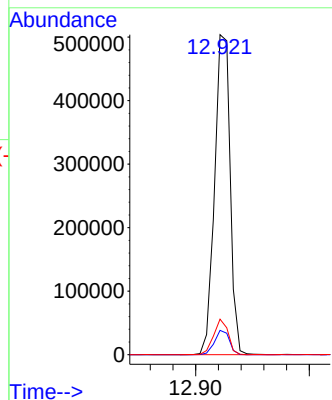

#86
Perylene-d12
Concen: 20.000 ng
RT: 15.457 min Scan# 2239
Delta R.T. -0.000 min
Lab File: BF128463.D
Acq: 25 May 2022 16:54

Tgt Ion:264 Resp: 126379
Ion Ratio Lower Upper
264 100
260 23.3 20.1 30.1
265 21.3 17.5 26.3

