

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF052522\
 Data File : BF128465.D
 Acq On : 25 May 2022 17:52
 Operator : CG\JU
 Sample : N2894-09
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 P004-SS006-0006-01

Quant Time: May 26 01:01:24 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF052022.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed May 25 12:38:46 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	6.810	152	78705	20.000	ng	0.00
21) Naphthalene-d8	8.092	136	268492	20.000	ng	0.00
39) Acenaphthene-d10	9.845	164	127625	20.000	ng	0.00
64) Phenanthrene-d10	11.339	188	209556	20.000	ng	0.00
76) Chrysene-d12	13.992	240	142564	20.000	ng	# 0.00
86) Perylene-d12	15.474	264	97140	20.000	ng	0.02
System Monitoring Compounds						
5) 2-Fluorophenol	5.439	112	447361	90.454	ng	0.00
7) Phenol-d6	6.463	99	556240	85.411	ng	0.00
23) Nitrobenzene-d5	7.375	82	354095	59.090	ng	0.00
42) 2,4,6-Tribromophenol	10.645	330	108504	82.438	ng	0.00
45) 2-Fluorobiphenyl	9.169	172	541814	69.426	ng	0.00
79) Terphenyl-d14	12.927	244	525167	71.111	ng	0.00
Target Compounds						
80) Butylbenzylphthalate	13.398	149	66023	15.423	ng	Qvalue 95
84) Bis(2-ethylhexyl)phtha...	13.957	149	136474	24.109	ng	100
92) Benzo(g,h,i)perylene	17.433	276	33177	7.148	ng	# 89


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF052522\
Data File : BF128465.D
Acq On : 25 May 2022 17:52
Operator : CG\JU
Sample : N2894-09
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
P004-SS006-0006-01


Quant Time: May 26 01:01:24 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF052022.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed May 25 12:38:46 2022
Response via : Initial Calibration

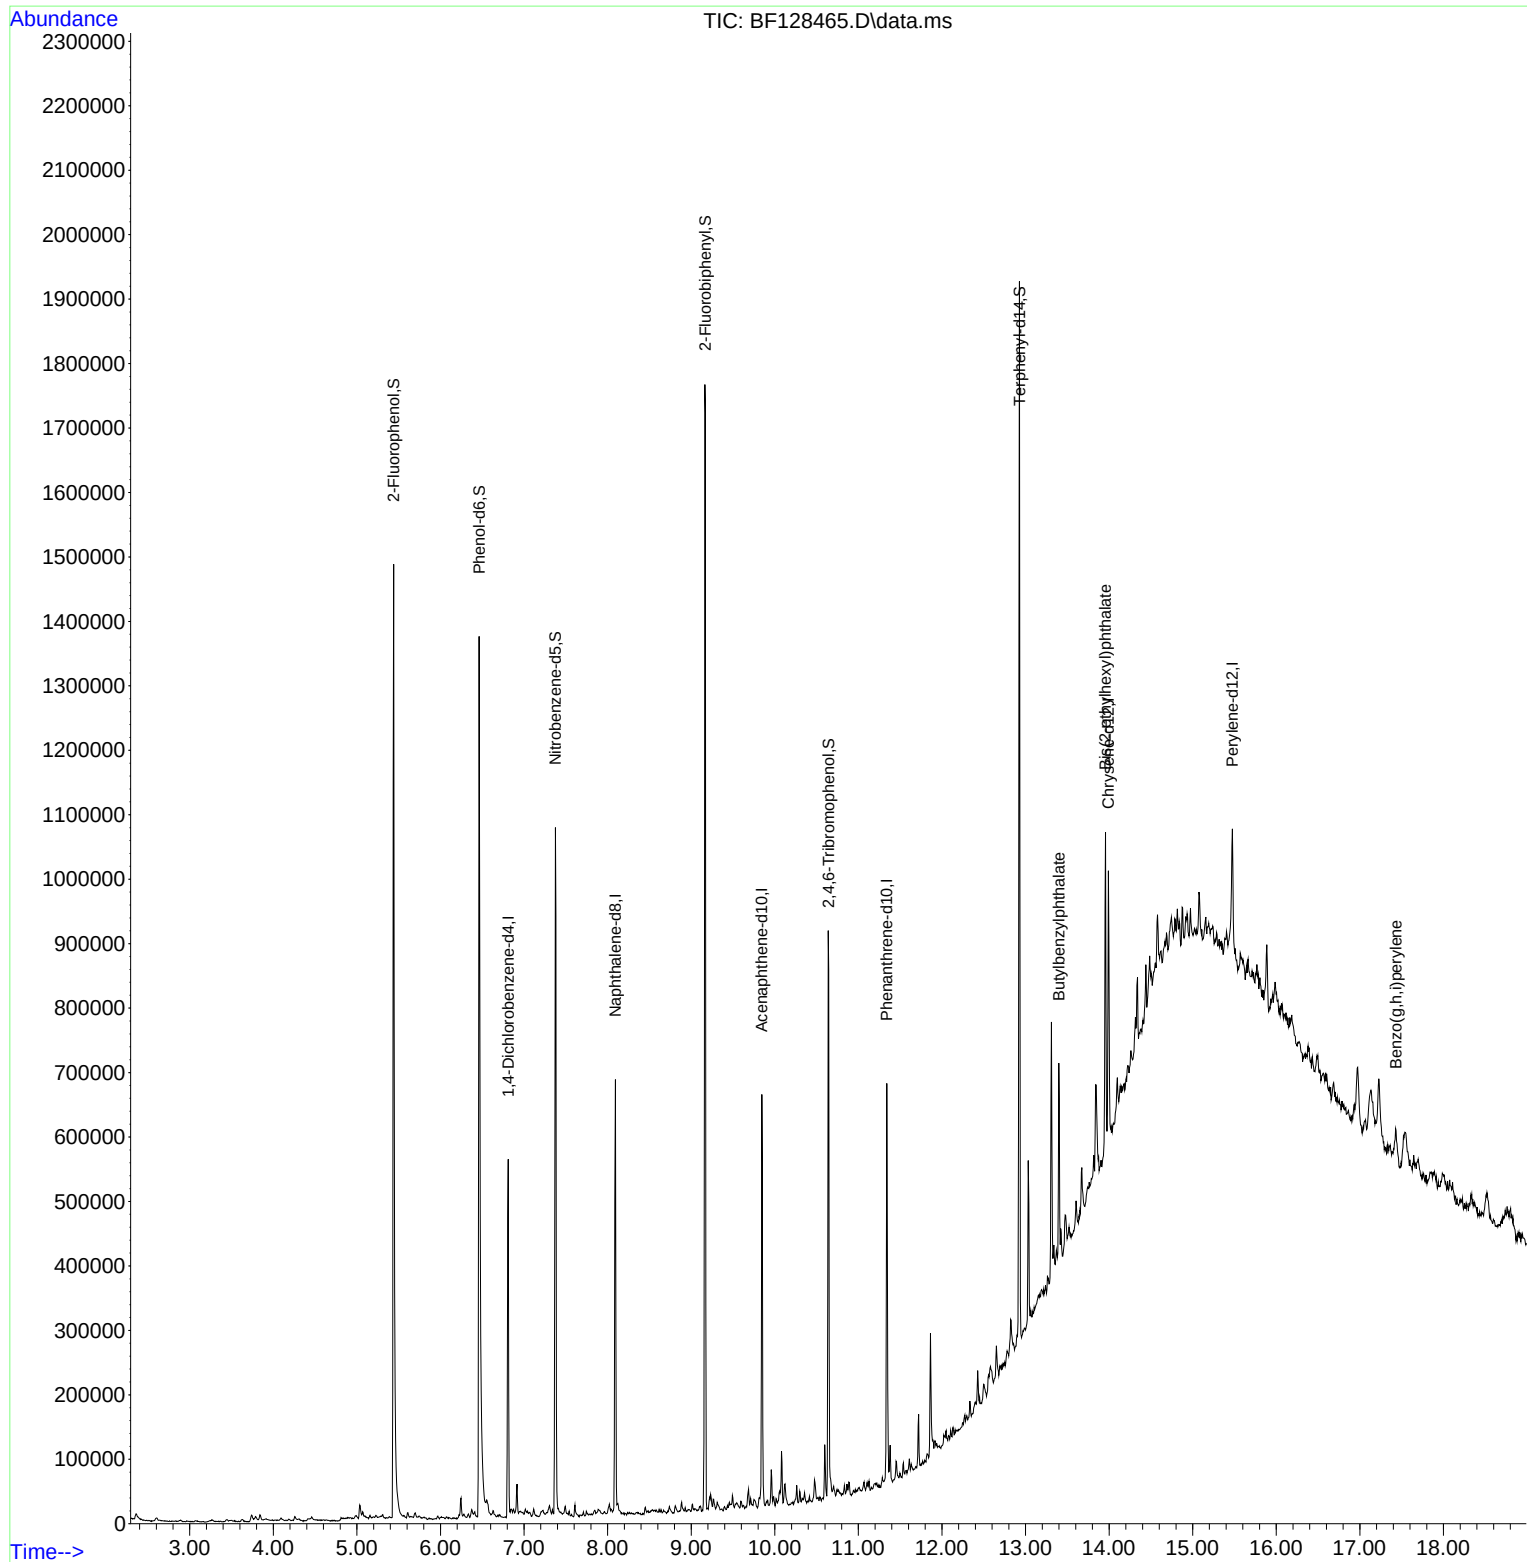






#1
1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 6.810 min Scan# 70
Delta R.T. 0.000 min
Lab File: BF128465.D
Acq: 25 May 2022 17:52

Instrument :
BNA_F
ClientSampleId :
P004-SS006-0006-01



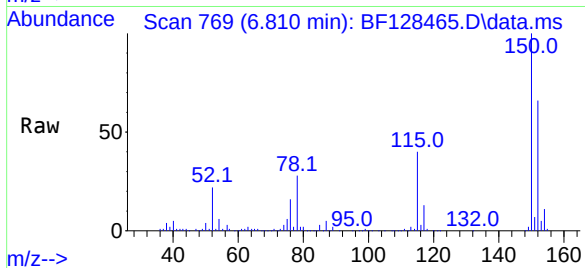



Tgt Ion:152 Resp: 78705
Ion Ratio Lower Upper
152 100
150 151.6 125.3 187.9
115 60.5 48.8 73.2

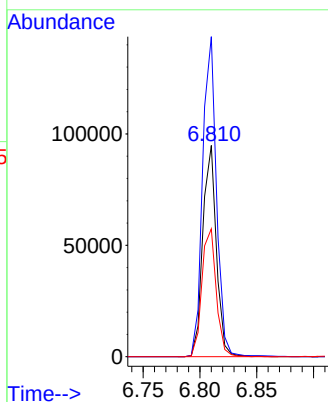

#5
2-Fluorophenol
Concen: 90.454 ng
RT: 5.439 min Scan# 536
Delta R.T. 0.006 min
Lab File: BF128465.D
Acq: 25 May 2022 17:52

Tgt Ion:112 Resp: 447361
Ion Ratio Lower Upper
112 100
64 63.2 49.5 74.3
63 34.5 26.3 39.5


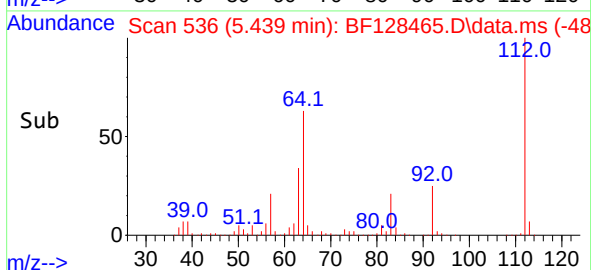
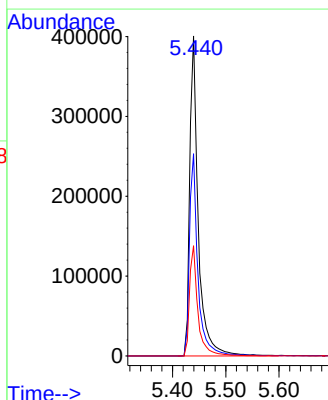
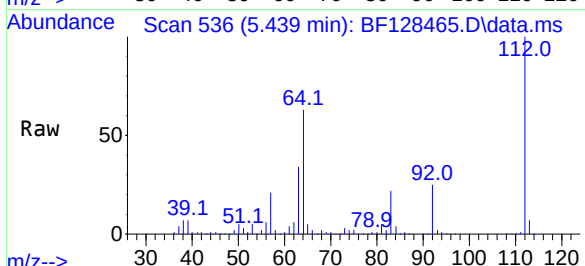


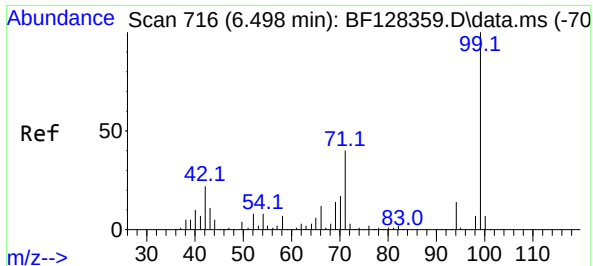

#7
Phenol-d6
Concen: 85.411 ng
RT: 6.463 min Scan# 71
Delta R.T. 0.006 min
Lab File: BF128465.D
Acq: 25 May 2022 17:52




Instrument :
BNA_F
ClientSampleId :
P004-SS006-0006-01


Tgt Ion: 99 Resp: 556240
Ion Ratio Lower Upper
99 100
42 20.8 16.6 24.8
71 38.3 30.0 45.0

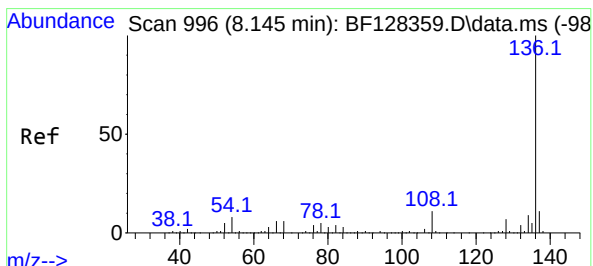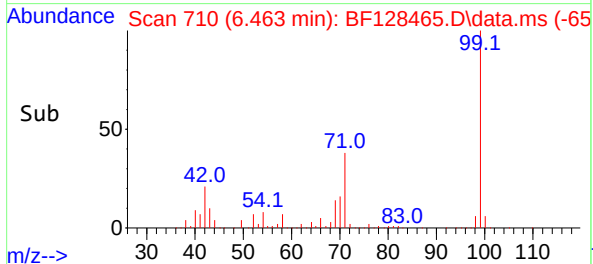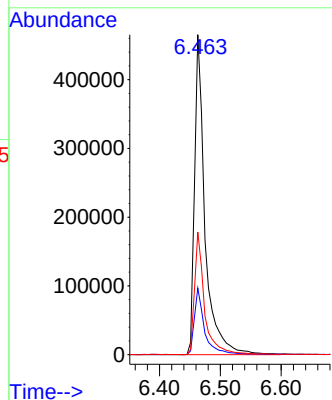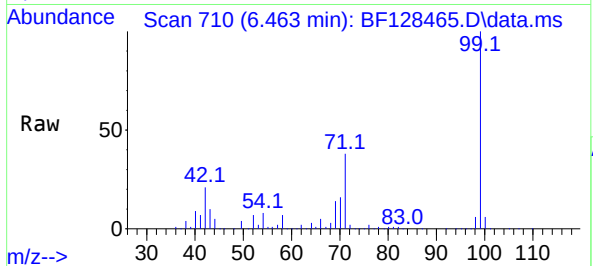

#21
Naphthalene-d8
Concen: 20.000 ng
RT: 8.092 min Scan# 987
Delta R.T. -0.000 min
Lab File: BF128465.D
Acq: 25 May 2022 17:52

Tgt Ion: 136 Resp: 268492
Ion Ratio Lower Upper
136 100
137 10.7 8.6 13.0
54 8.3 6.8 10.2
68 6.3 5.1 7.7


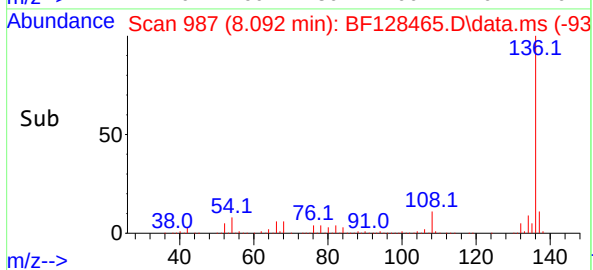
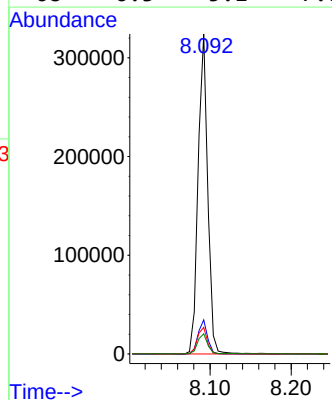
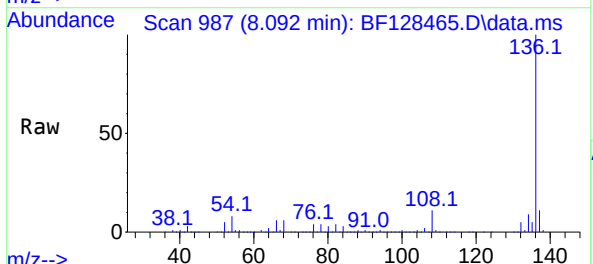


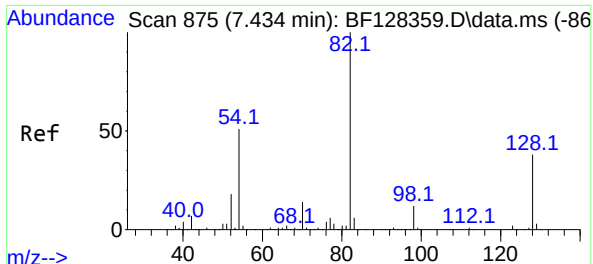

#23
Nitrobenzene-d5
Concen: 59.090 ng
RT: 7.375 min Scan# 80
Delta R.T. -0.006 min
Lab File: BF128465.D
Acq: 25 May 2022 17:52




Instrument :
BNA_F
ClientSampleId :
P004-SS006-0006-01


Tgt Ion: 82 Resp: 354095
Ion Ratio Lower Upper
82 100
128 36.9 30.0 45.0
54 51.3 41.3 61.9

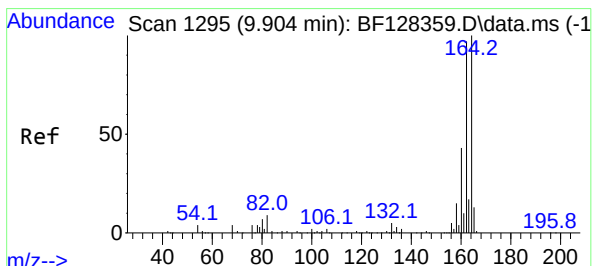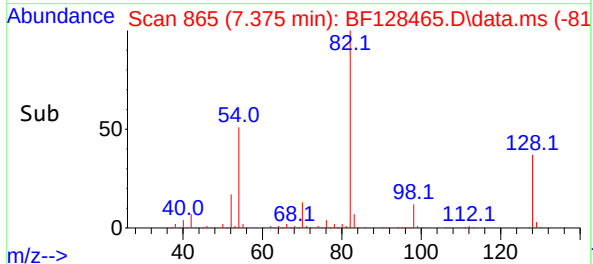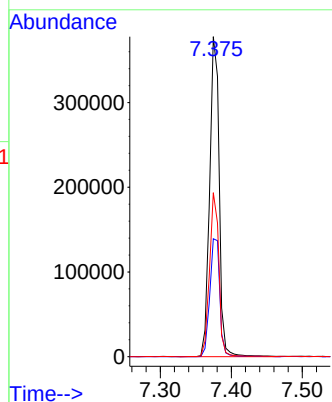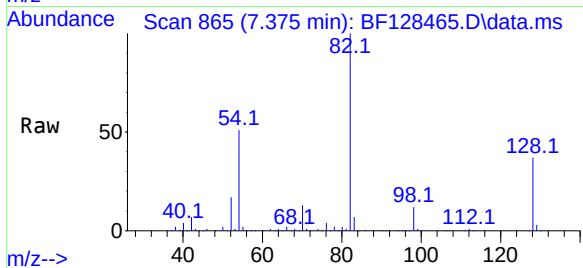

#39
Acenaphthene-d10
Concen: 20.000 ng
RT: 9.845 min Scan# 1285
Delta R.T. -0.006 min
Lab File: BF128465.D
Acq: 25 May 2022 17:52

Tgt Ion:164 Resp: 127625
Ion Ratio Lower Upper
164 100
162 95.9 76.0 114.0
160 42.7 34.8 52.2

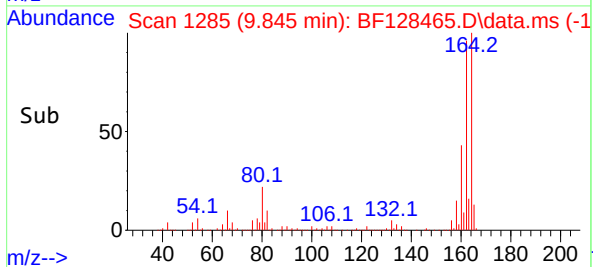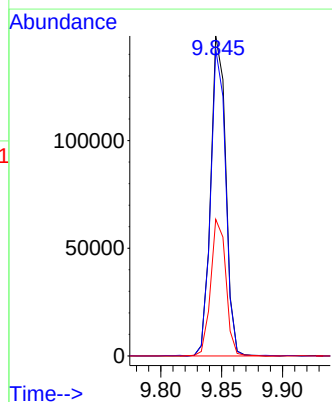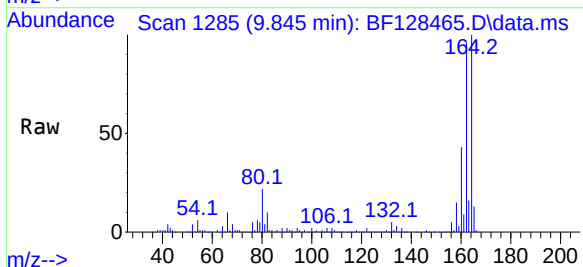

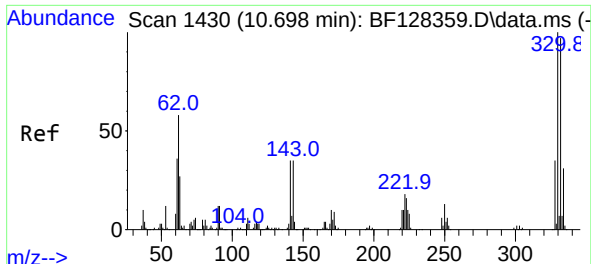

#42

2,4,6-Tribromophenol

Concen: 82.438 ng

RT: 10.645 min Scan# 1430

Delta R.T. -0.000 min

Lab File: BF128465.D


Acq: 25 May 2022 17:52

Instrument :

BNA_F

ClientSampleId :

P004-SS006-0006-01

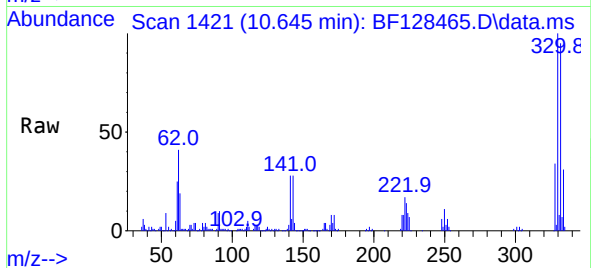




Tgt Ion:330 Resp: 108504

Ion Ratio Lower Upper

330 100

332 95.8 79.0 118.4

141 33.4 28.9 43.3

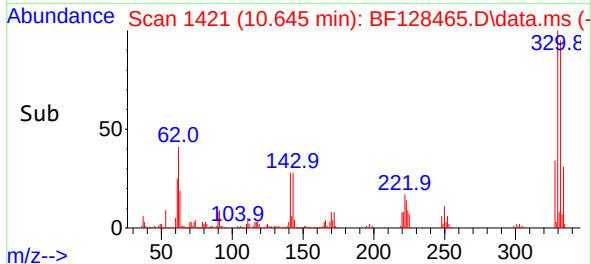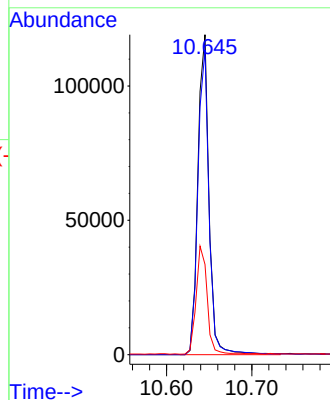

#45

2-Fluorobiphenyl

Concen: 69.426 ng

RT: 9.169 min Scan# 1170

Delta R.T. -0.000 min

Lab File: BF128465.D

Acq: 25 May 2022 17:52




Tgt Ion:172 Resp: 541814


Ion Ratio Lower Upper

172 100

171 34.4 28.6 42.8

170 23.9 19.1 28.7


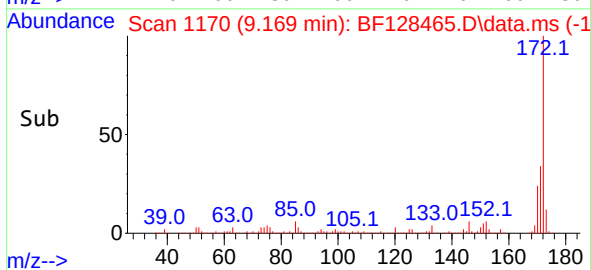
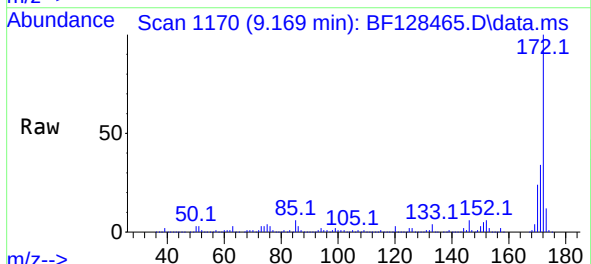
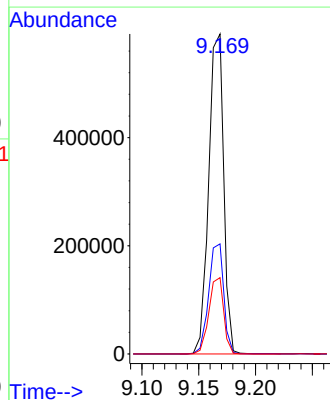




#64
Phenanthrene-d10
Concen: 20.000 ng
RT: 11.339 min Scan# 11
Delta R.T. -0.000 min
Lab File: BF128465.D
Acq: 25 May 2022 17:52




Instrument :
BNA_F
ClientSampleId :
P004-SS006-0006-01


Tgt Ion:188 Resp: 209556
Ion Ratio Lower Upper
188 100
94 9.7 8.0 12.0
80 10.4 8.9 13.3

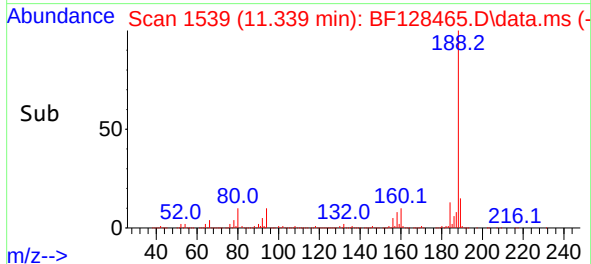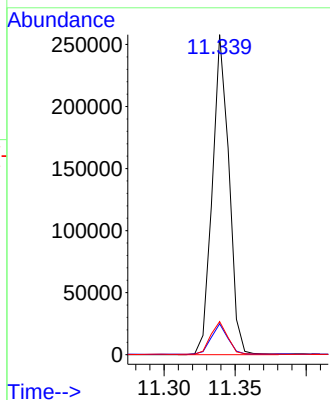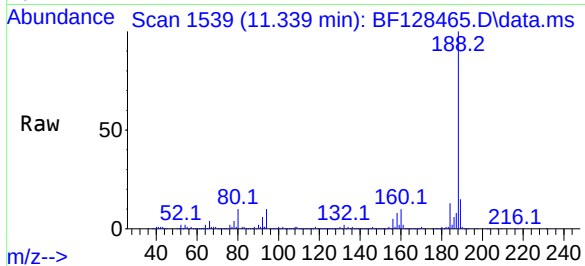

#76
Chrysene-d12
Concen: 20.000 ng
RT: 13.992 min Scan# 1990
Delta R.T. -0.000 min
Lab File: BF128465.D
Acq: 25 May 2022 17:52

Tgt Ion:240 Resp: 142564
Ion Ratio Lower Upper
240 100
120 10.9 7.0 10.6#
236 26.1 20.3 30.5


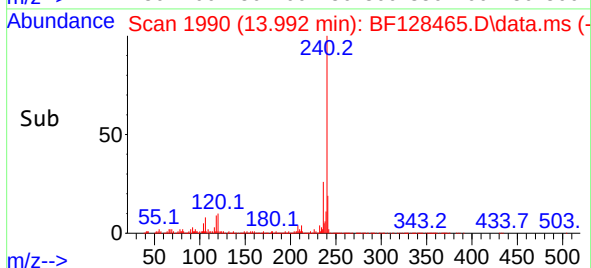
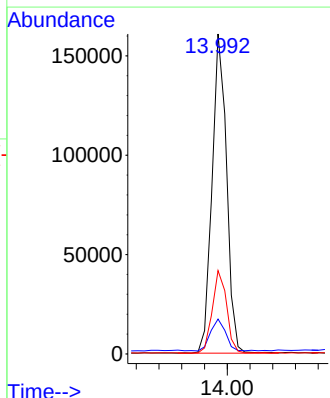
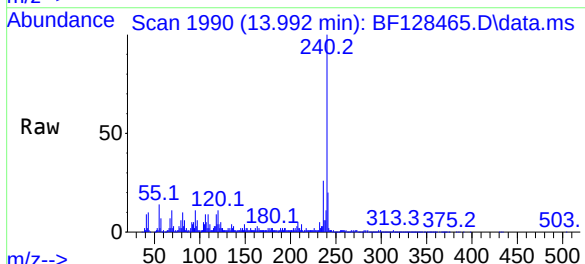




#79
 Terphenyl-d14
 Concen: 71.111 ng
 RT: 12.927 min Scan# 1809
 Delta R.T. -0.000 min
 Lab File: BF128465.D
 Acq: 25 May 2022 17:52




Instrument :
 BNA_F
 ClientSampleId :
 P004-SS006-0006-01


Tgt Ion:244 Resp: 525167
 Ion Ratio Lower Upper
 244 100
 212 7.7 6.2 9.4
 122 9.9 8.6 12.8

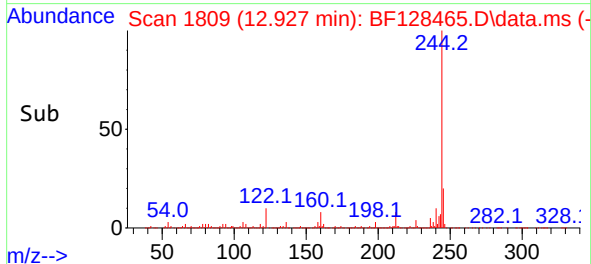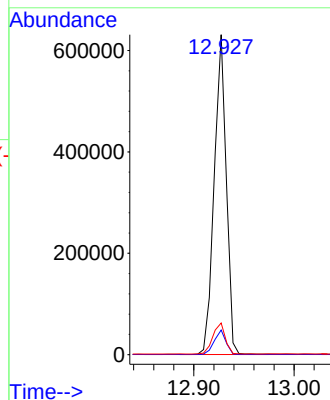

#80
 Butylbenzylphthalate
 Concen: 15.423 ng
 RT: 13.398 min Scan# 1889
 Delta R.T. -0.000 min
 Lab File: BF128465.D
 Acq: 25 May 2022 17:52

Tgt Ion:149 Resp: 66023
 Ion Ratio Lower Upper
 149 100
 91 87.4 65.8 98.6
 206 18.8 15.4 23.2


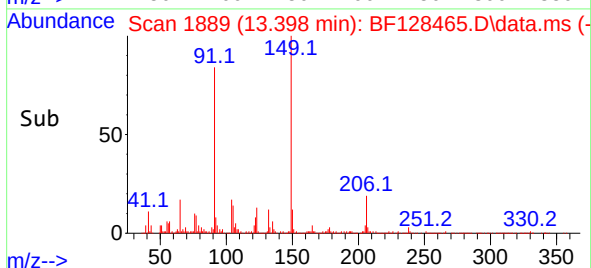
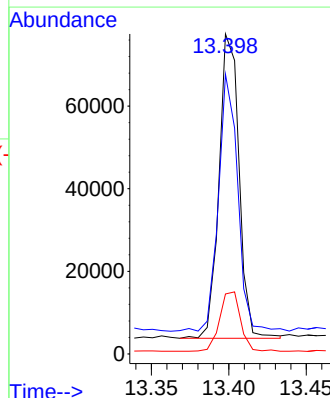
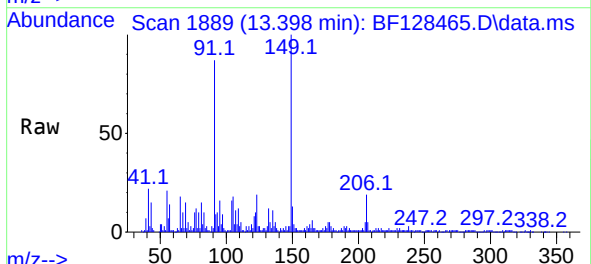




#84
Bis(2-ethylhexyl)phthalate
Concen: 24.109 ng
RT: 13.957 min Scan# 1992
Delta R.T. 0.006 min
Lab File: BF128465.D
Acq: 25 May 2022 17:52




Instrument :
BNA_F
ClientSampleId :
P004-SS006-0006-01


Tgt Ion:149 Resp: 136474
Ion Ratio Lower Upper
149 100
167 27.3 22.0 33.0
279 4.3 3.4 5.0

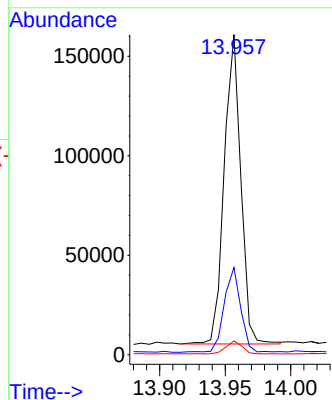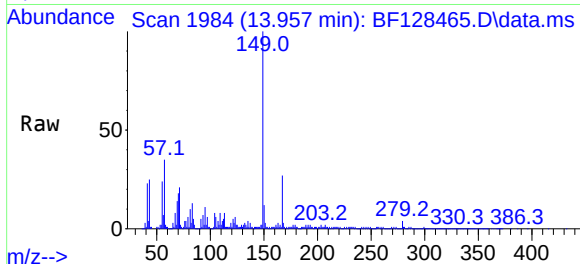

#86
Perylene-d12
Concen: 20.000 ng
RT: 15.474 min Scan# 2242
Delta R.T. 0.018 min
Lab File: BF128465.D
Acq: 25 May 2022 17:52


Tgt Ion:264 Resp: 97140
Ion Ratio Lower Upper
264 100
260 24.9 20.1 30.1
265 21.7 17.5 26.3

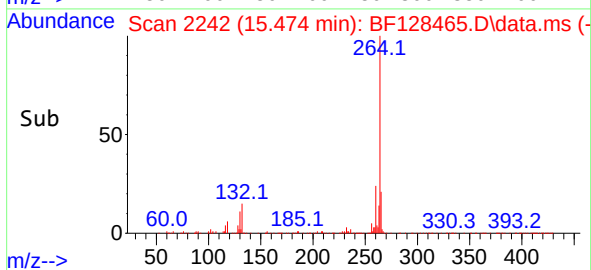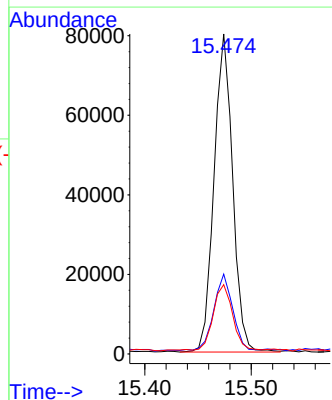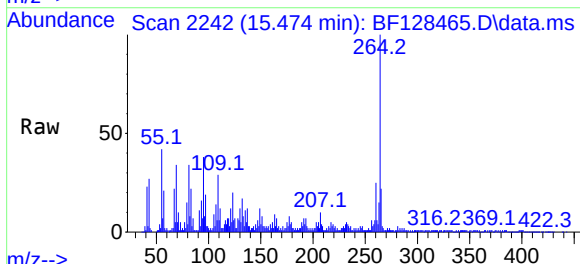

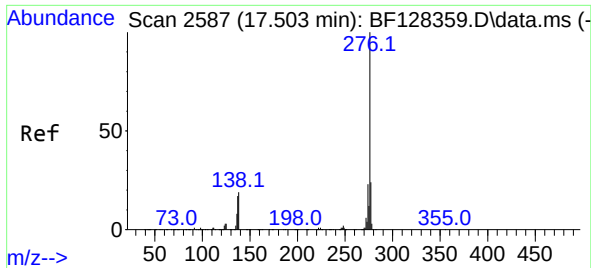

#92
Benzo(g,h,i)perylene
Concen: 7.148 ng
RT: 17.433 min Scan# 21
Delta R.T. 0.053 min
Lab File: BF128465.D
Acq: 25 May 2022 17:52

Instrument :
BNA_F
ClientSampleId :
P004-SS006-0006-01

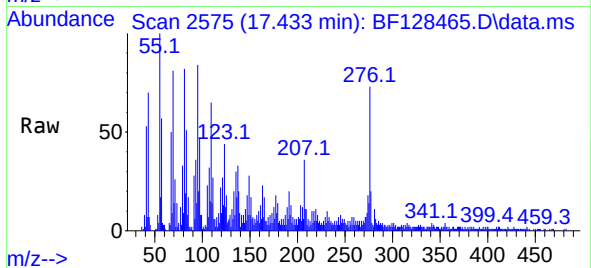

Tgt Ion:	276	Resp:	33177
Ion	Ratio	Lower	Upper
276	100		
277	27.1	18.8	28.2
138	27.6	16.2	24.2

