

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF052522\
 Data File : BF128474.D
 Acq On : 25 May 2022 22:15
 Operator : CG\JU
 Sample : N2896-17 2X
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 P040-SS001-0006-01

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF052022.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF128474.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.846	261	265	271	rBV	6907	9890	1.44%	0.149%
2	5.028	463	466	472	rVB	9122	12421	1.81%	0.187%
3	5.440	533	536	555	rBV	536878	640310	93.25%	9.616%
4	6.463	706	710	725	rBV	548998	653506	95.17%	9.814%
5	6.810	766	769	775	rBV	690364	557134	81.13%	8.367%
6	7.375	862	865	876	rBV	454227	395980	57.66%	5.947%
7	8.092	984	987	991	rBV	760116	645059	93.94%	9.687%
8	8.128	991	993	1002	rVB3	8770	12336	1.80%	0.185%
9	8.739	1091	1097	1101	rBV4	7260	8291	1.21%	0.125%
10	9.169	1166	1170	1173	rBV	833535	686691	100.00%	10.312%
11	9.851	1282	1286	1289	rBV	786333	621857	90.56%	9.339%
12	10.645	1417	1421	1429	rBV	329861	287963	41.93%	4.324%
13	10.745	1434	1438	1445	rVB4	6544	8436	1.23%	0.127%
14	11.286	1526	1530	1536	rBV4	7962	9342	1.36%	0.140%
15	11.345	1536	1540	1543	rBV	706912	594087	86.51%	8.922%
16	11.616	1580	1586	1588	rBV5	5904	8343	1.21%	0.125%
17	11.869	1624	1629	1631	rBV5	5543	8105	1.18%	0.122%
18	12.816	1787	1790	1791	rBV3	8318	8038	1.17%	0.121%
19	12.927	1805	1809	1812	rVB	733225	601692	87.62%	9.036%
20	13.486	1901	1904	1907	rBV3	18078	19196	2.80%	0.288%
21	13.992	1987	1990	1994	rBV	501155	461031	67.14%	6.924%
22	14.080	2002	2005	2009	rBV	71814	77717	11.32%	1.167%
23	15.468	2237	2241	2248	rVB2	255630	331498	48.27%	4.978%




Sum of corrected areas: 6658923

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF052522\
Data File : BF128474.D
Acq On : 25 May 2022 22:15
Operator : CG\JU
Sample : N2896-17 2X
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
P040-SS001-0006-01

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF052022.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

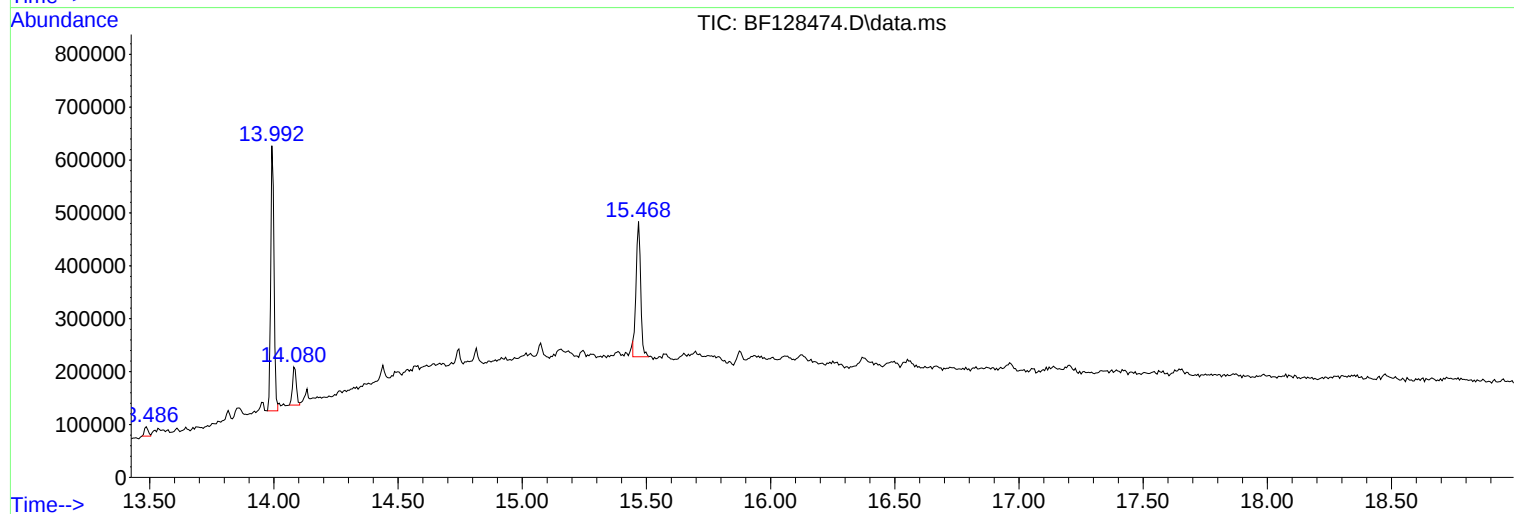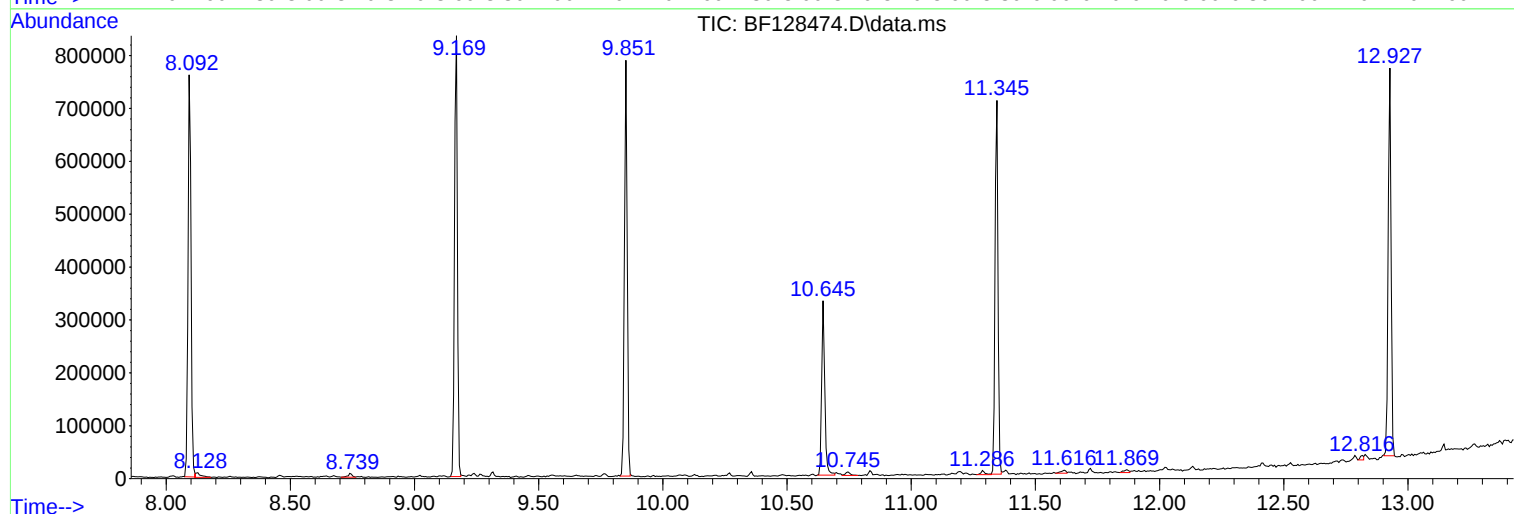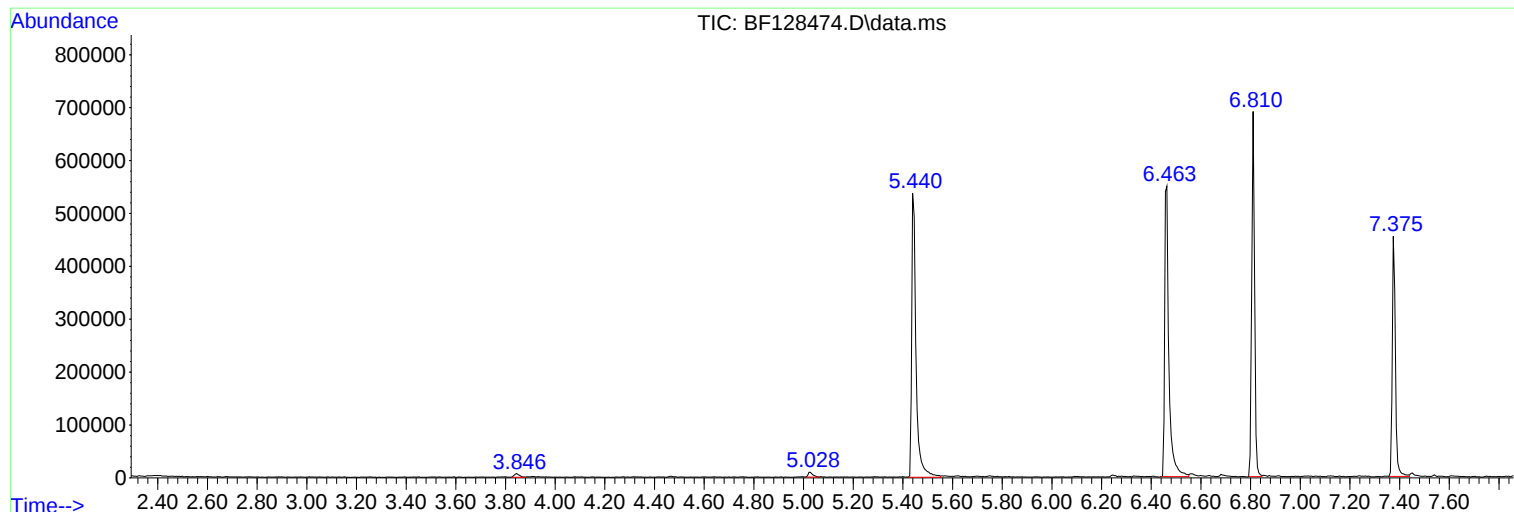

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF052522\
Data File : BF128474.D
Acq On : 25 May 2022 22:15
Operator : CG\JU
Sample : N2896-17 2X
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
P040-SS001-0006-01










Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF052022.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Triphenylphosphine oxide Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
14.080	3.37 ng	77717	Chrysene-d12	13.992

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Triphenylphosphine oxide	278	C18H15OP	000791-28-6	83
2			(E)-7-Benzylidene-1-azabicyclo[3...]	293	C15H19NO3S	1000483-83-4	50
3			Formaldehyde, (triphenylphosphor...]	304	C19H17N2P	015990-54-2	50
4			4-Nitro-4'-methyldiphenylsulfone	277	C13H11NO4S	004094-37-5	46
5			Benzoic acid, 2-(diphenylphosphi...]	306	C19H15O2P	017261-28-8	34

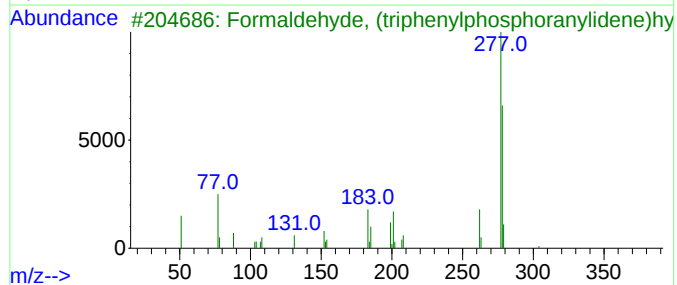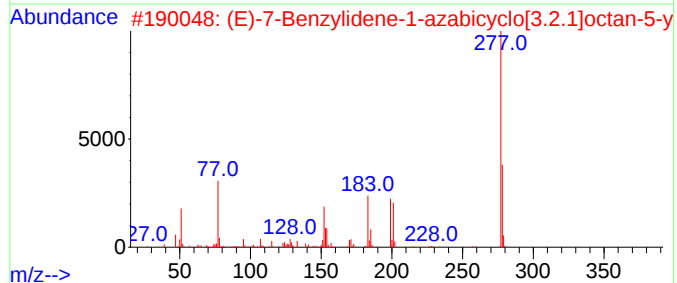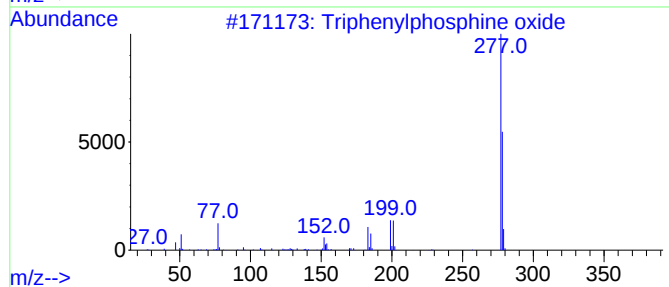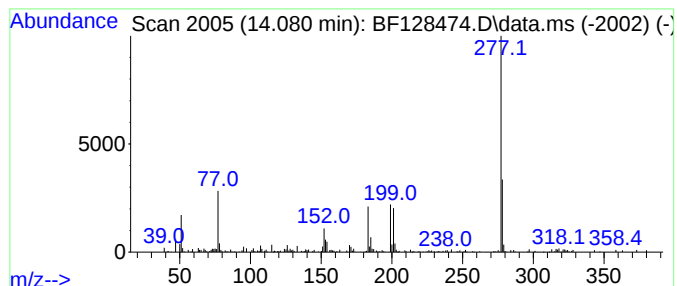

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF052522\
Data File : BF128474.D
Acq On : 25 May 2022 22:15
Operator : CG\JU
Sample : N2896-17 2X
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
P040-SS001-0006-01

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF052022.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Triphenylphosph...	14.080	3.4	ng	77717	5	13.992	461031	20.0