
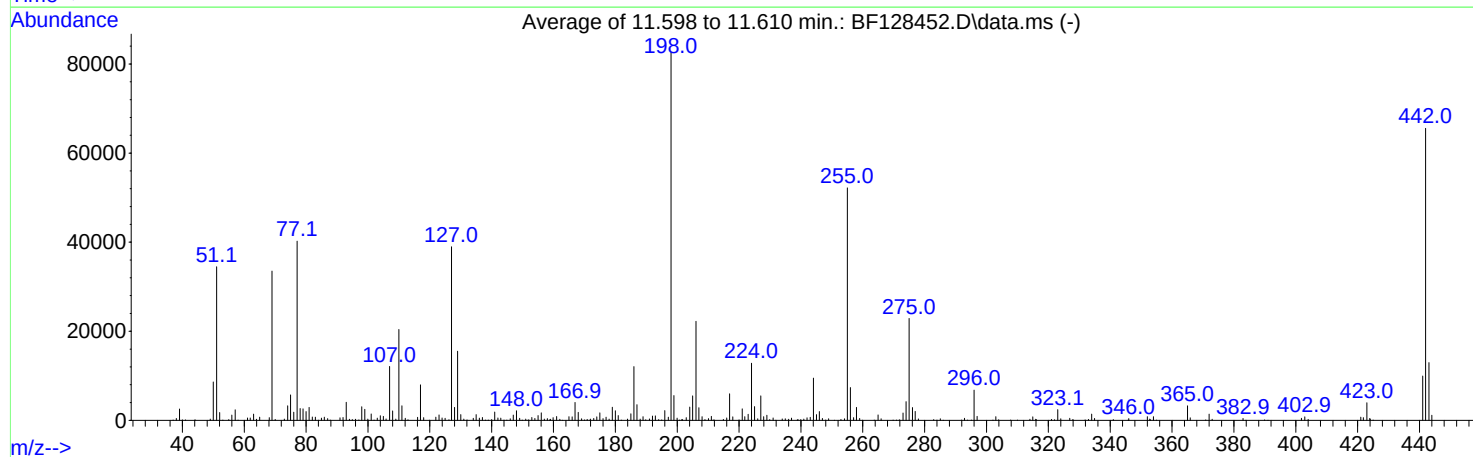


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF052522\
 Data File : BF128452.D
 Acq On : 25 May 2022 10:44
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF052022.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu May 26 06:01:06 2022

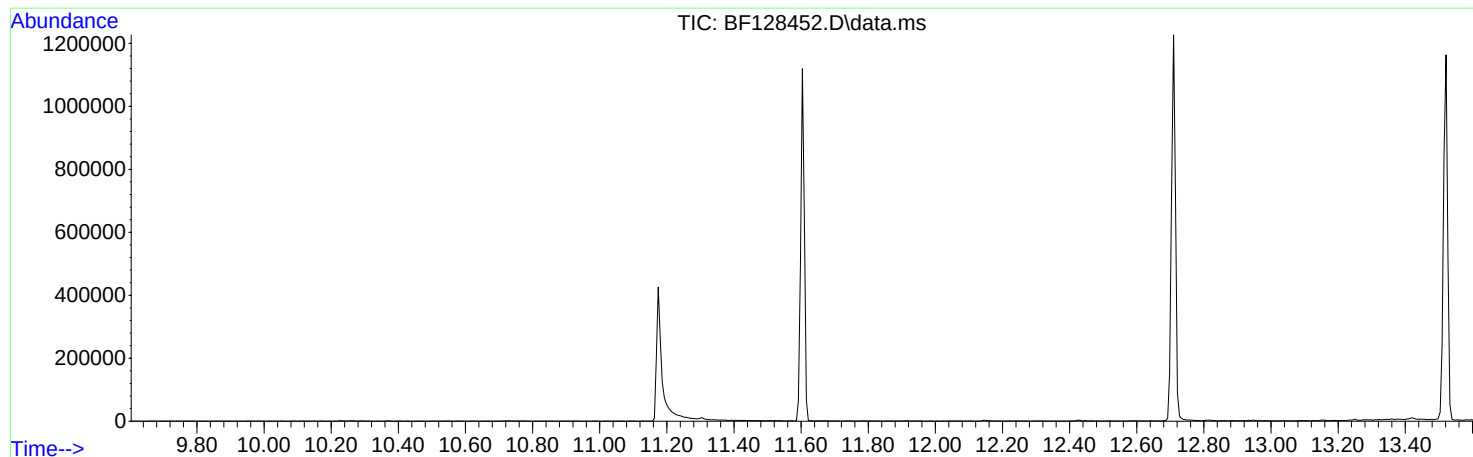




AutoFind: Scans 1583, 1584, 1585; Background Corrected with Scan 1578

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	41.8	34485	PASS
68	69	0.00	2	1.8	611	PASS
69	198	0.00	100	40.6	33504	PASS
70	69	0.00	2	0.6	207	PASS
127	198	10	80	47.2	38984	PASS
197	198	0.00	2	0.9	712	PASS
198	198	100	100	100.0	82581	PASS
199	198	5	9	6.7	5571	PASS
275	198	10	60	27.7	22866	PASS
365	198	1	100	4.0	3269	PASS
441	198	0.01	100	12.0	9945	PASS
442	442	50	100	100.0	65563	PASS
443	442	15	24	19.8	12976	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF052522\
 Data File : BF128452.D
 Acq On : 25 May 2022 10:44
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Quant Time: May 26 06:01:11 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF052022.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu May 26 06:01:06 2022
 Response via : Initial Calibration

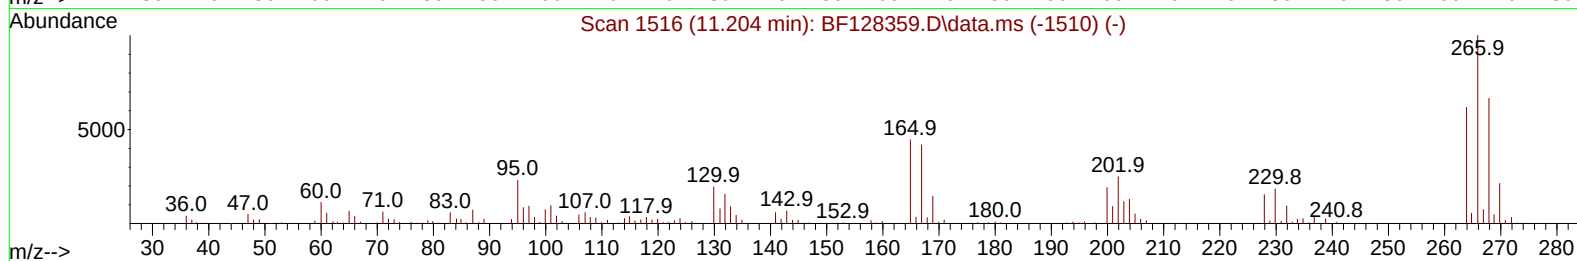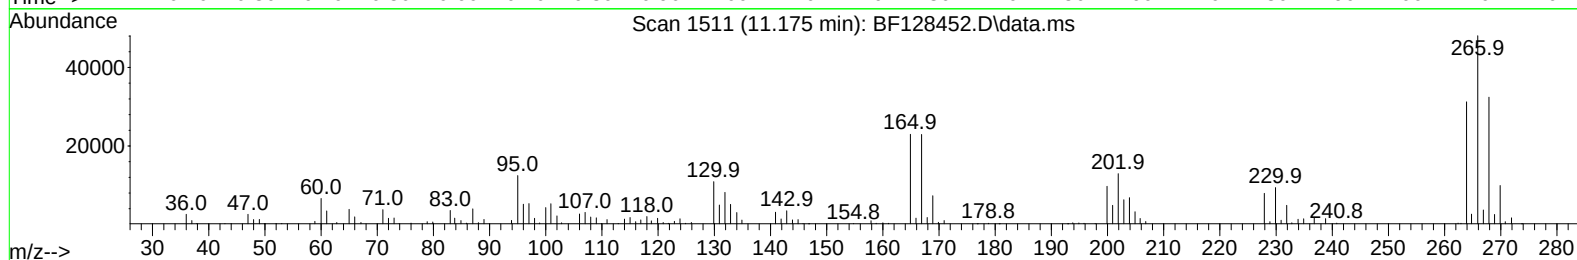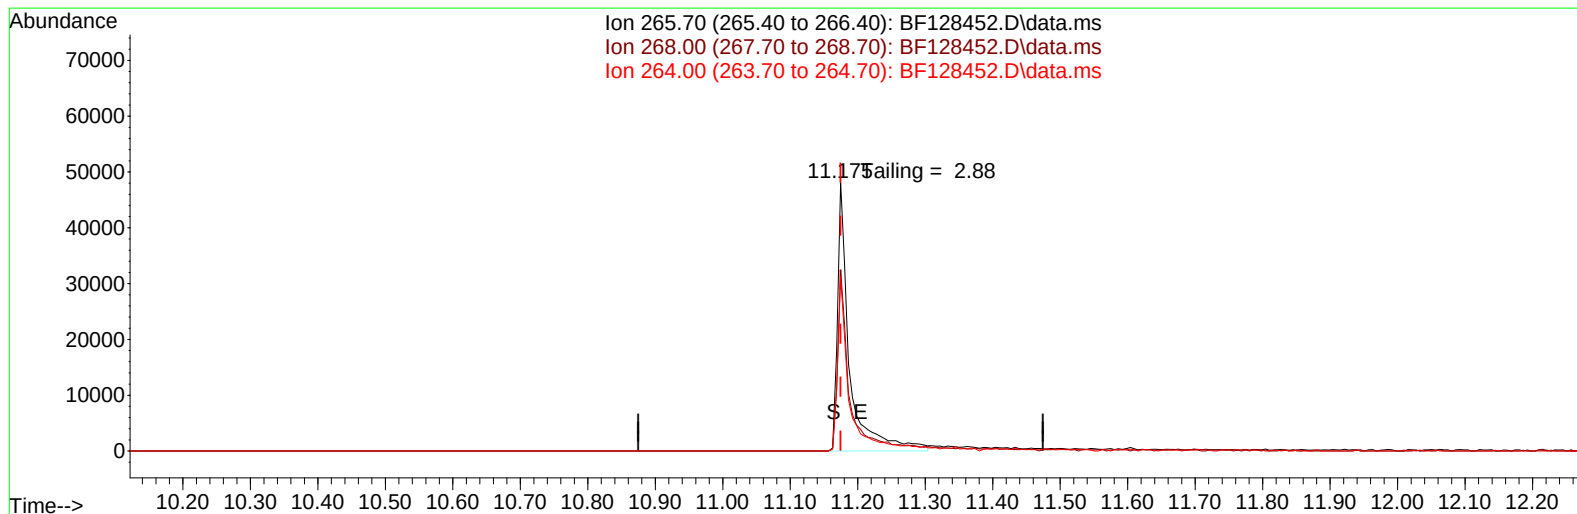

TIC: BF128452.D\data.ms

(70) Pentachlorophenol (C)

11.175min (0.000) 43187.79 ng




response 58070

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	66.30	67.47
264.00	66.40	64.95
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF052522\
Data File : BF128452.D
Acq On : 25 May 2022 10:44
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: May 26 06:01:11 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF052022.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu May 26 06:01:06 2022
Response via : Initial Calibration

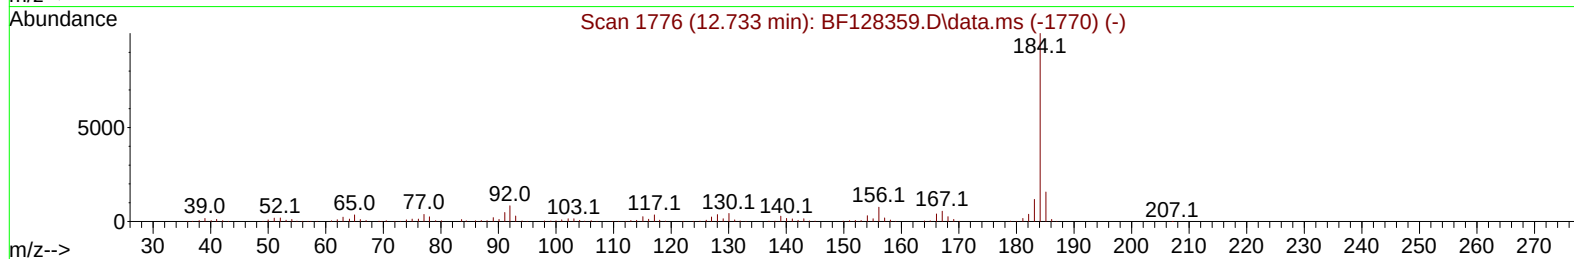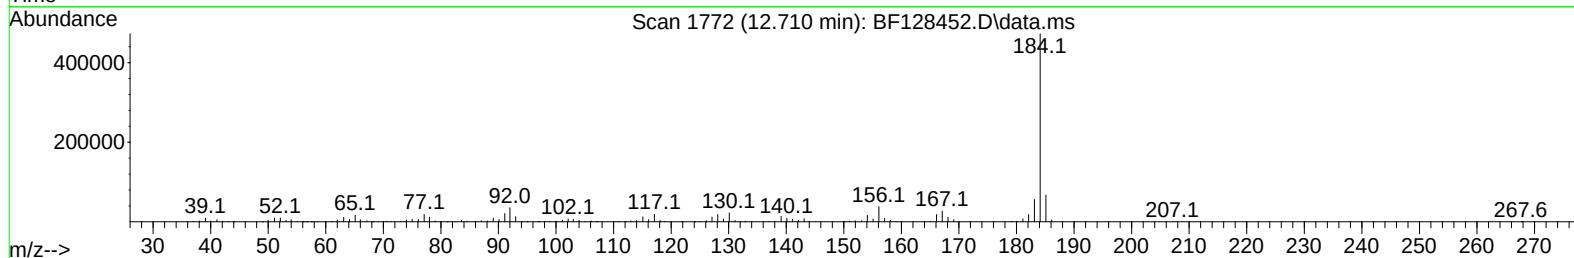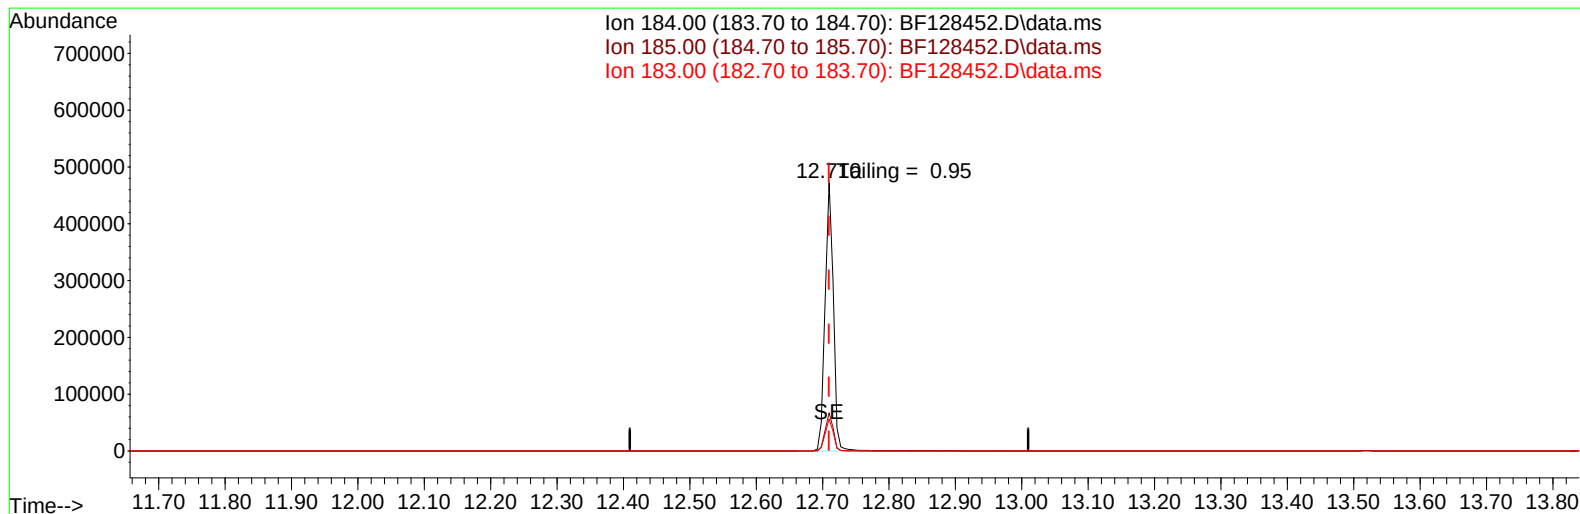

TIC: BF128452.D\data.ms

(77) Benzidine

12.710min (0.000) 58763.38 ng

response 410659

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.10	14.25
183.00	11.20	11.85
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
5/25/2022	BNA_F	<u>BF128452.D</u>
Compound Name	Response	Retention Time
DDT	190547	13.521
DDD	2628	13.251
DDE	132	12.892
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
2760	193307	1.43

Instrument :
BNA_F
ClientSampleId :
DFTPP