
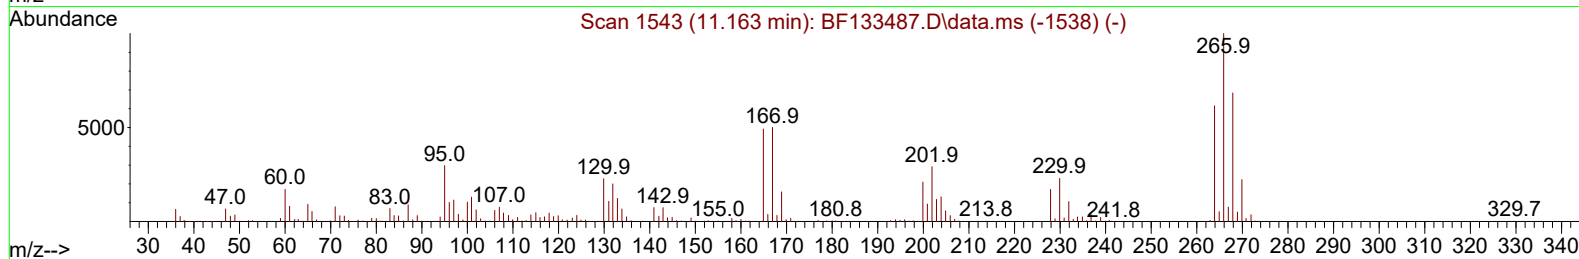
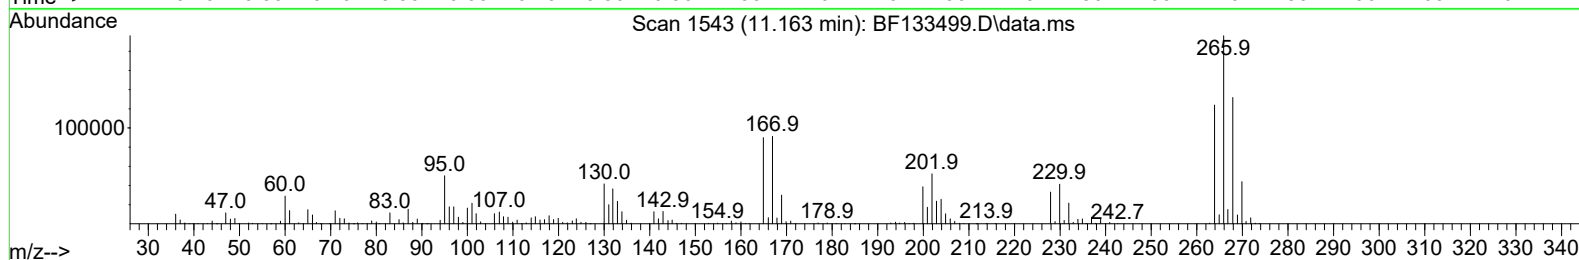


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF052623\
Data File : BF133499.D
Acq On : 26 May 2023 11:36
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 27 06:55:40 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF052523.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu May 25 23:30:55 2023
Response via : Initial Calibration

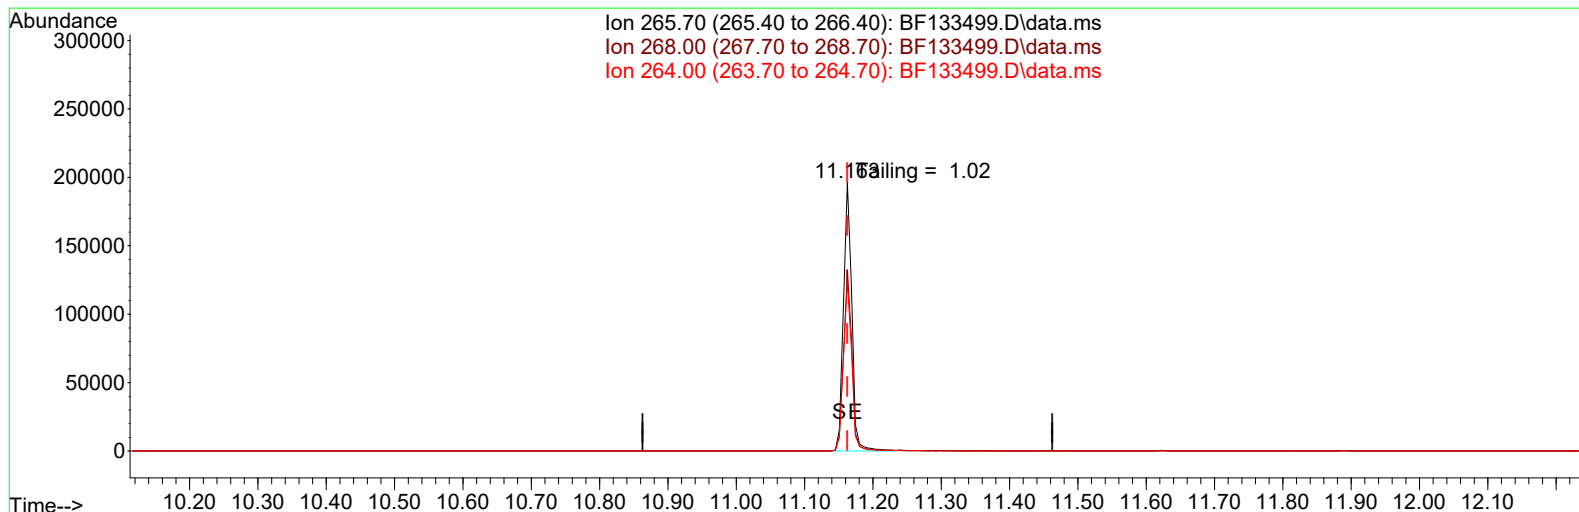

TIC: BF133499.D\data.ms

(70) Pentachlorophenol (C)




11.163min (-0.000) 101123.67 ng

response 167878

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	68.30	67.18
264.00	61.50	63.14
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF052623\
Data File : BF133499.D
Acq On : 26 May 2023 11:36
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 27 06:55:40 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF052523.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu May 25 23:30:55 2023
Response via : Initial Calibration

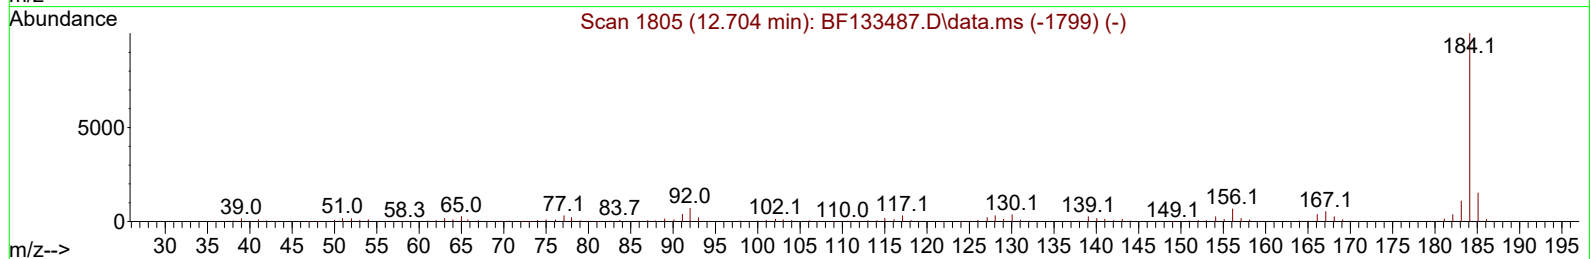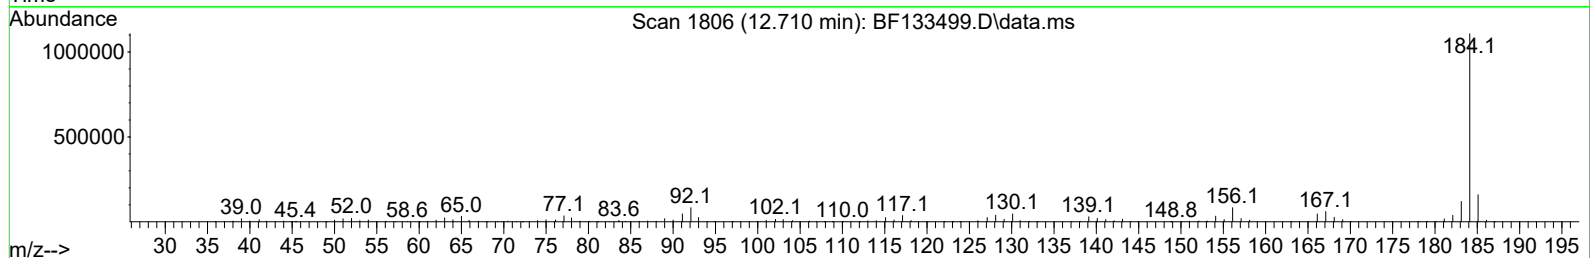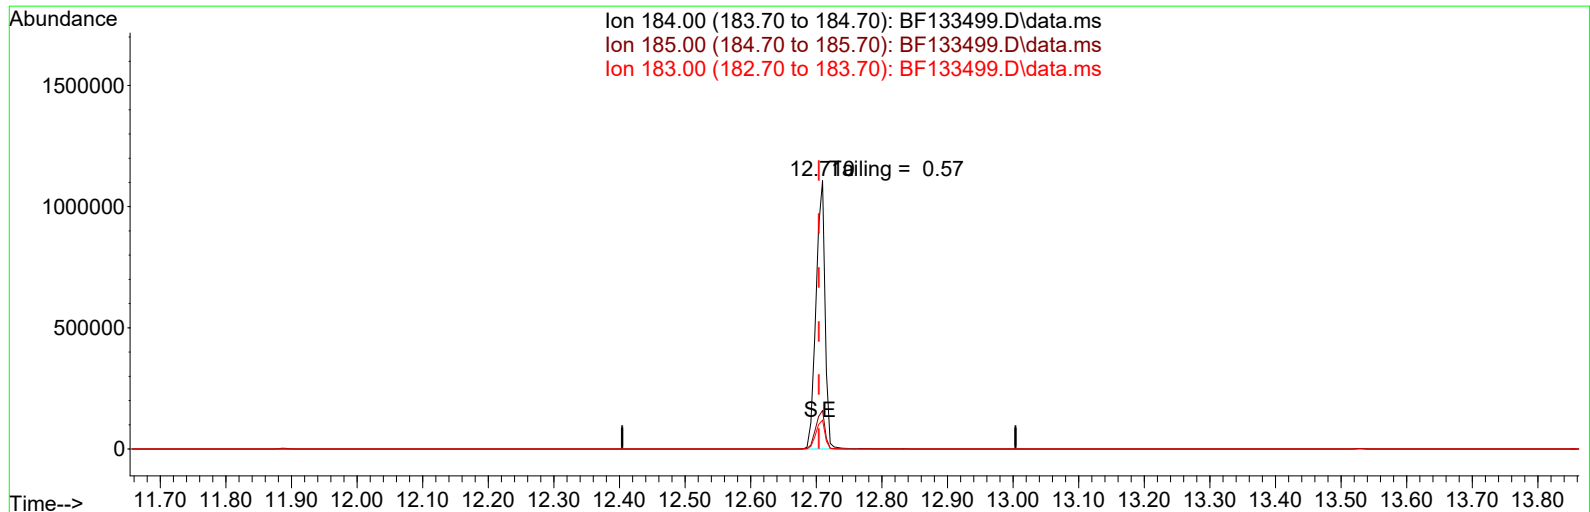

TIC: BF133499.D\data.ms

(77) Benzidine

12.710min (+ 0.006) 0.00 ng

response 1050684

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.20	14.41
183.00	10.90	10.80
0.00	0.00	0.00