


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF052623\
 Data File : BF133499.D
 Acq On : 26 May 2023 11:36
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF052523.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue May 30 12:58:40 2023

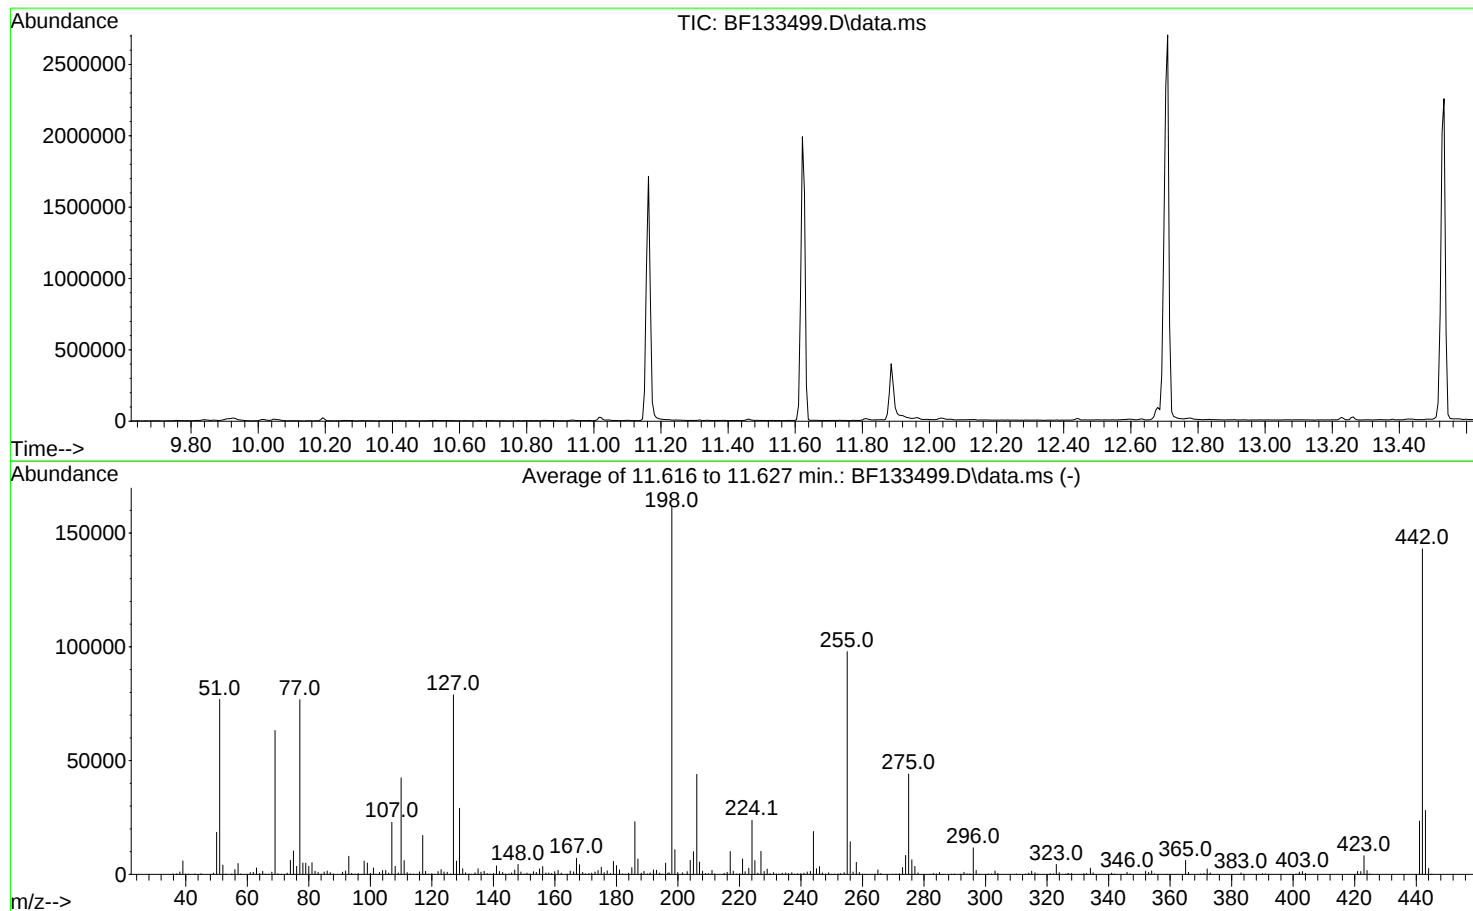

AutoFind: Scans 1620, 1621, 1622; Background Corrected with Scan 1615

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	47.5	76880	PASS
68	69	0.00	2	1.6	1009	PASS
69	198	0.00	100	39.1	63235	PASS
70	69	0.00	2	0.5	315	PASS
127	198	10	80	48.8	78920	PASS
197	198	0.00	2	0.5	735	PASS
198	198	100	100	100.0	161693	PASS
199	198	5	9	6.7	10858	PASS
275	198	10	60	27.3	44067	PASS
365	198	1	100	3.8	6110	PASS
441	198	0.01	100	14.5	23421	PASS
442	442	50	100	100.0	143091	PASS
443	442	15	24	19.6	28051	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
5/26/2023	BNA_F	<u>BF133499.D</u>
Compound Name	Response	Retention Time
DDT	388778	13.533
DDD	6166	13.262
DDE	0	12.896
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
6166	394944	1.56

Instrument :
BNA_F
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF052623\
Data File : BF133499.D
Acq On : 26 May 2023 11:36
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: May 27 06:55:40 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF052523.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu May 25 23:30:55 2023
Response via : Initial Calibration

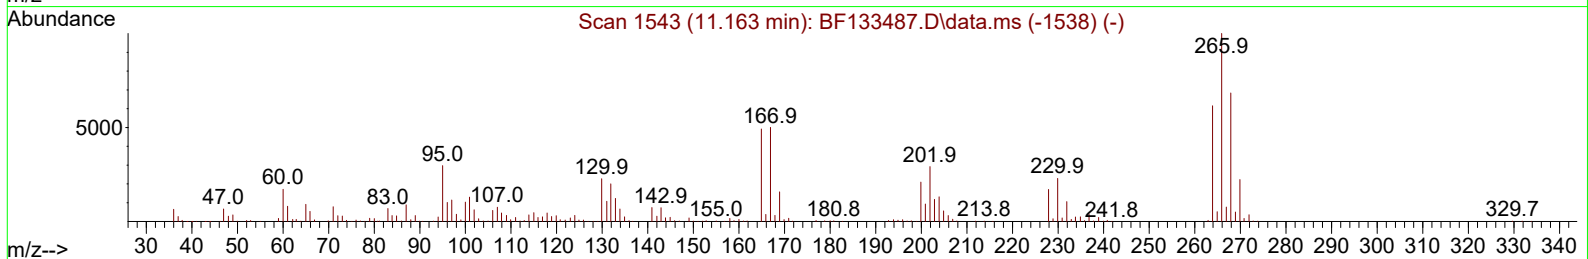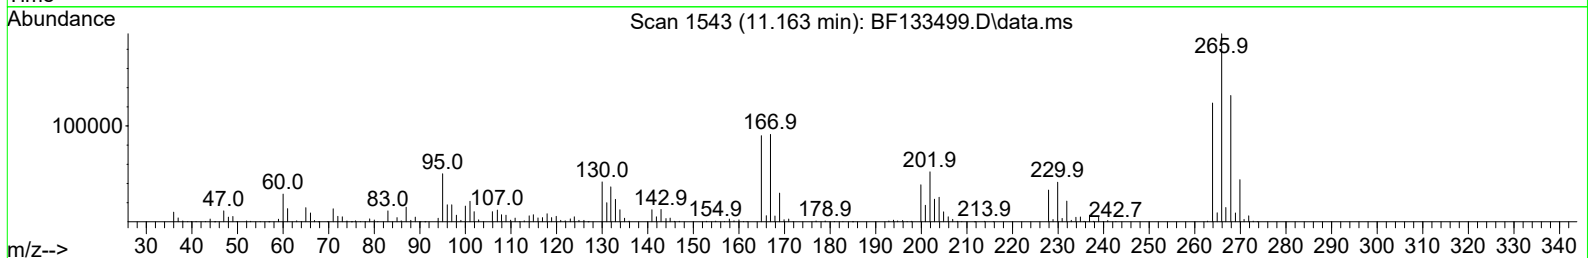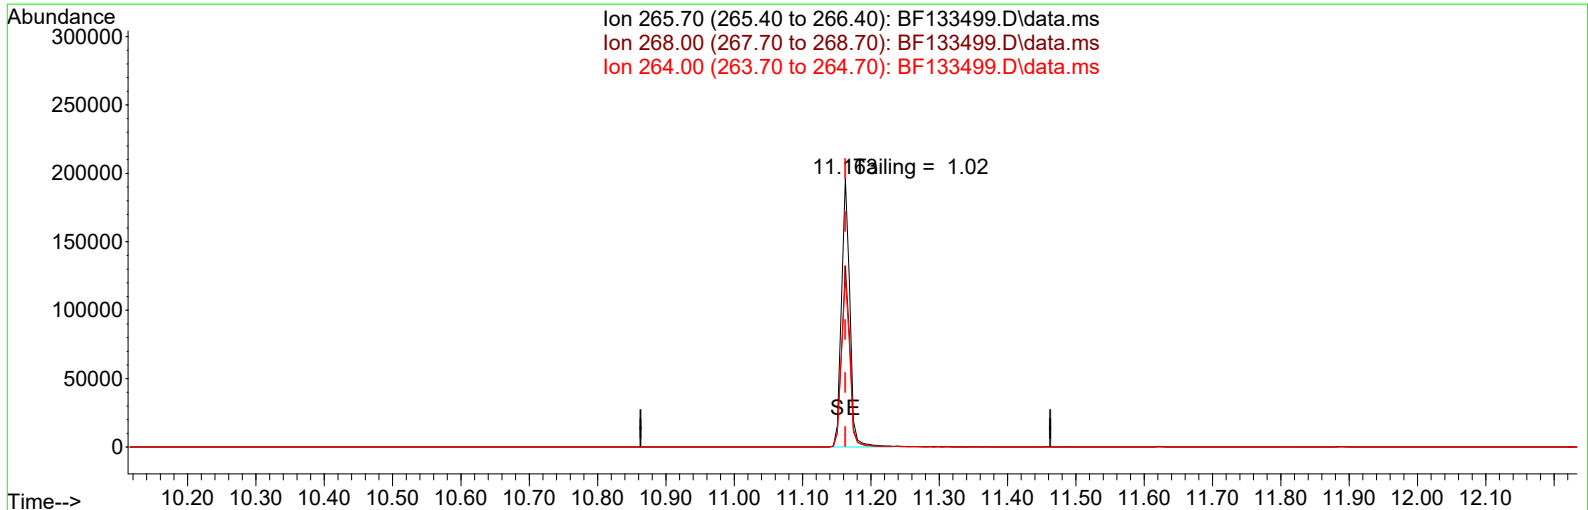

TIC: BF133499.D\data.ms

(70) Pentachlorophenol (C)

11.163min (-0.000) 101123.67 ng




response 167878

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	68.30	67.18
264.00	61.50	63.14
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF052623\
Data File : BF133499.D
Acq On : 26 May 2023 11:36
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: May 27 06:55:40 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF052523.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu May 25 23:30:55 2023
Response via : Initial Calibration

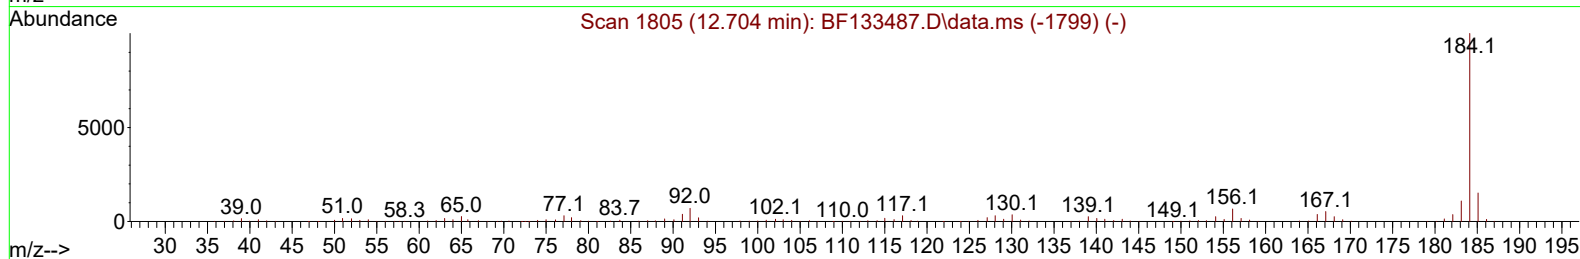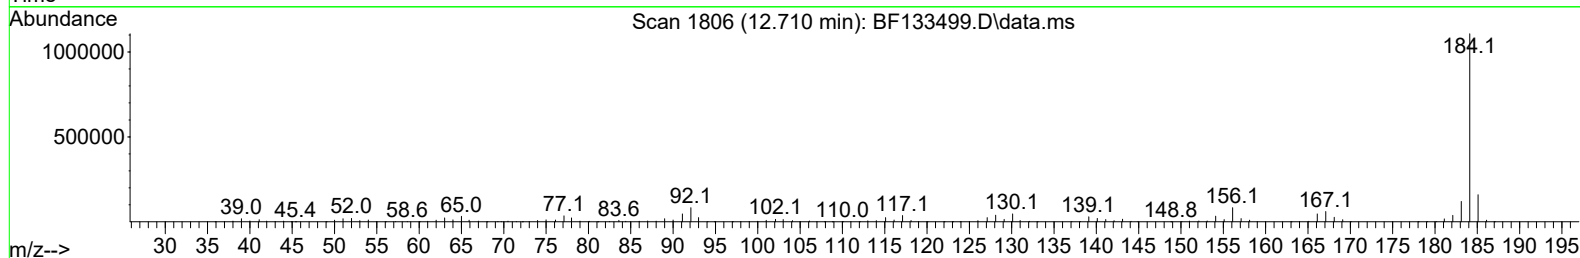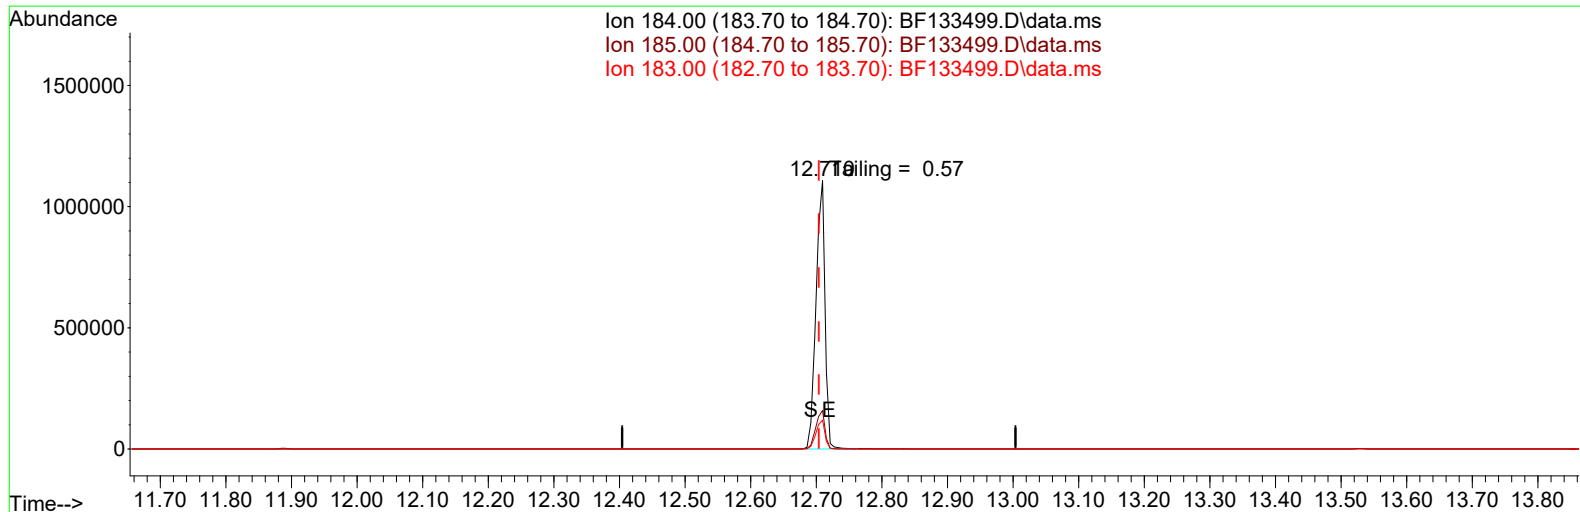

TIC: BF133499.D\data.ms

(77) Benzidine

12.710min (+ 0.006) 0.00 ng

response 1050684

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.20	14.41
183.00	10.90	10.80
0.00	0.00	0.00