
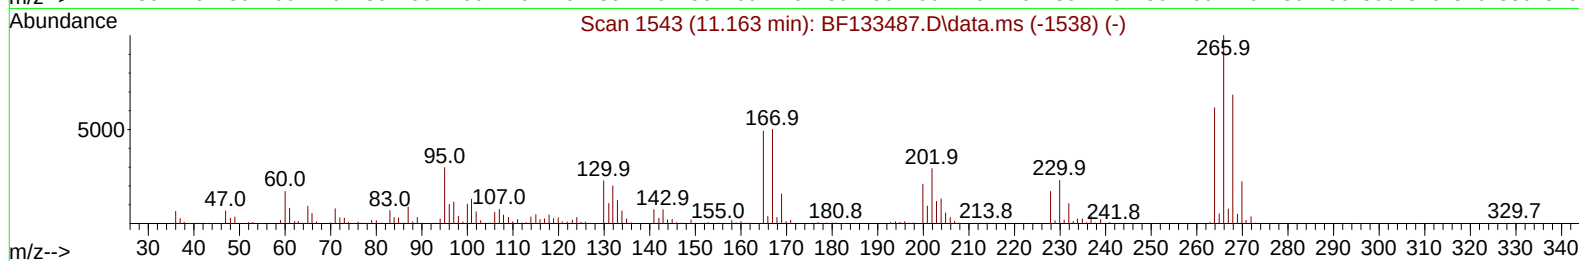
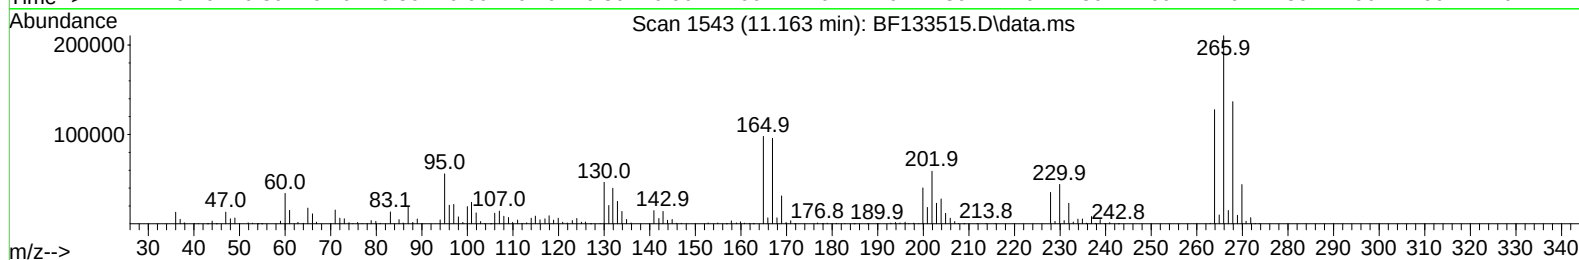


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF053023\
Data File : BF133515.D
Acq On : 30 May 2023 09:43
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 30 12:49:17 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF052523.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu May 25 23:30:55 2023
Response via : Initial Calibration

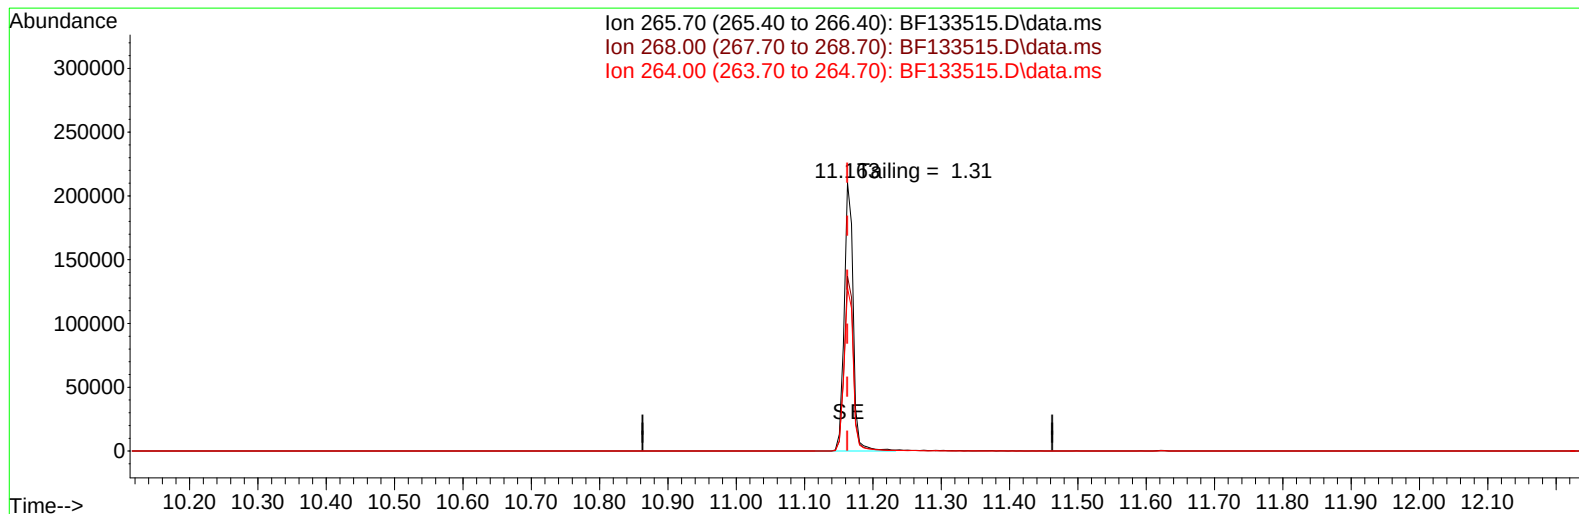

TIC: BF133515.D\data.ms

(70) Pentachlorophenol (C)




11.163min (-0.000) 417388.07 ng

response 191245

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	68.30	64.96
264.00	61.50	60.73
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF053023\
Data File : BF133515.D
Acq On : 30 May 2023 09:43
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 30 12:49:17 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF052523.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu May 25 23:30:55 2023
Response via : Initial Calibration

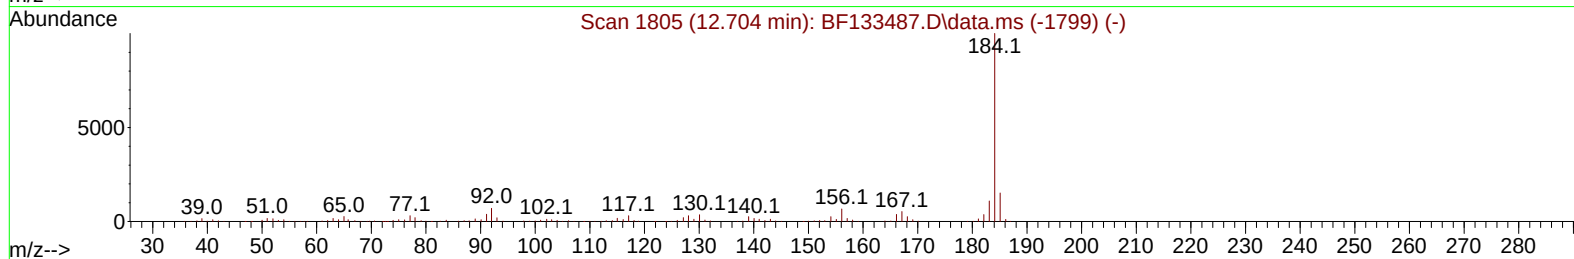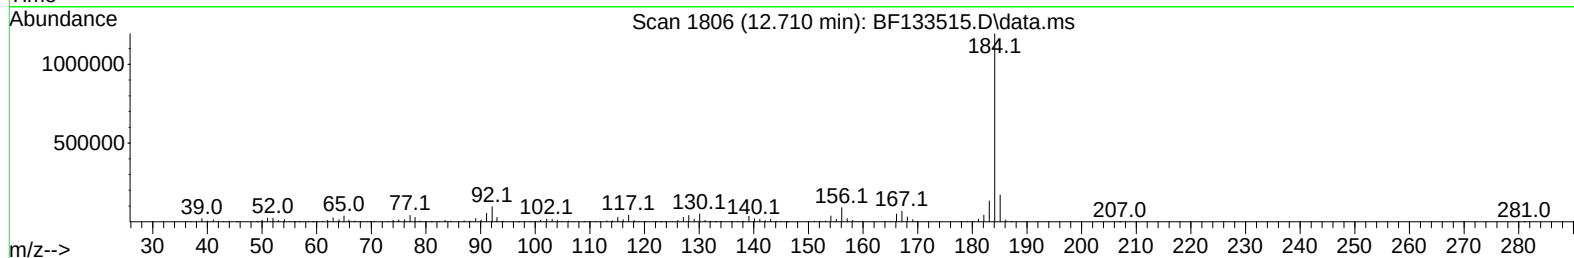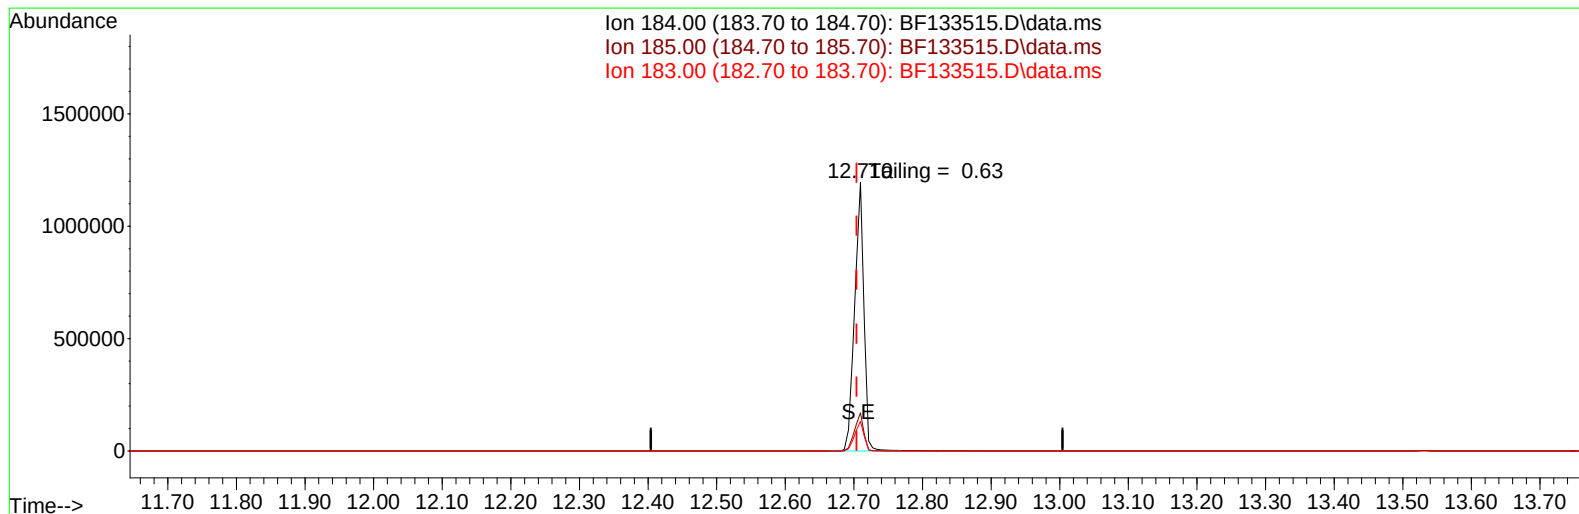

TIC: BF133515.D\data.ms

(77) Benzidine

12.710min (+ 0.006) 6348.38 ng m

response 1126304

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.20	14.26
183.00	10.90	11.07
0.00	0.00	0.00