


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF053023\
Data File : BF133515.D
Acq On : 30 May 2023 09:43
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF052523.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Tue May 30 12:58:40 2023

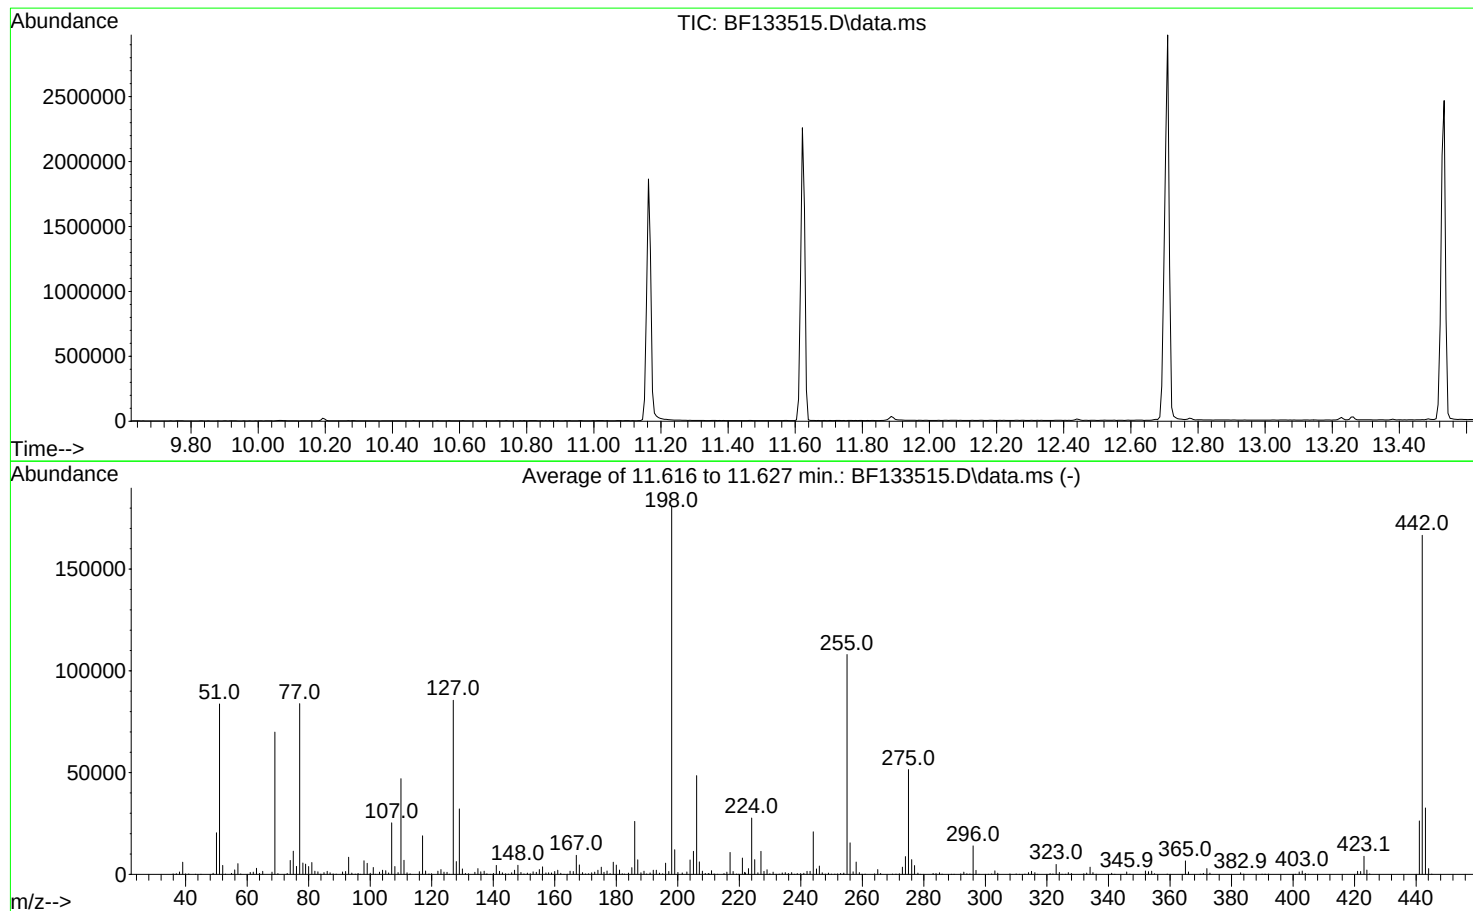

AutoFind: Scans 1620, 1621, 1622; Background Corrected with Scan 1615

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	46.3	83781	PASS
68	69	0.00	2	1.6	1122	PASS
69	198	0.00	100	38.7	69883	PASS
70	69	0.00	2	0.6	428	PASS
127	198	10	80	47.3	85587	PASS
197	198	0.00	2	0.8	1389	PASS
198	198	100	100	100.0	180773	PASS
199	198	5	9	6.7	12119	PASS
275	198	10	60	28.5	51525	PASS
365	198	1	100	3.6	6597	PASS
441	198	0.01	100	14.5	26248	PASS
442	442	50	100	100.0	166635	PASS
443	442	15	24	19.6	32673	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
5/30/2023	BNA_F	<u>BF133515.D</u>
Compound Name	Response	Retention Time
DDT	404494	13.533
DDD	6898	13.227
DDE	150	12.892
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
7048	411542	1.71

Instrument :
BNA_F
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF053023\
 Data File : BF133515.D
 Acq On : 30 May 2023 09:43
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Quant Time: May 30 12:49:17 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF052523.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu May 25 23:30:55 2023
 Response via : Initial Calibration

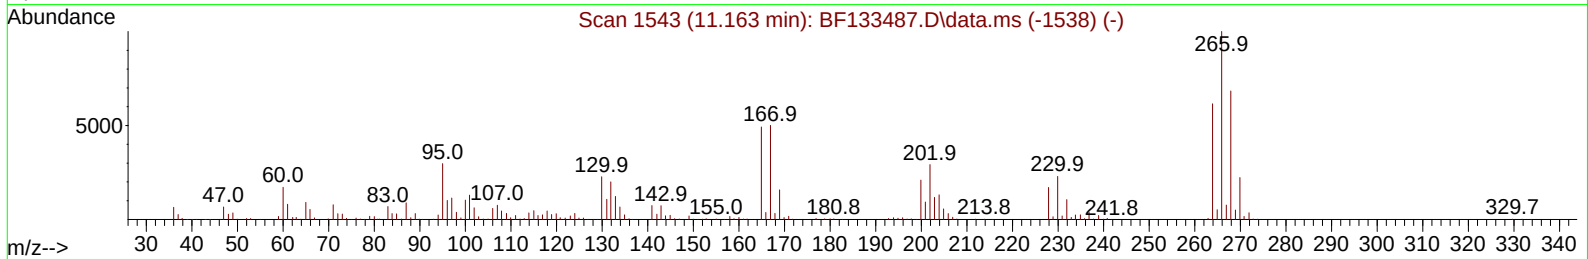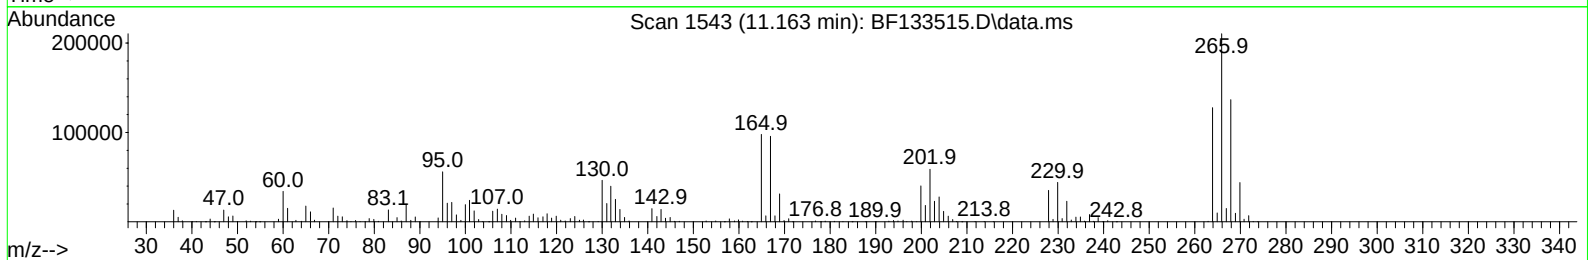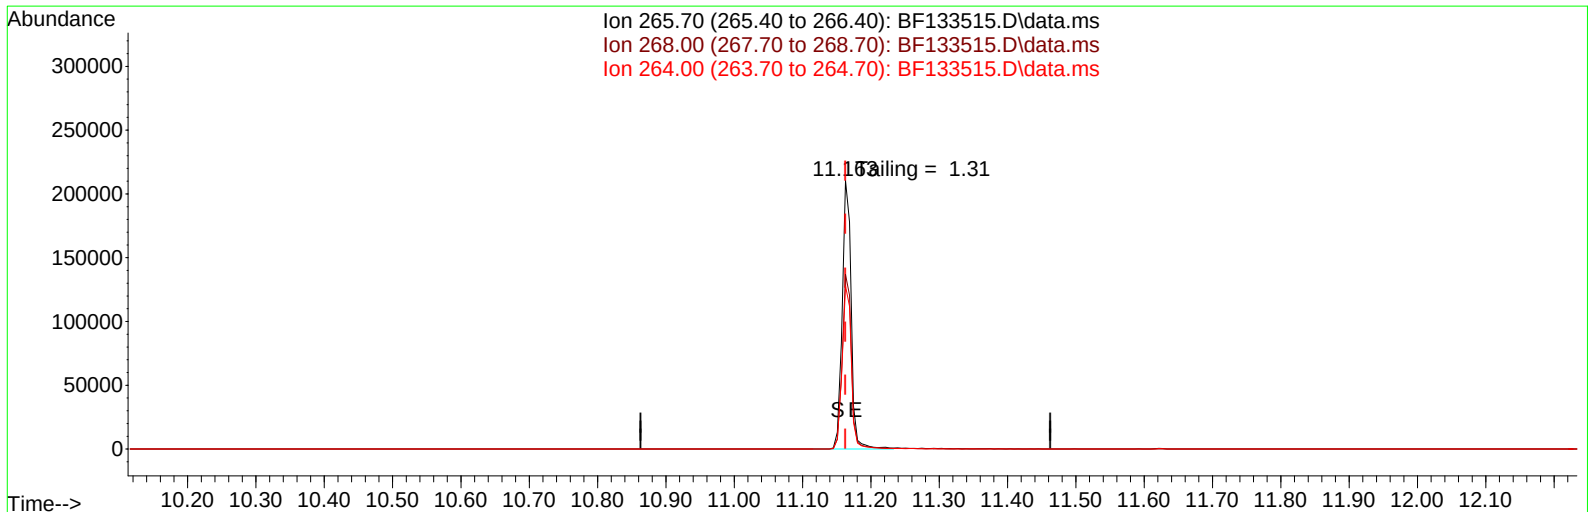

TIC: BF133515.D\data.ms

(70) Pentachlorophenol (C)

11.163min (-0.000) 417388.07 ng




response 191245

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	68.30	64.96
264.00	61.50	60.73
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF053023\
Data File : BF133515.D
Acq On : 30 May 2023 09:43
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: May 30 12:49:17 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF052523.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu May 25 23:30:55 2023
Response via : Initial Calibration

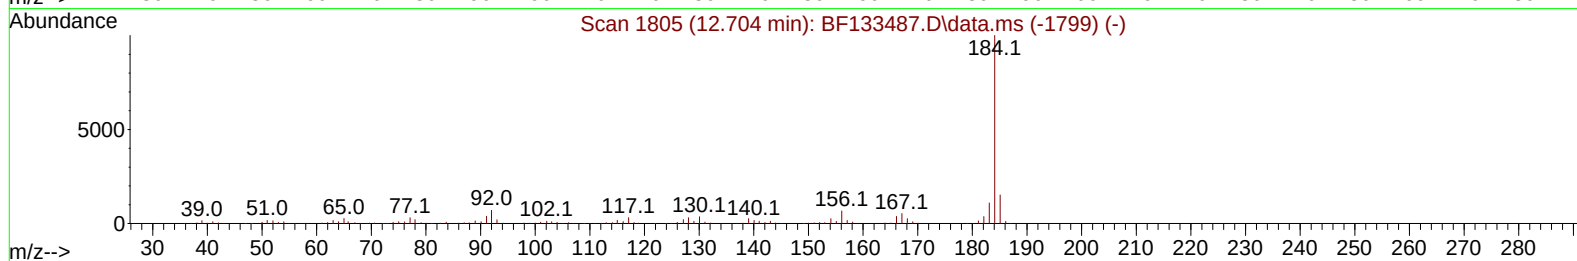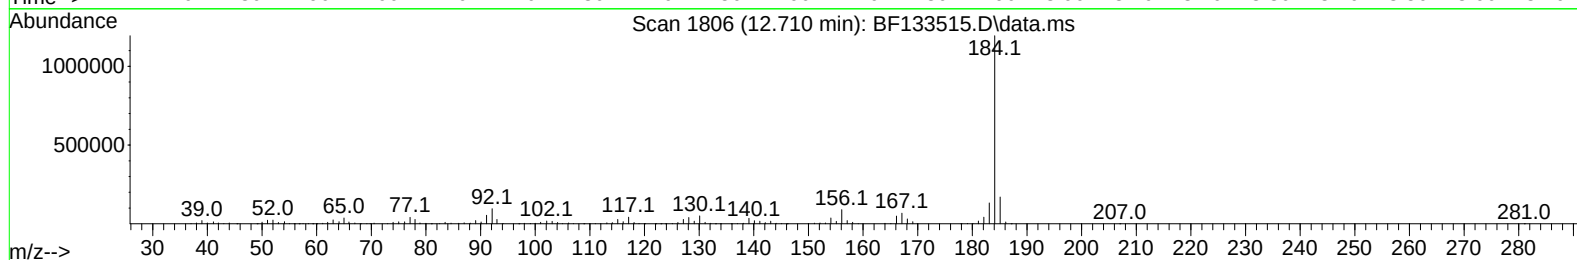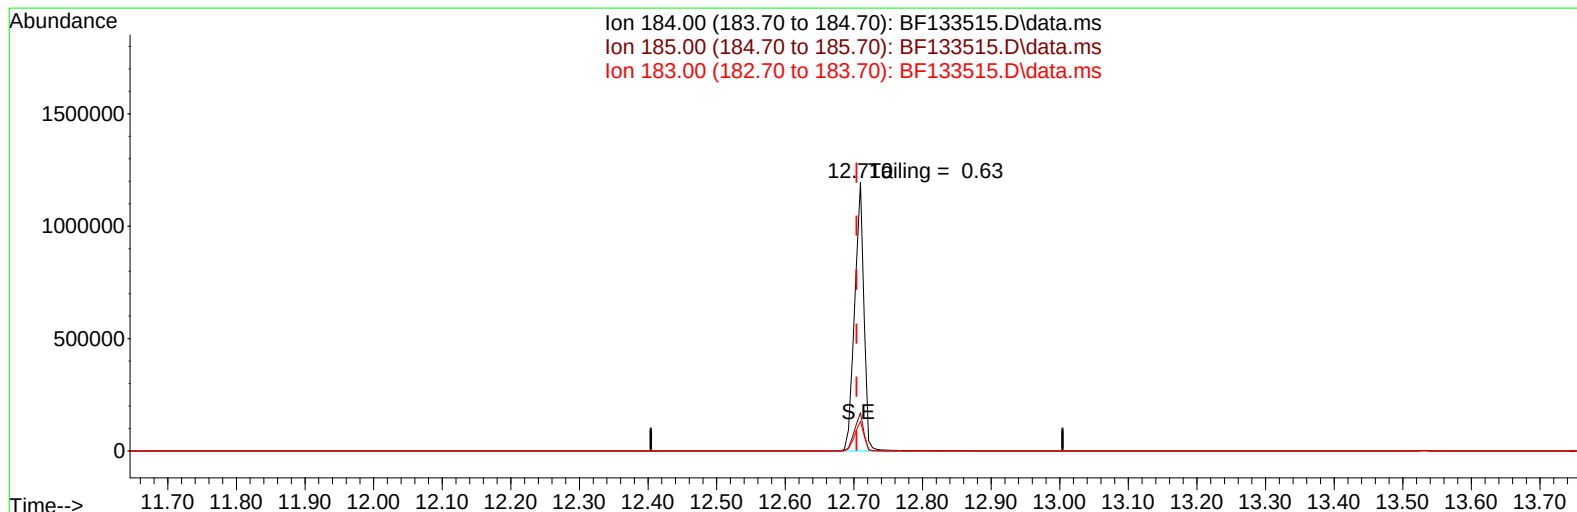

TIC: BF133515.D\data.ms

(77) Benzidine

12.710min (+ 0.006) 6348.38 ng m

response 1126304

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.20	14.26
183.00	10.90	11.07
0.00	0.00	0.00