
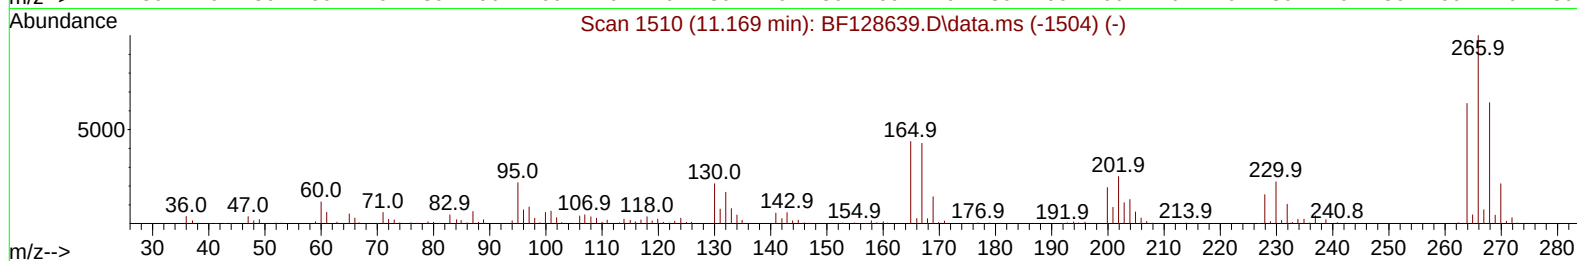
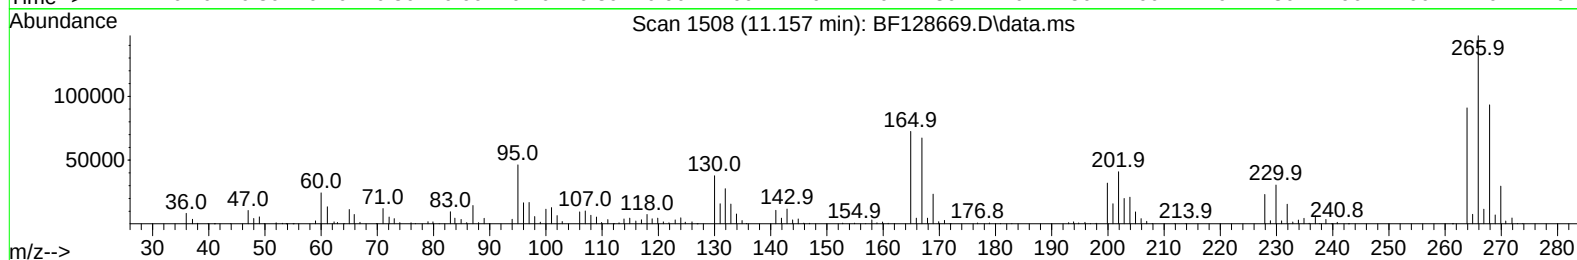


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF060322\
 Data File : BF128669.D
 Acq On : 03 Jun 2022 09:45
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 04 05:06:54 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF060222.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Jun 02 17:07:23 2022
 Response via : Initial Calibration

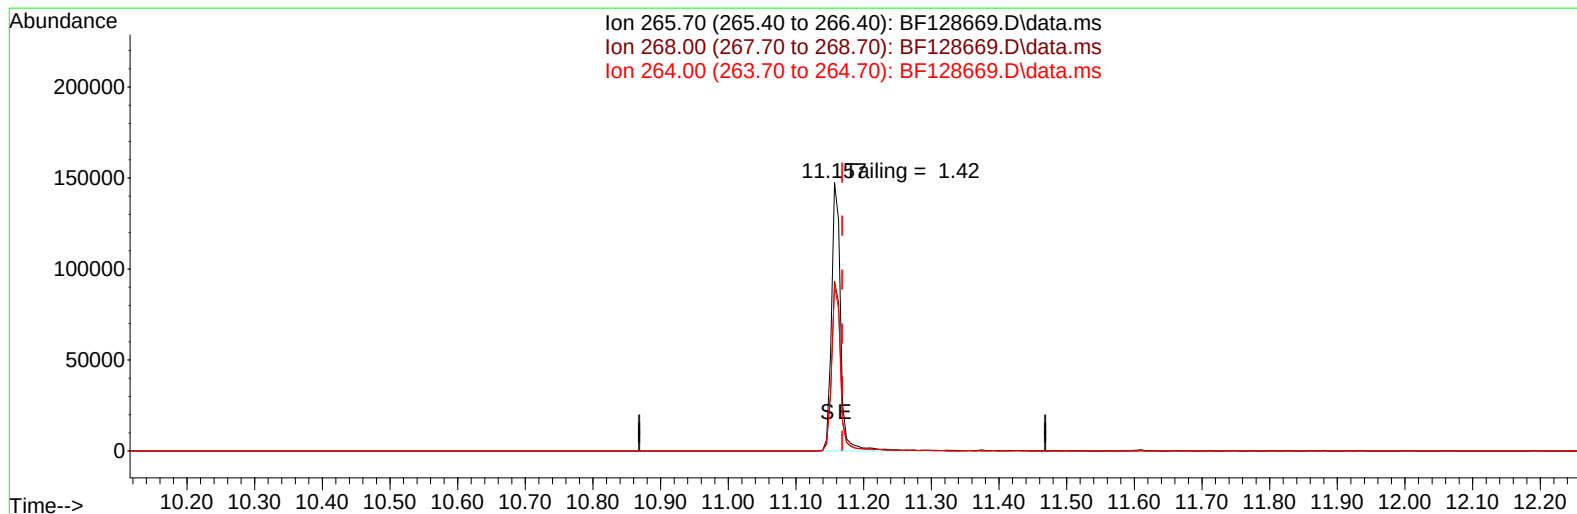

TIC: BF128669.D\data.ms

(70) Pentachlorophenol (C)




11.157min (-0.012) 31770.93 ng

response 136705

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.70	63.24
264.00	61.80	61.68
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF060322\
 Data File : BF128669.D
 Acq On : 03 Jun 2022 09:45
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 04 05:06:54 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF060222.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Jun 02 17:07:23 2022
 Response via : Initial Calibration

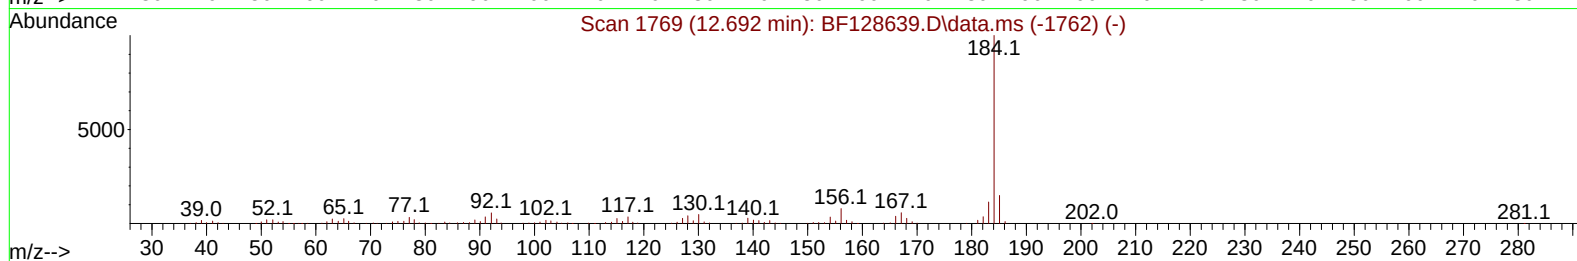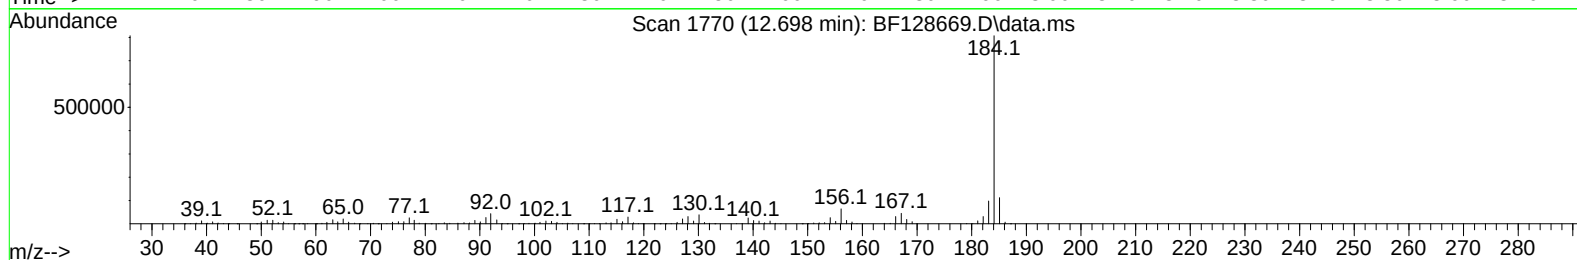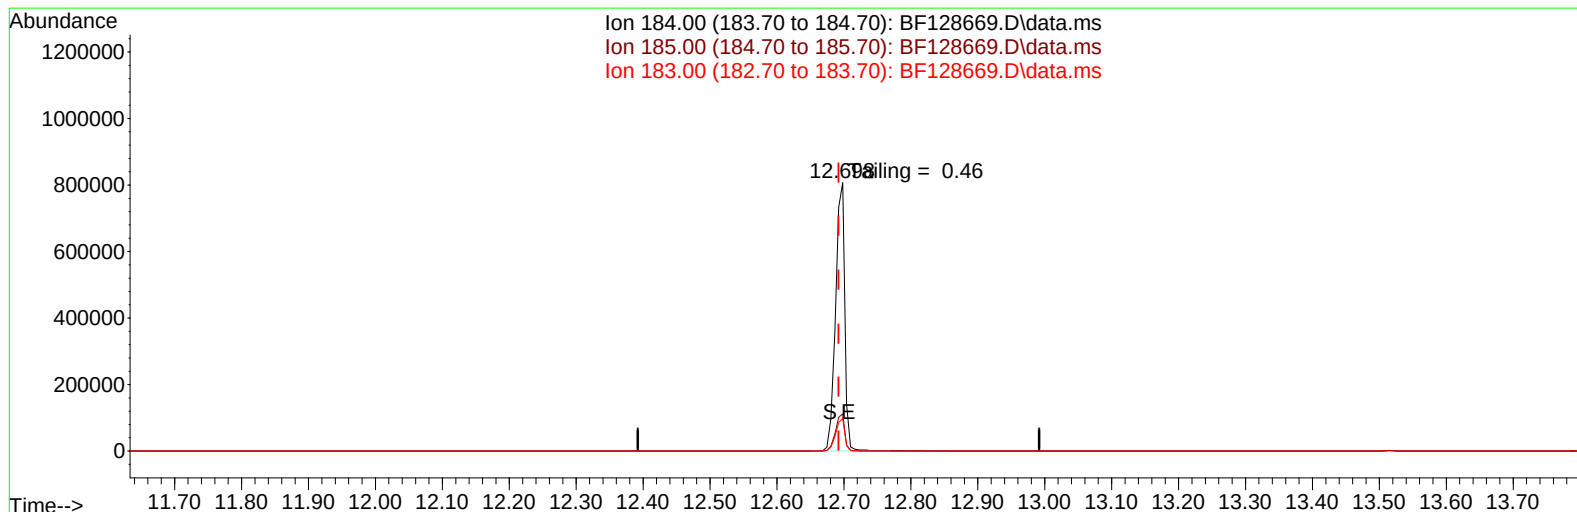

TIC: BF128669.D\data.ms

(77) Benzidine

12.698min (+ 0.006) 0.00 ng

response 773975

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.90	13.88
183.00	11.60	12.12
0.00	0.00	0.00