


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF060322\
 Data File : BF128669.D
 Acq On : 03 Jun 2022 09:45
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF060222.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Jun 02 17:07:23 2022

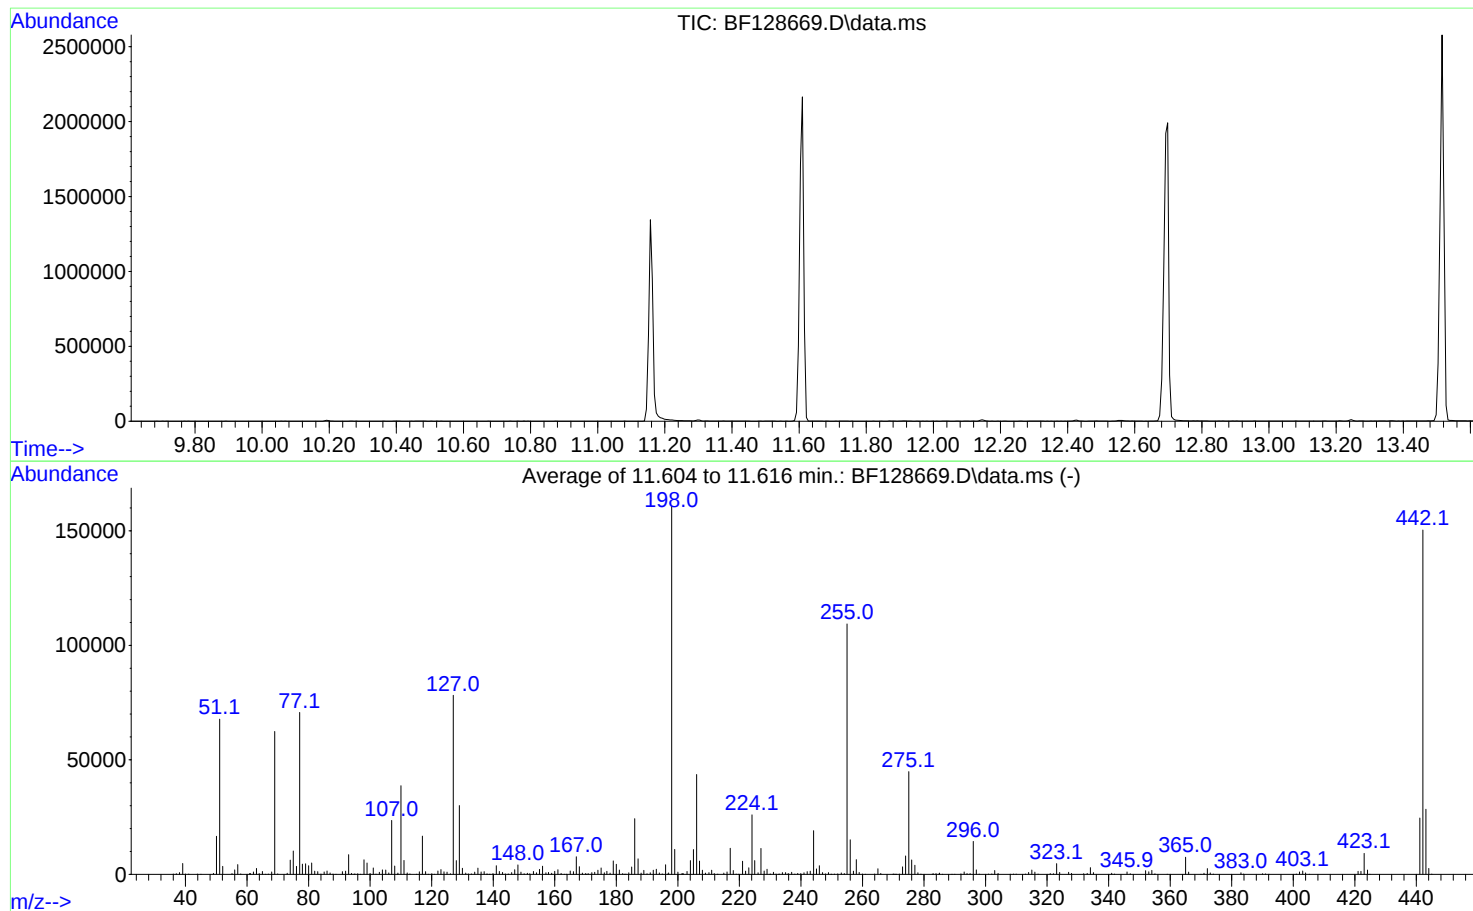




AutoFind: Scans 1584, 1585, 1586; Background Corrected with Scan 1578

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	42.2	67772	PASS
68	69	0.00	2	1.7	1080	PASS
69	198	0.00	100	38.8	62377	PASS
70	69	0.00	2	0.4	225	PASS
127	198	10	80	48.7	78155	PASS
197	198	0.00	2	0.4	667	PASS
198	198	100	100	100.0	160637	PASS
199	198	5	9	6.8	10899	PASS
275	198	10	60	27.9	44843	PASS
365	198	1	100	4.7	7498	PASS
441	198	0.01	100	15.3	24613	PASS
442	442	50	100	100.0	150349	PASS
443	442	15	24	18.9	28419	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF060322\
Data File : BF128669.D
Acq On : 03 Jun 2022 09:45
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Jun 04 05:06:54 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF060222.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jun 02 17:07:23 2022
Response via : Initial Calibration

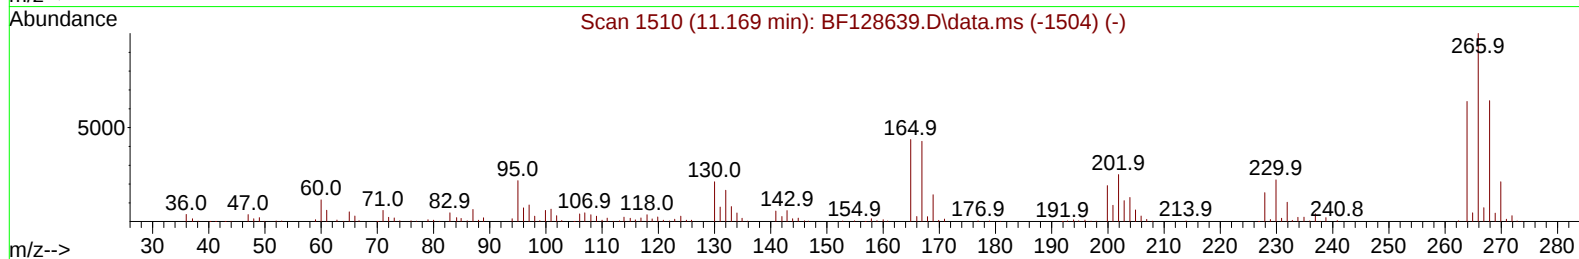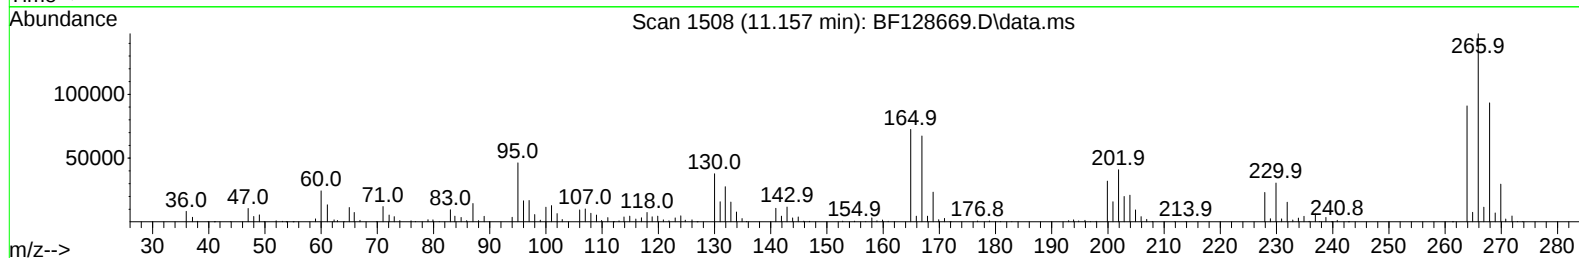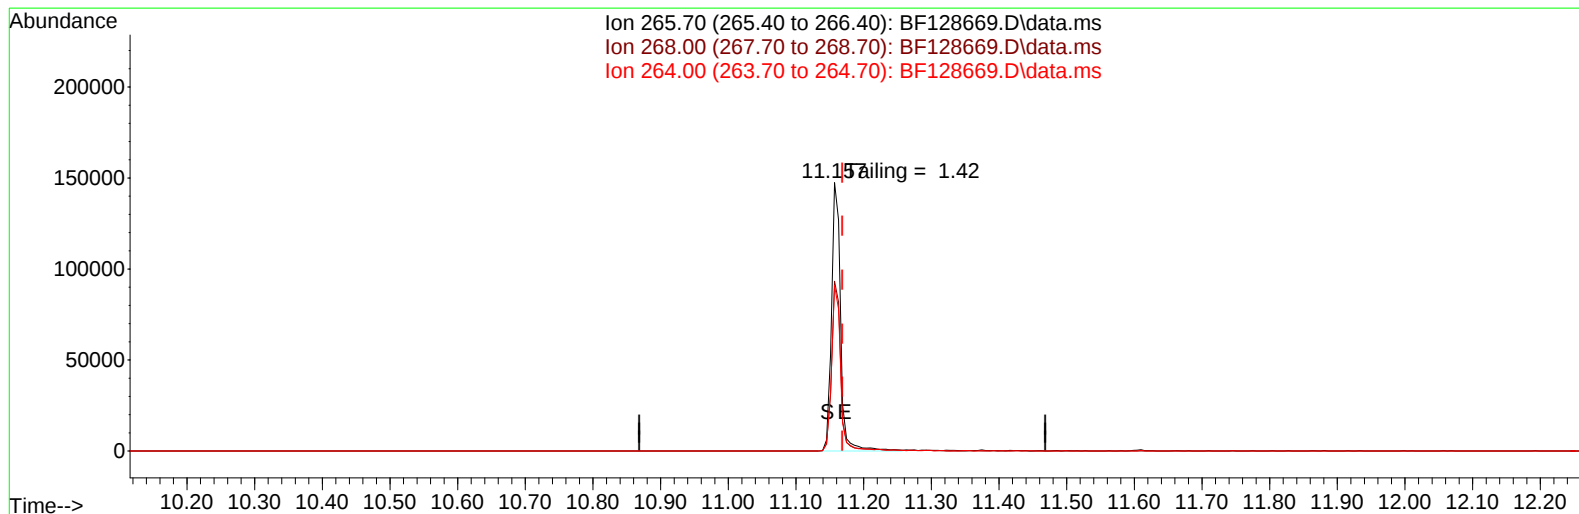

TIC: BF128669.D\data.ms

(70) Pentachlorophenol (C)

11.157min (-0.012) 31770.93 ng




response 136705

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.70	63.24
264.00	61.80	61.68
0.00	0.00	0.00

```
Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF060322\  
Data File : BF128669.D  
Acq On    : 03 Jun 2022  09:45  
Operator  : CG\JU  
Sample    : DFTPP  
Misc      :  
ALS Vial  : 1    Sample Multiplier: 1
```

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Jun 04 05:06:54 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF060222.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jun 02 17:07:23 2022
Response via : Initial Calibration

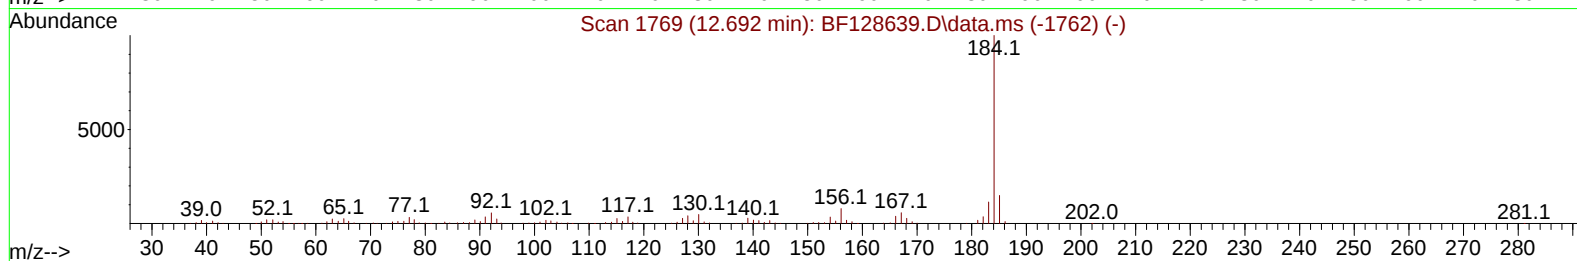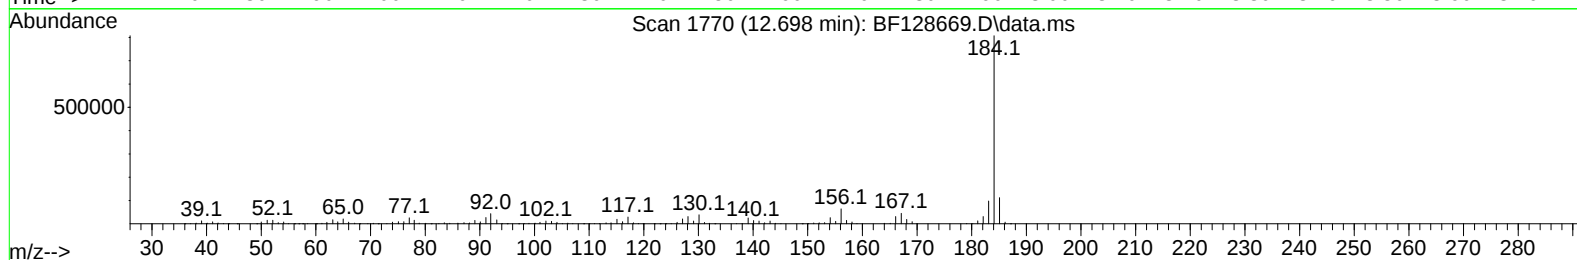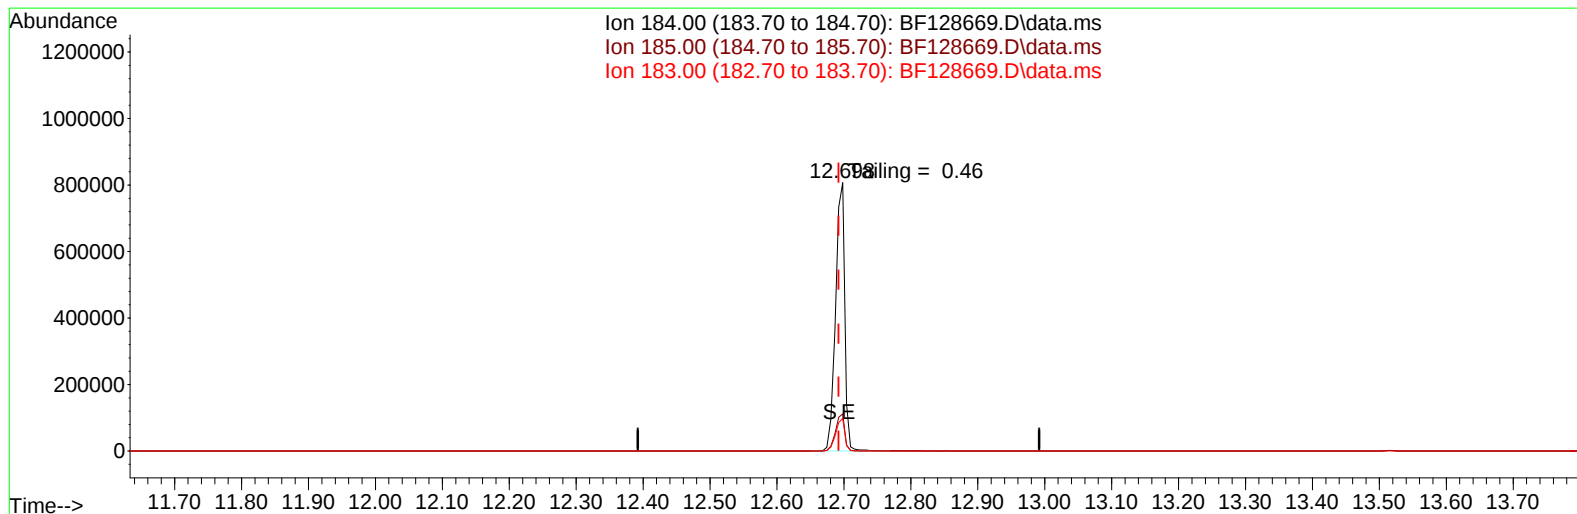

TIC: BF128669.D\data.ms

(77) Benzidine

12.698min (+ 0.006) 0.00 ng

response **773975**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.90	13.88
183.00	11.60	12.12
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
6/3/2022	BNA_F	<u>BF128669.D</u>
Compound Name	Response	Retention Time
DDT	392052	13.516
DDD	2075	13.245
DDE	208	12.874
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
2283	394335	0.58

Instrument :
BNA_F
ClientSampleId :
DFTPP