
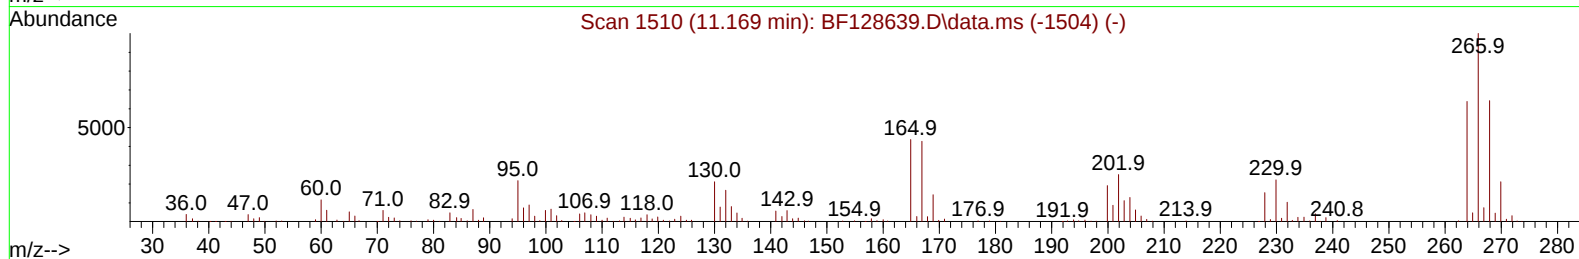
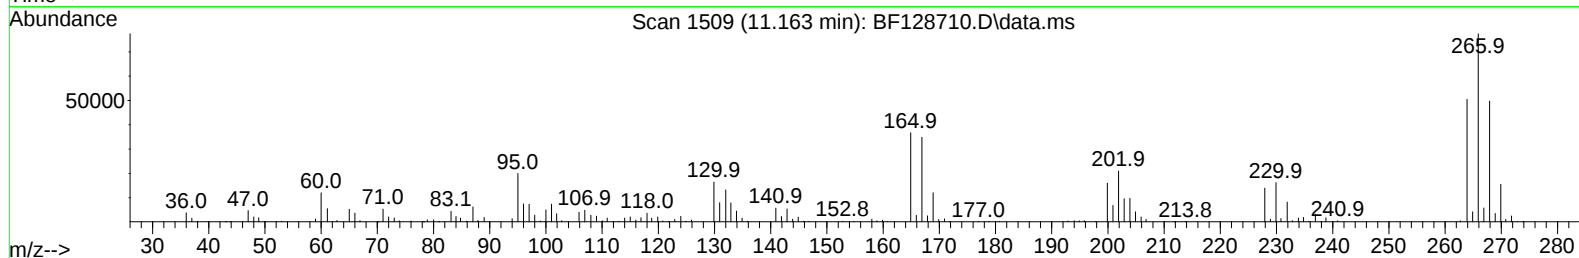


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF060722\
Data File : BF128710.D
Acq On : 07 Jun 2022 10:51
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 08 05:12:17 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF060222.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jun 02 17:07:23 2022
Response via : Initial Calibration

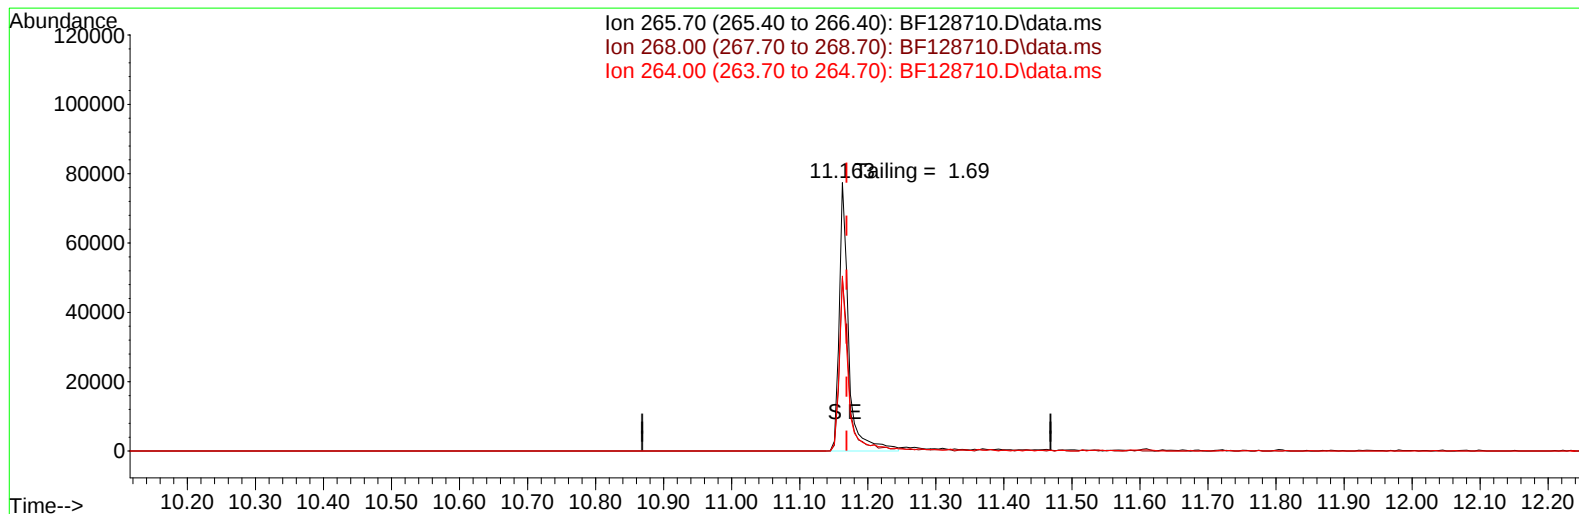

TIC: BF128710.D\data.ms

(70) Pentachlorophenol (C)




11.163min (-0.006) 17126.04 ng

response 74961

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.70	64.26
264.00	61.80	65.15
0.00	0.00	0.00

```
Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF060722\  
Data File : BF128710.D  
Acq On    : 07 Jun 2022  10:51  
Operator  : CG\JU  
Sample    : DFTPP  
Misc      :  
ALS Vial  : 1    Sample Multiplier: 1
```

Quant Time: Jun 08 05:12:17 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF060222.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jun 02 17:07:23 2022
Response via : Initial Calibration

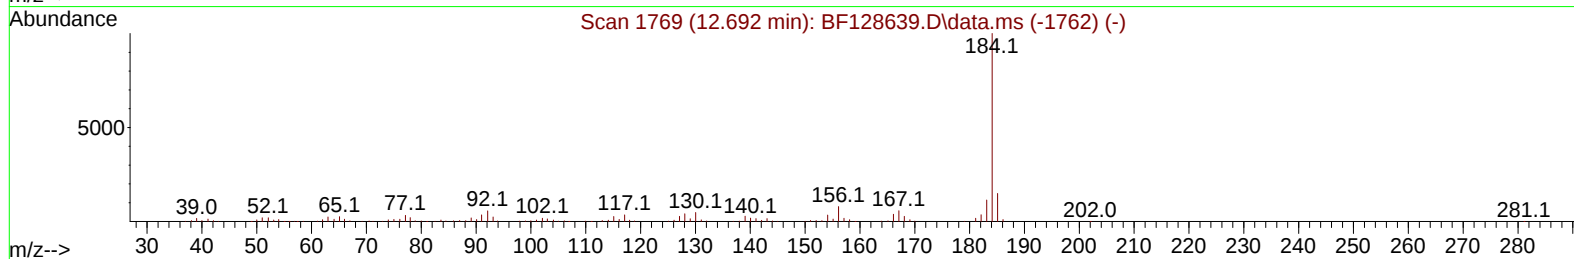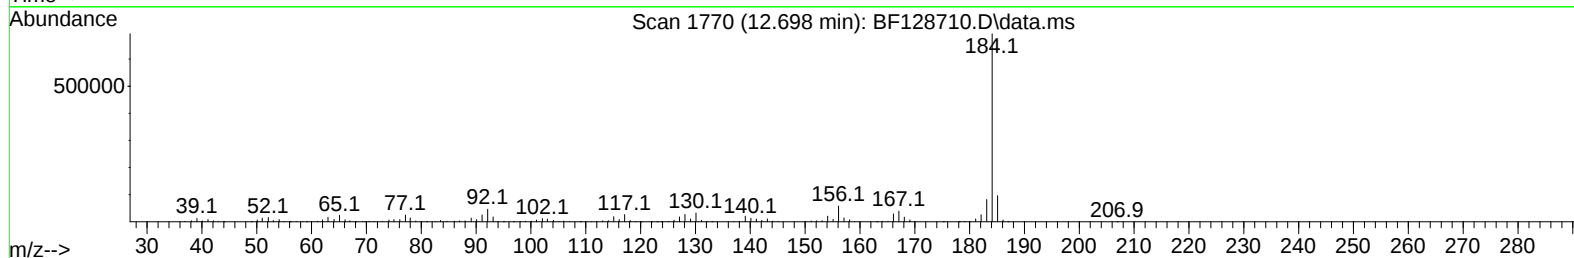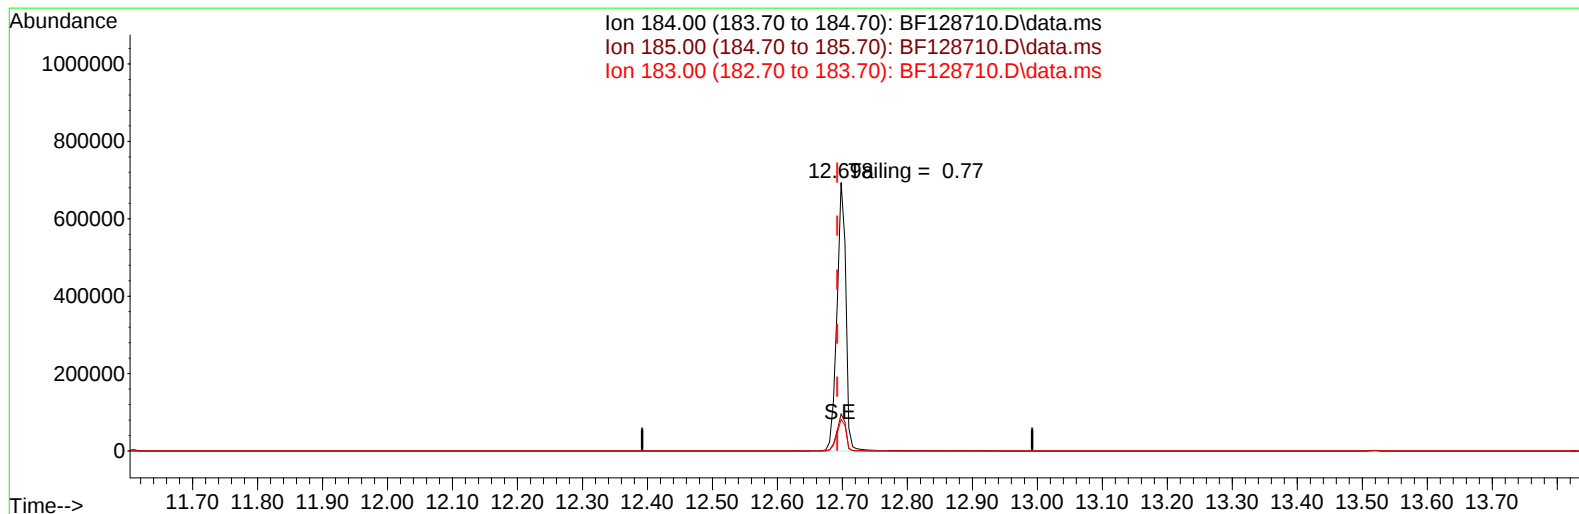

TIC: BF128710.D\data.ms

(77) Benzidine

12.698min (+ 0.006) 0.00 ng

response **662765**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.90	13.92
183.00	11.60	11.82
0.00	0.00	0.00