

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF060722\
 Data File : BF128712.D
 Acq On : 07 Jun 2022 12:18
 Operator : CG\JU
 Sample : PB145347BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB145347BL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF060222.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF128712.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.481	540	543	558	rVB	3270445	3034292	81.44%	14.053%
2	6.493	711	715	729	rBV	2988632	2764635	74.20%	12.804%
3	6.822	767	771	774	rBV	741283	571308	15.33%	2.646%
4	7.392	861	868	871	rBV	1734907	1903620	51.09%	8.817%
5	8.104	984	989	993	rBV	801932	733637	19.69%	3.398%
6	9.186	1167	1173	1176	rBV	3928286	3529432	94.73%	16.346%
7	9.863	1282	1288	1291	rBV	1018441	846189	22.71%	3.919%
8	10.657	1417	1423	1426	rBV	2235605	2116750	56.81%	9.804%
9	11.351	1537	1541	1544	rBV	1096669	872788	23.43%	4.042%
10	12.945	1807	1812	1815	rBV	3948987	3725770	100.00%	17.256%
11	13.998	1987	1991	1994	rBV	725922	694006	18.63%	3.214%
12	14.092	2002	2007	2013	rBV	122018	146264	3.93%	0.677%
13	15.463	2235	2240	2249	rBV	470200	602401	16.17%	2.790%
14	16.939	2483	2491	2493	rBV6	18434	50372	1.35%	0.233%




Sum of corrected areas: 21591464

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF060722\
Data File : BF128712.D
Acq On : 07 Jun 2022 12:18
Operator : CG\JU
Sample : PB145347BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB145347BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF060222.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

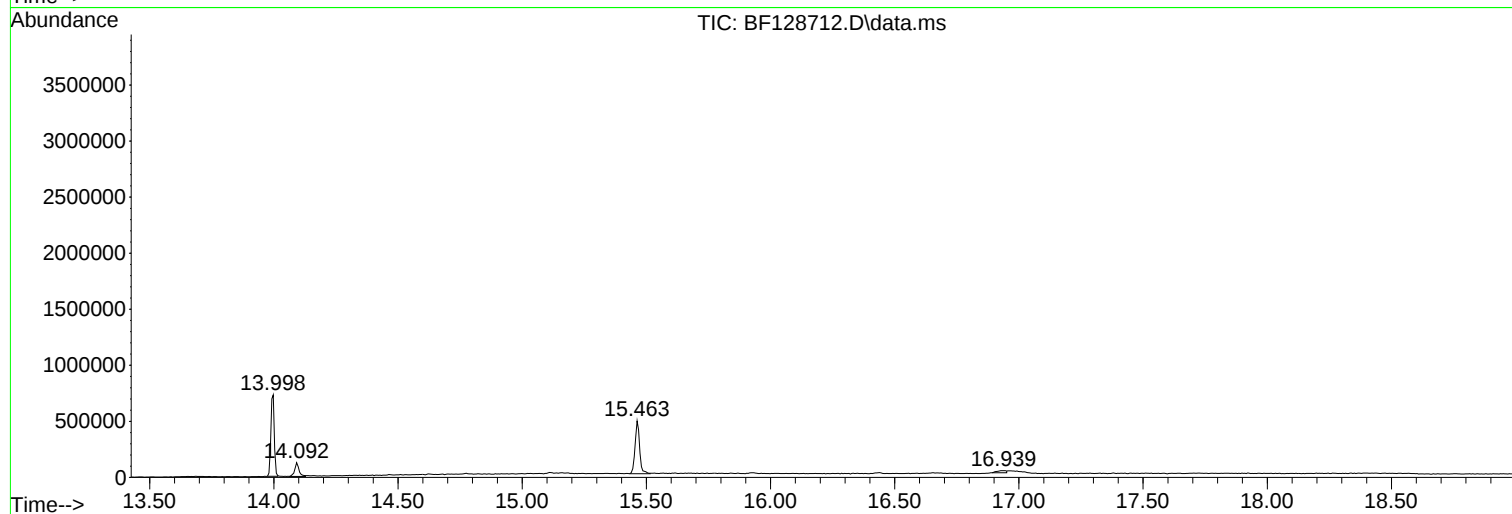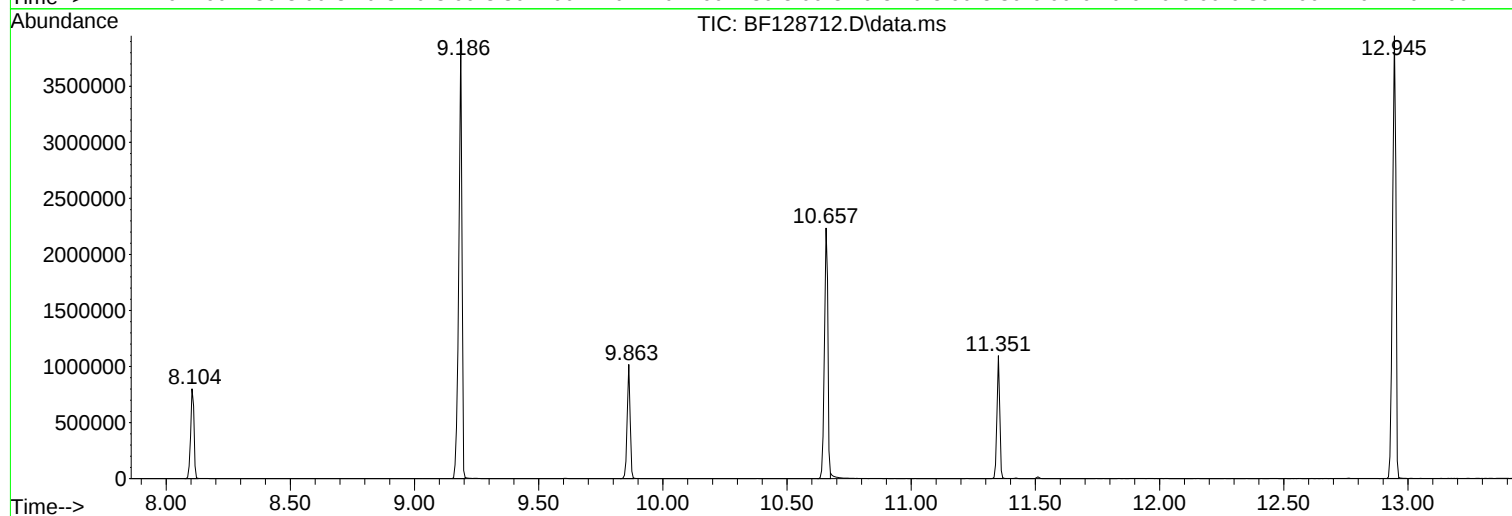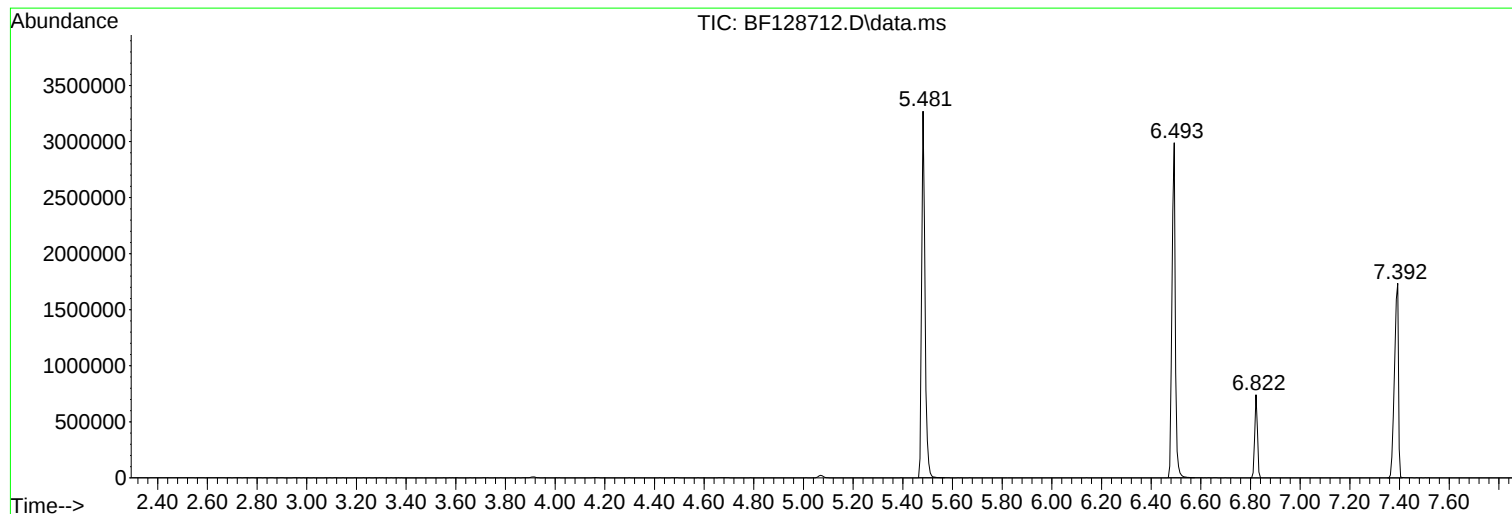

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF060722\
Data File : BF128712.D
Acq On : 07 Jun 2022 12:18
Operator : CG\JU
Sample : PB145347BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB145347BL










Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF060222.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Triphenylphosphine oxide Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
14.092	4.22 ng	146264	Chrysene-d12	13.998

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Triphenylphosphine oxide	278	C18H15OP	000791-28-6	91
2			(E)-7-Benzylidene-1-azabicyclo[3...	293	C15H19NO3S	1000483-83-4	53
3			Formaldehyde, (triphenylphosphor...	304	C19H17N2P	015990-54-2	45
4			Furo[3,2-c]quinoline, 8-bromo-2,...	277	C13H12BrNO	1000310-92-7	37
5			Carbazol-1-one, 1,2,3,4-tetrahyd...	277	C18H15NO2	299962-12-2	37

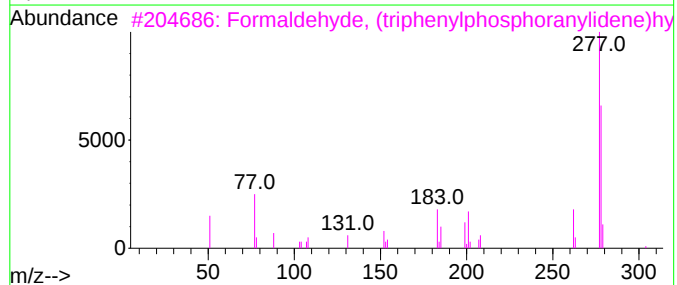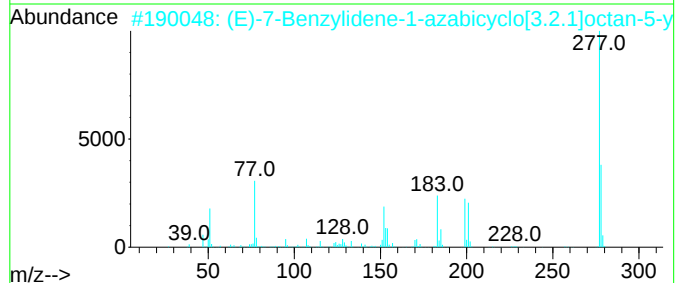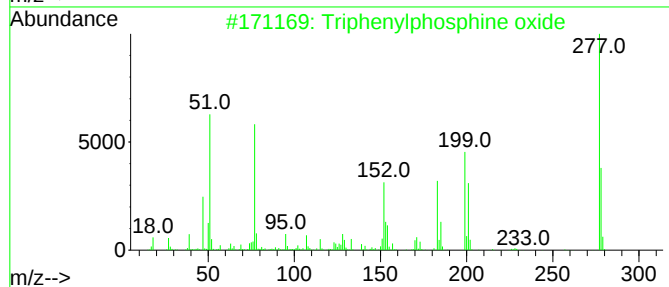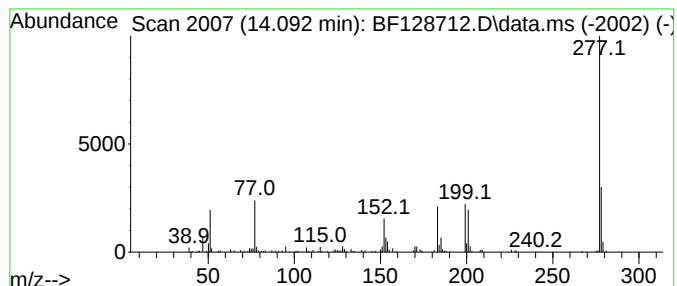

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF060722\
Data File : BF128712.D
Acq On : 07 Jun 2022 12:18
Operator : CG\JU
Sample : PB145347BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB145347BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF060222.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Triphenylphosph...	14.092	4.2	ng	146264	5	13.998	694006	20.0