

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF060722\
 Data File : BF128719.D
 Acq On : 07 Jun 2022 16:47
 Operator : CG\JU
 Sample : N3209-14
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 WC-14B-2-1-GR

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF060222.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF128719.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	4.128	303	313	317	rBV2	390488	613555	16.51%	0.564%
2	4.463	363	370	379	rVB4	429515	632774	17.03%	0.581%
3	4.869	431	439	445	rVB	498833	637155	17.14%	0.585%
4	4.952	450	453	455	rVV	501992	672463	18.09%	0.618%
5	4.975	455	457	462	rVV	673447	645850	17.38%	0.593%
6	5.028	462	466	470	rVV	1094039	1180409	31.76%	1.084%
7	5.228	494	500	503	rBV2	986436	1058045	28.47%	0.972%
8	5.410	529	531	537	rVV4	263618	443915	11.94%	0.408%
9	5.475	537	542	545	rVV	1074202	1158711	31.18%	1.064%
10	5.593	558	562	567	rVV2	594443	987329	26.57%	0.907%
11	5.634	567	569	572	rVV	974814	786744	21.17%	0.723%
12	5.675	572	576	583	rVV2	562563	790802	21.28%	0.726%
13	5.846	598	605	608	rVB4	794316	1151668	30.99%	1.058%
14	5.893	608	613	616	rBV	486148	716151	19.27%	0.658%
15	5.981	624	628	632	rVB3	1163801	1527710	41.11%	1.403%
16	6.022	632	635	638	rBV2	410635	532482	14.33%	0.489%
17	6.075	640	644	650	rVB2	2550020	2899901	78.03%	2.664%
18	6.128	650	653	656	rBV	1211015	1007608	27.11%	0.926%
19	6.263	670	676	679	rBV	1292504	1584675	42.64%	1.456%
20	6.357	688	692	700	rBV4	1302670	2163472	58.21%	1.987%
21	6.440	700	706	709	rBV3	291808	468538	12.61%	0.430%
22	6.487	709	714	718	rBV3	1128595	1677418	45.13%	1.541%
23	6.569	723	728	732	rBV5	977974	1846849	49.69%	1.697%
24	6.604	732	734	740	rVB2	756070	886815	23.86%	0.815%
25	6.663	740	744	745	rBV3	433309	445809	12.00%	0.410%
26	6.681	745	747	750	rVB2	549466	487034	13.10%	0.447%
27	6.763	754	761	763	rBV6	375202	683442	18.39%	0.628%
28	6.840	767	774	778	rVB2	1856166	2737813	73.67%	2.515%
29	6.887	778	782	784	rBV	552800	600565	16.16%	0.552%
30	6.922	784	788	789	rBV2	472315	544935	14.66%	0.501%
31	6.975	794	797	801	rVB	1785619	1664204	44.78%	1.529%
32	7.057	808	811	813	rBV2	560991	579341	15.59%	0.532%
33	7.098	815	818	822	rVB2	1133042	1237040	33.29%	1.136%
34	7.222	833	839	842	rBV3	940007	1058954	28.49%	0.973%
35	7.251	842	844	850	rVB5	443523	591010	15.90%	0.543%
36	7.363	856	863	865	rBV2	1777059	2545545	68.49%	2.338%

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF060722\
 Data File : BF128719.D
 Acq On : 07 Jun 2022 16:47
 Operator : CG\JU
 Sample : N3209-14
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 WC-14B-2-1-GR

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF060222.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

37	7.387	865	867	869	rBV2	472727	435235	11.71%	0.400%
38	7.469	877	881	885	rBV5	1022224	1605677	43.20%	1.475%
39	7.528	885	891	895	rBV4	561574	1426105	38.37%	1.310%
40	7.581	897	900	902	rVV2	468746	573562	15.43%	0.527%

41	7.610	902	905	907	rVV2	831855	974173	26.21%	0.895%
42	7.634	907	909	912	rVB2	999403	778269	20.94%	0.715%
43	7.710	919	922	924	rBV3	473161	596670	16.05%	0.548%
44	7.728	924	925	927	rVV	825829	664501	17.88%	0.610%
45	7.751	927	929	933	rVB3	1181702	1036722	27.90%	0.952%

46	7.793	933	936	938	rVB3	390891	474069	12.76%	0.436%
47	7.851	943	946	948	rBV	1123372	981240	26.40%	0.901%
48	7.928	956	959	964	rBV2	693138	811548	21.84%	0.746%
49	7.981	965	968	972	rVV3	663313	844030	22.71%	0.775%
50	8.051	977	980	981	rVV2	552667	551570	14.84%	0.507%

51	8.069	981	983	985	rVV3	629937	709183	19.08%	0.651%
52	8.110	985	990	993	rVV5	1101199	2335964	62.85%	2.146%
53	8.175	996	1001	1003	rVV2	2341628	2571343	69.19%	2.362%
54	8.204	1003	1006	1008	rVV2	752580	742242	19.97%	0.682%
55	8.269	1013	1017	1019	rBV3	409858	533135	14.35%	0.490%

56	8.316	1022	1025	1028	rVB2	924534	893545	24.04%	0.821%
57	8.404	1032	1040	1043	rBV5	1561265	2060917	55.45%	1.893%
58	8.463	1047	1050	1052	rBV3	460837	480077	12.92%	0.441%
59	8.498	1052	1056	1058	rVB4	533094	622112	16.74%	0.572%
60	8.540	1058	1063	1065	rBV	2440520	2379086	64.01%	2.186%

61	8.575	1068	1069	1072	rVB2	736299	553926	14.90%	0.509%
62	8.616	1073	1076	1079	rBV2	622726	596950	16.06%	0.548%
63	8.657	1079	1083	1085	rBV3	1113088	1212103	32.61%	1.113%
64	8.704	1089	1091	1095	rBV3	333233	536962	14.45%	0.493%
65	8.804	1104	1108	1111	rVB3	1315035	1614291	43.44%	1.483%

66	8.892	1120	1123	1126	rBV5	551445	817349	21.99%	0.751%
67	8.992	1137	1140	1142	rBV4	589144	672902	18.11%	0.618%
68	9.022	1142	1145	1149	rVV4	1006816	1123185	30.22%	1.032%
69	9.110	1157	1160	1162	rVV2	443979	450418	12.12%	0.414%
70	9.139	1162	1165	1170	rVV	3048170	2646385	71.21%	2.431%

71	9.187	1170	1173	1175	rVB	1278322	956488	25.74%	0.879%
72	9.275	1184	1188	1192	rBV4	989638	1407219	37.86%	1.293%
73	9.387	1205	1207	1211	rVB5	377238	450113	12.11%	0.413%
74	9.463	1217	1220	1222	rVB2	804835	678253	18.25%	0.623%
75	9.528	1229	1231	1234	rBV	1120329	1007173	27.10%	0.925%

76	9.598	1237	1243	1245	rVB2	2752715	3079741	82.87%	2.829%
----	-------	------	------	------	------	---------	---------	--------	--------

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF060722\
 Data File : BF128719.D
 Acq On : 07 Jun 2022 16:47
 Operator : CG\JU
 Sample : N3209-14
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 WC-14B-2-1-GR

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF060222.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

77	9.739	1263	1267	1270	rVB2	596584	709314	19.09%	0.652%
78	9.781	1271	1274	1277	rVB2	890201	865148	23.28%	0.795%
79	9.845	1282	1285	1286	rBV3	519675	581229	15.64%	0.534%
80	9.869	1287	1289	1292	rVB2	1132885	963152	25.92%	0.885%
81	9.975	1304	1307	1312	rVB2	655852	778852	20.96%	0.715%
82	10.016	1312	1314	1319	rBV5	343519	628013	16.90%	0.577%
83	10.069	1320	1323	1327	rVV3	975709	1228498	33.06%	1.129%
84	10.116	1328	1331	1340	rVB4	1052689	1995127	53.68%	1.833%
85	10.192	1340	1344	1346	rBV2	839019	926063	24.92%	0.851%
86	10.239	1350	1352	1355	rVB2	515610	516560	13.90%	0.475%
87	10.281	1355	1359	1364	rBV4	892649	1219005	32.80%	1.120%
88	10.357	1370	1372	1377	rVB4	460684	586803	15.79%	0.539%
89	10.410	1378	1381	1383	rBV3	639927	712065	19.16%	0.654%
90	10.528	1397	1401	1405	rVB	2228453	2334726	62.82%	2.145%
91	10.569	1406	1408	1413	rVB3	465807	608377	16.37%	0.559%
92	10.792	1442	1446	1449	rBV	3585627	3716497	100.00%	3.414%
93	11.257	1522	1525	1530	rVB	2835772	2793534	75.17%	2.566%
94	11.363	1540	1543	1545	rBV2	721409	743859	20.02%	0.683%
95	11.604	1581	1584	1587	rBV	816014	804779	21.65%	0.739%
96	12.339	1706	1709	1715	rVB	622362	782354	21.05%	0.719%
97	12.945	1808	1812	1815	rBV2	1271504	1299711	34.97%	1.194%
98	14.004	1989	1992	1995	rBV	700712	704421	18.95%	0.647%
99	14.333	2046	2048	2053	rVB2	529599	588715	15.84%	0.541%
100	15.480	2240	2243	2251	rVB	438999	637972	17.17%	0.586%




Sum of corrected areas: 108855938

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF060722\
Data File : BF128719.D
Acq On : 07 Jun 2022 16:47
Operator : CG\JU
Sample : N3209-14
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
WC-14B-2-1-GR

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF060222.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

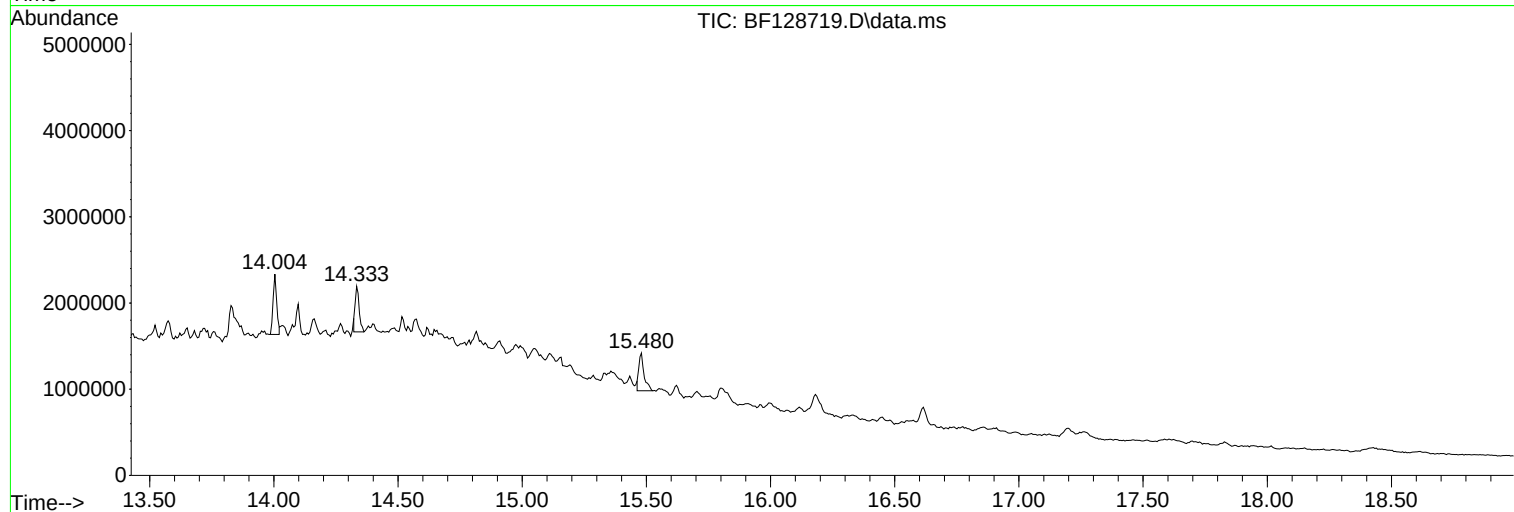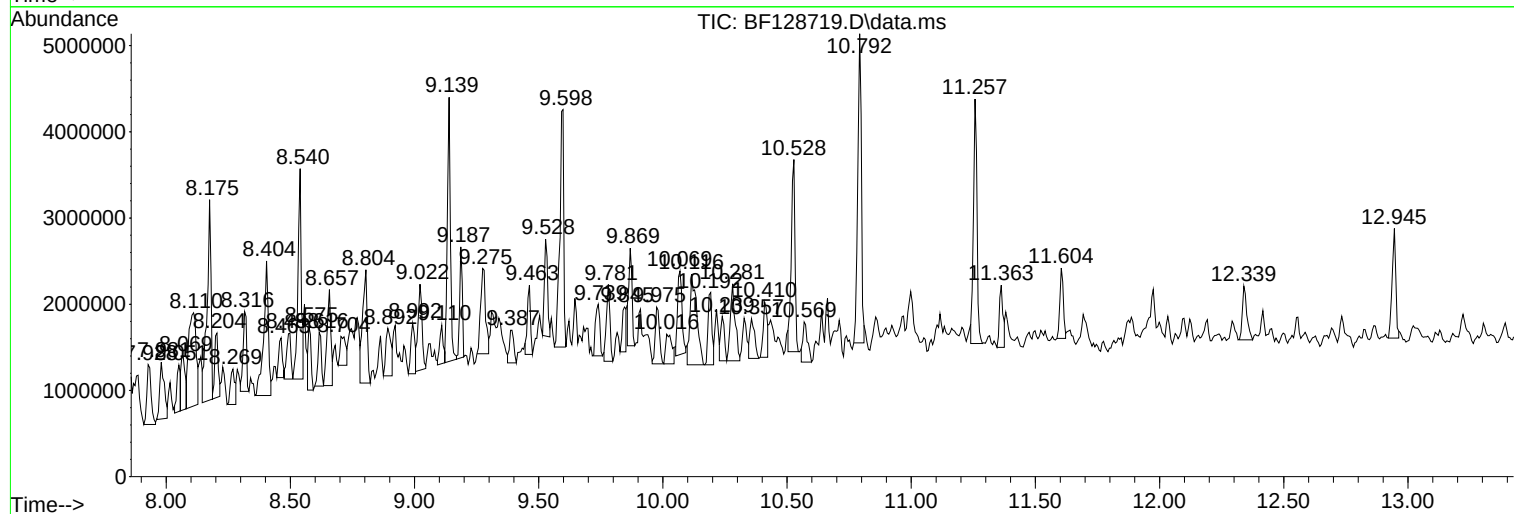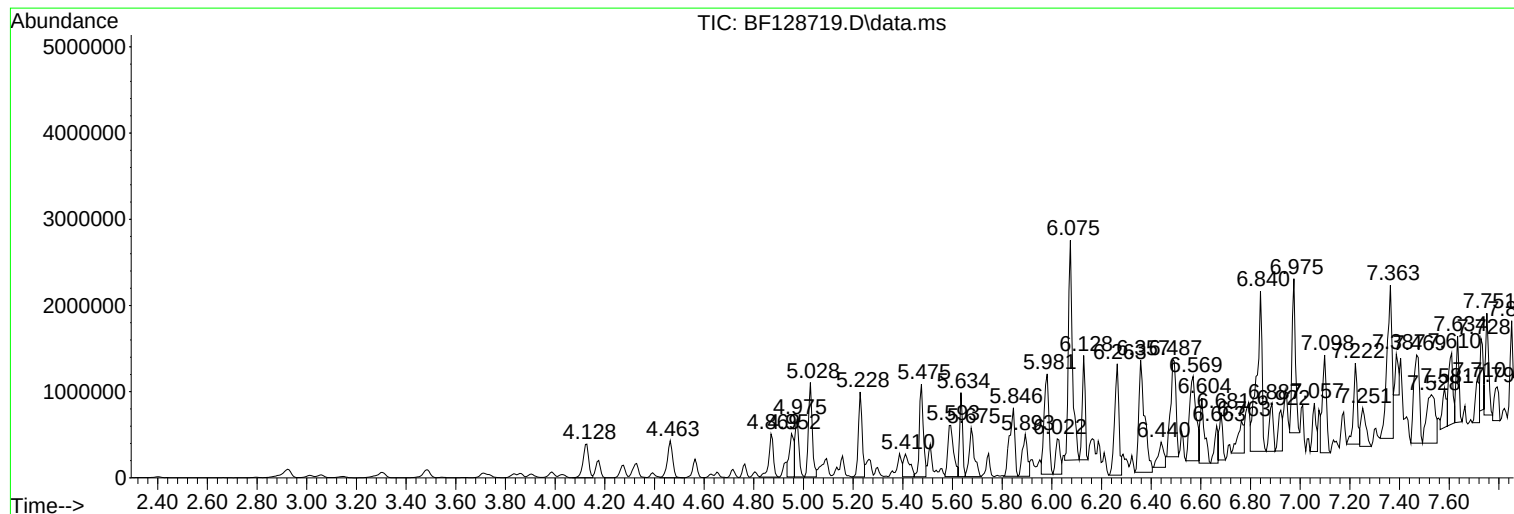

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF060722\
Data File : BF128719.D
Acq On : 07 Jun 2022 16:47
Operator : CG\JU
Sample : N3209-14
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
WC-14B-2-1-GR

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF060222.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF060722\
Data File : BF128719.D
Acq On : 07 Jun 2022 16:47
Operator : CG\JU
Sample : N3209-14
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
WC-14B-2-1-GR

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF060222.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------