


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF060722\
Data File : BF128710.D
Acq On : 07 Jun 2022 10:51
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF060222.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Wed Jun 08 14:28:39 2022

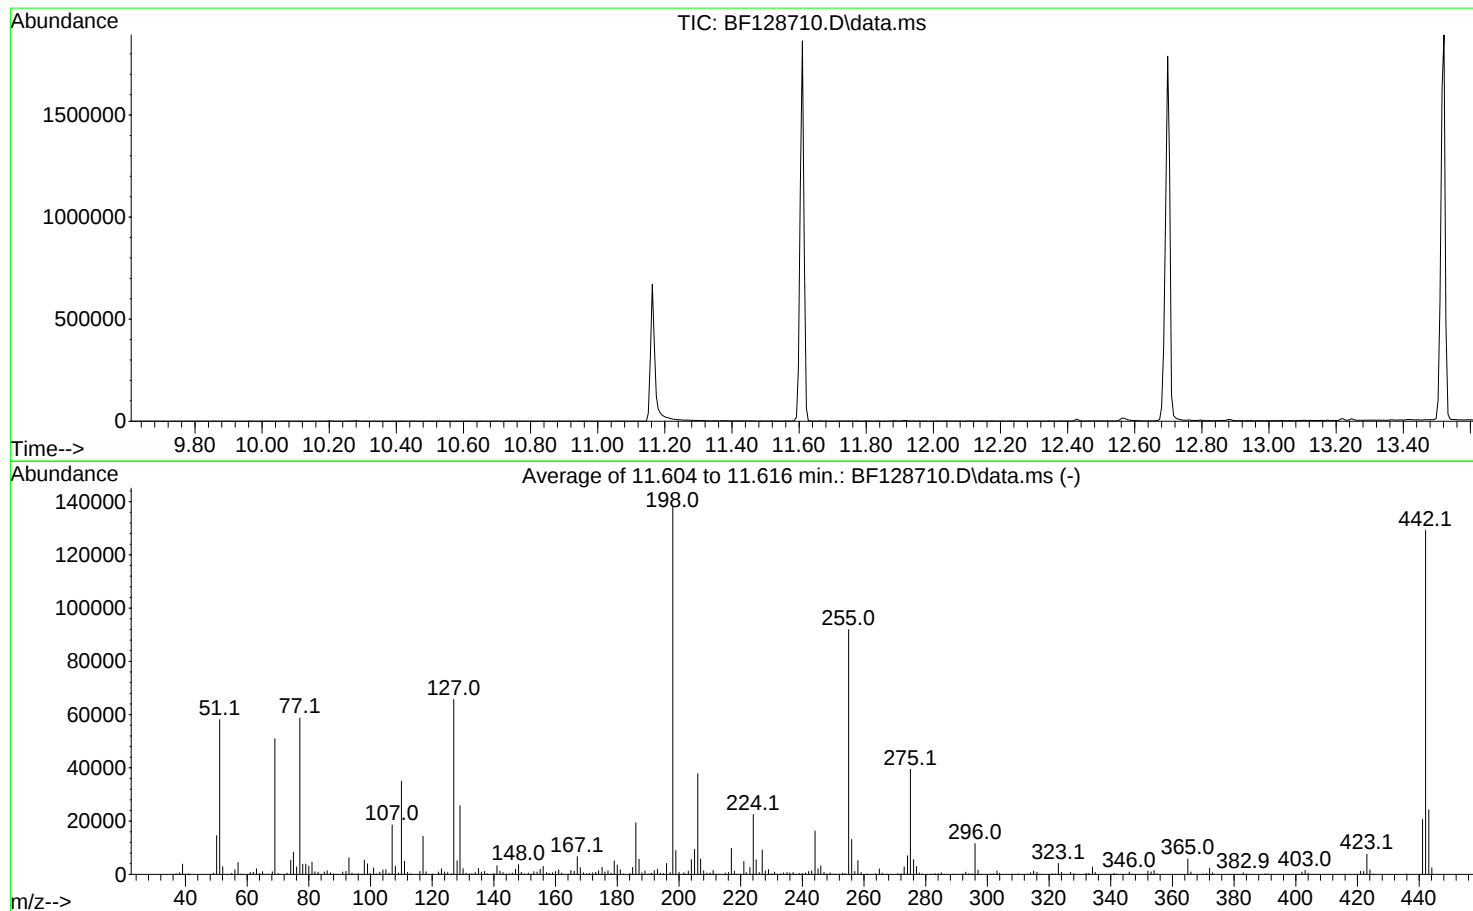




AutoFind: Scans 1584, 1585, 1586; Background Corrected with Scan 1579

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	42.1	58144	PASS
68	69	0.00	2	1.9	988	PASS
69	198	0.00	100	36.9	50989	PASS
70	69	0.00	2	0.6	296	PASS
127	198	10	80	47.6	65712	PASS
197	198	0.00	2	0.5	688	PASS
198	198	100	100	100.0	138171	PASS
199	198	5	9	6.5	8934	PASS
275	198	10	60	28.5	39413	PASS
365	198	1	100	4.2	5781	PASS
441	198	0.01	100	14.9	20626	PASS
442	442	50	100	100.0	129205	PASS
443	442	15	24	18.8	24253	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF060722\
Data File : BF128710.D
Acq On : 07 Jun 2022 10:51
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Jun 08 05:12:17 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF060222.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jun 02 17:07:23 2022
Response via : Initial Calibration

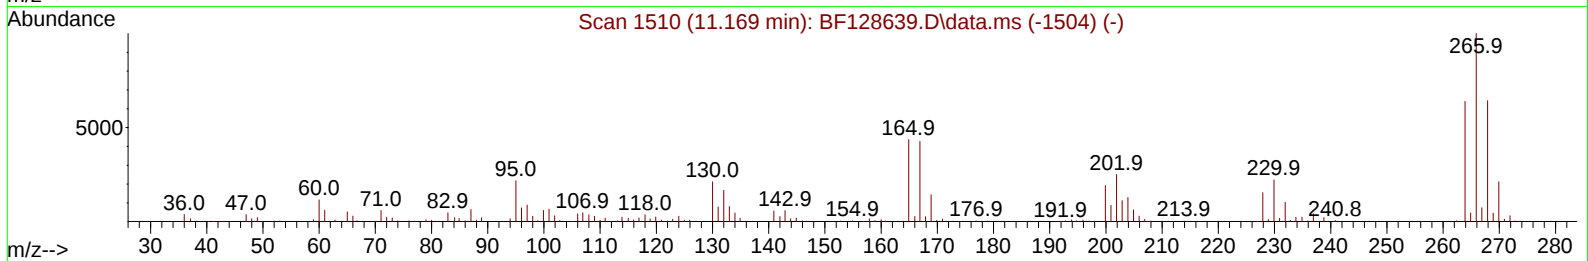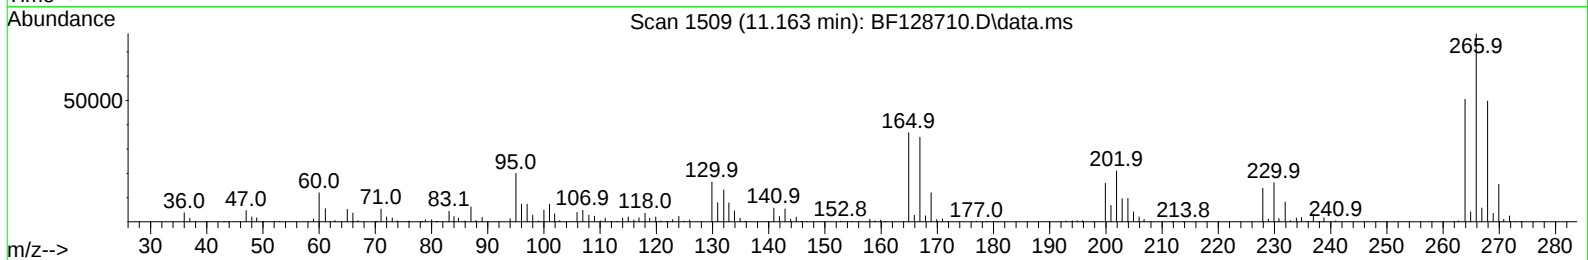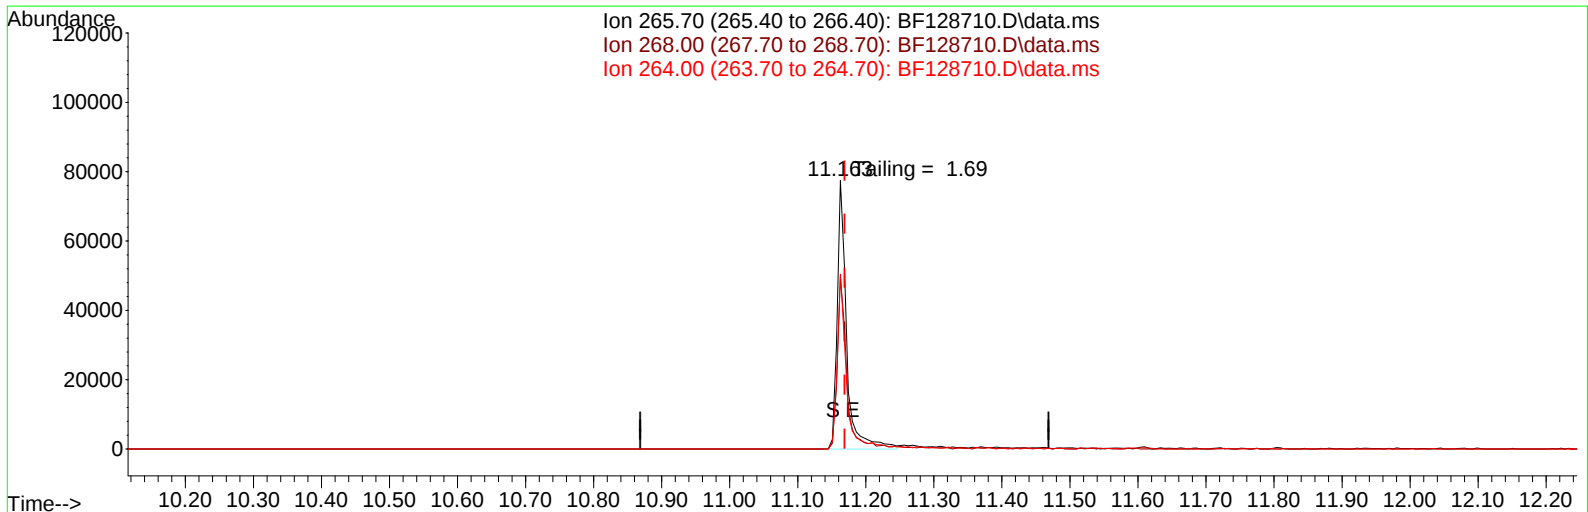

TIC: BF128710.D\data.ms

(70) Pentachlorophenol (C)

11.163min (-0.006) 17126.04 ng




response 74961

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.70	64.26
264.00	61.80	65.15
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF060722\
Data File : BF128710.D
Acq On : 07 Jun 2022 10:51
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Jun 08 05:12:17 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF060222.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jun 02 17:07:23 2022
Response via : Initial Calibration

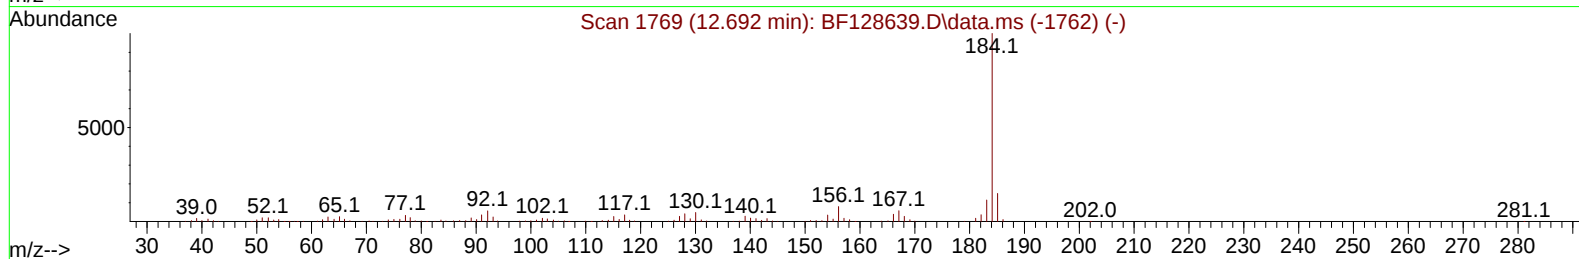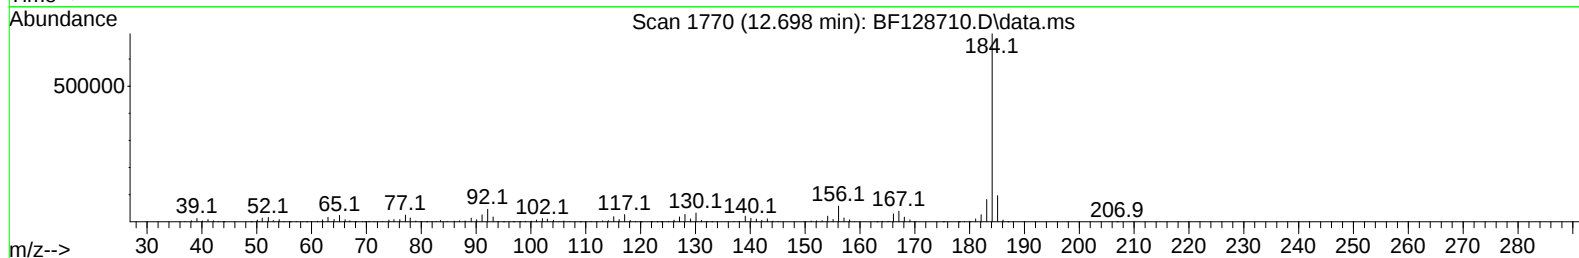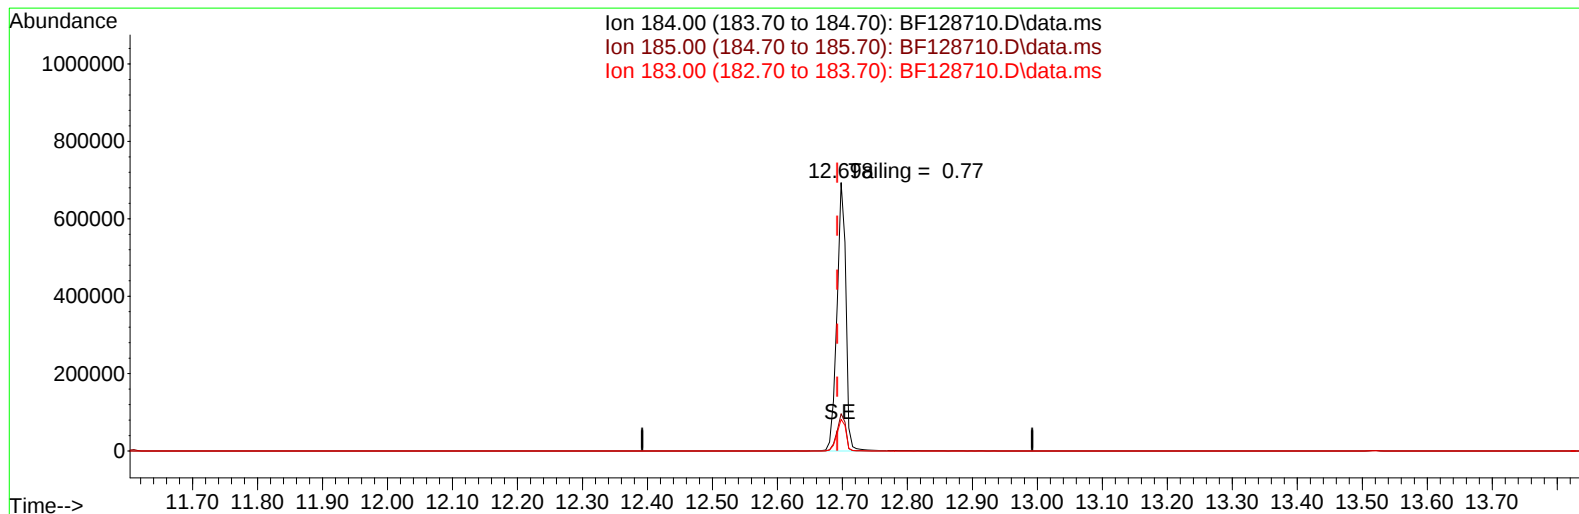

TIC: BF128710.D\data.ms

(77) Benzidine

12.698min (+ 0.006) 0.00 ng

response 662765

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.90	13.92
183.00	11.60	11.82
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
6/7/2022	BNA_F	<u>BF128710.D</u>
Compound Name	Response	Retention Time
DDT	317485	13.521
DDD	3730	13.216
DDE	1346	12.88
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
5076	322561	1.57

Instrument :
BNA_F
ClientSampleId :
DFTPP