
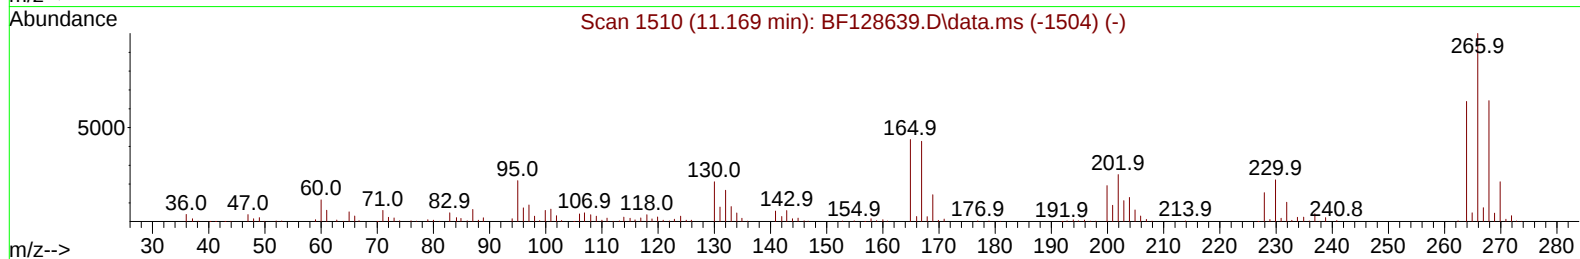
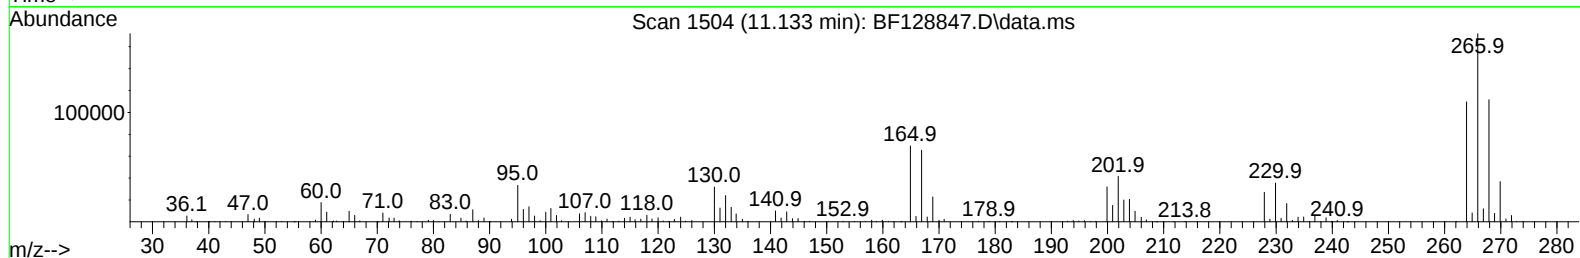


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF061722\
Data File : BF128847.D
Acq On : 17 Jun 2022 10:49
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 18 07:53:33 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF060222.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jun 14 14:53:53 2022
Response via : Initial Calibration

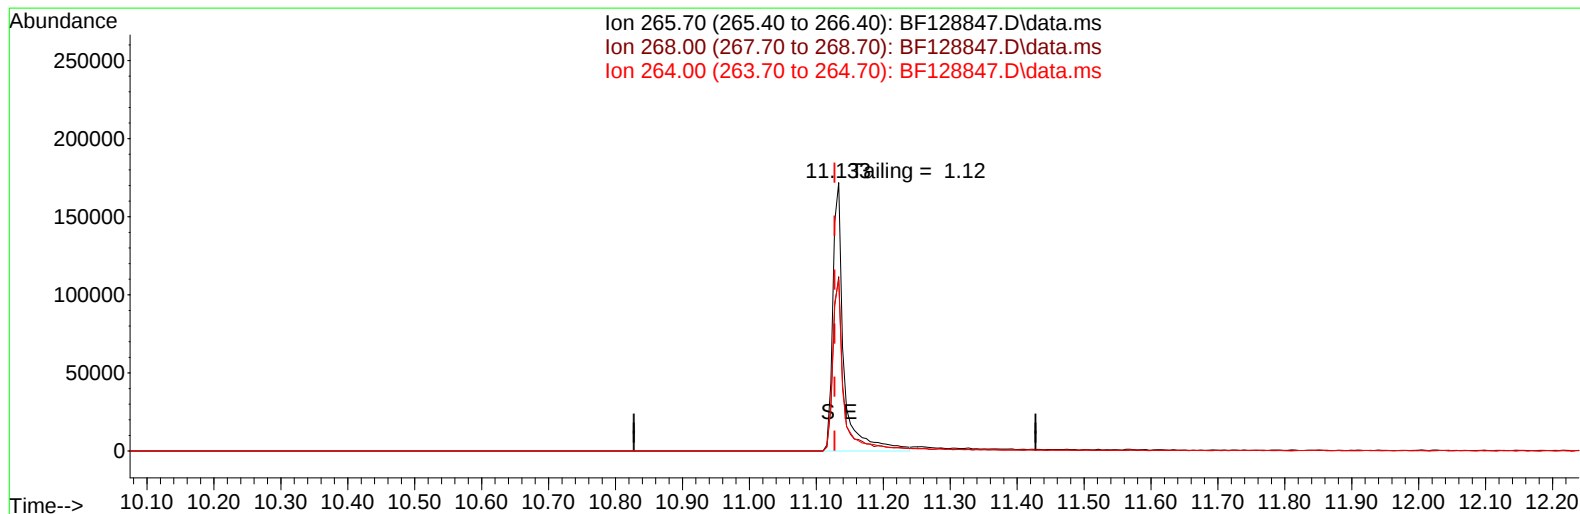

TIC: BF128847.D\data.ms

(70) Pentachlorophenol (C)




11.133min (+ 0.006) 38263.38 ng

response 198468

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.70	64.94
264.00	61.80	63.77
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF061722\
Data File : BF128847.D
Acq On : 17 Jun 2022 10:49
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 18 07:53:33 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF060222.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jun 14 14:53:53 2022
Response via : Initial Calibration

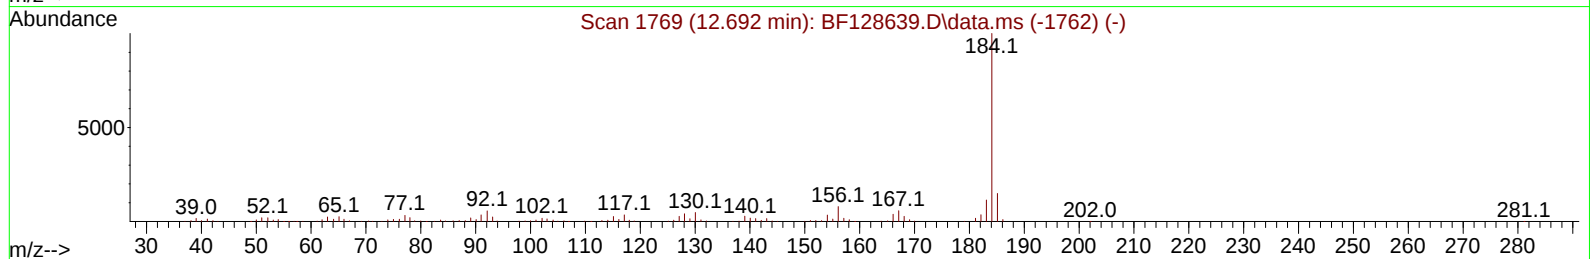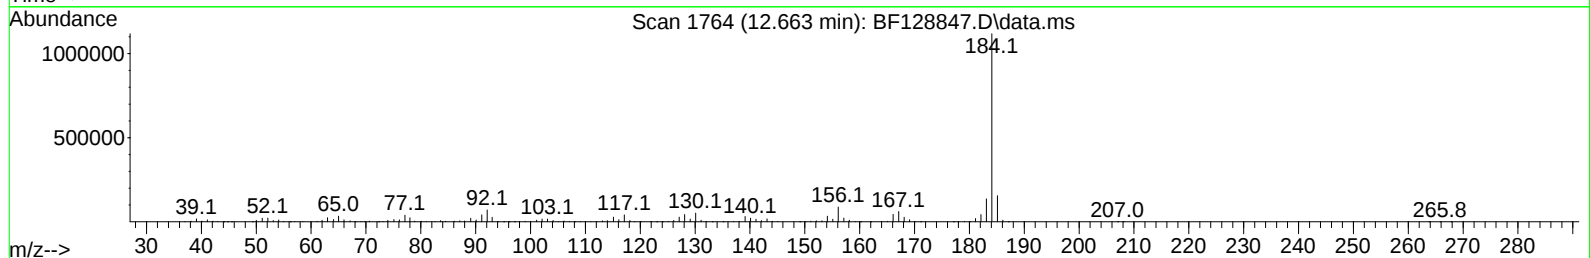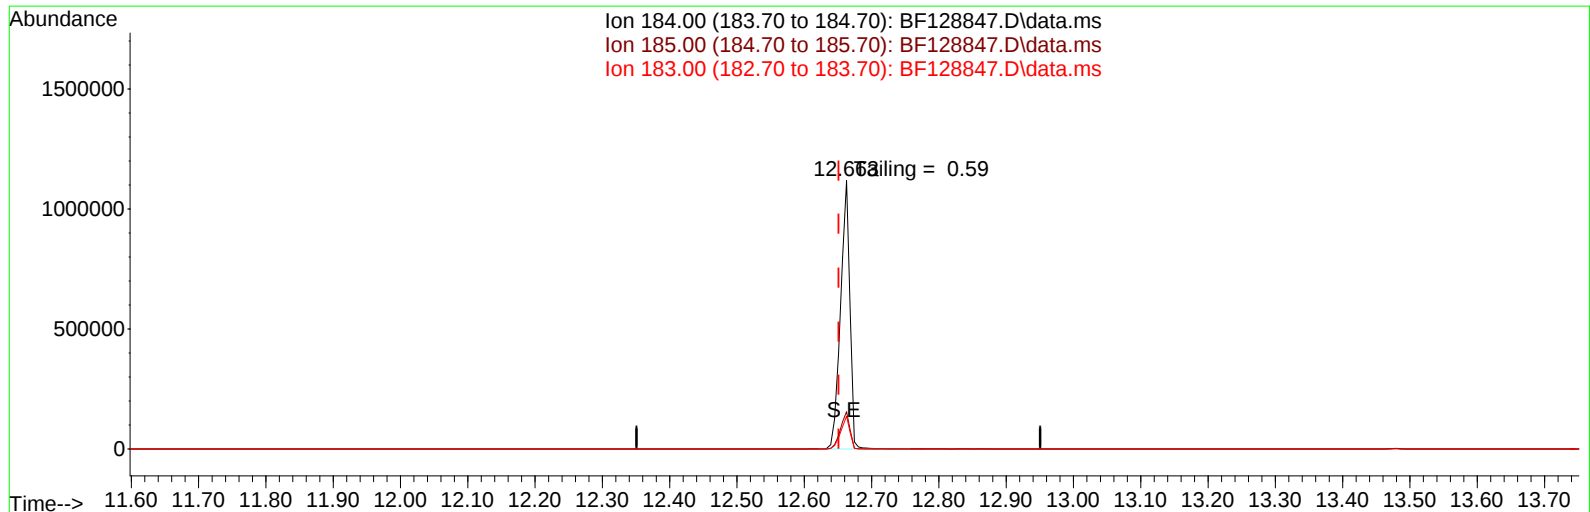

TIC: BF128847.D\data.ms

(77) Benzidine**12.663min (+ 0.012) 341990.17 ng****response 886261**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.90	13.90
183.00	11.60	12.21
0.00	0.00	0.00