

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF061722\
 Data File : BF128849.D
 Acq On : 17 Jun 2022 12:18
 Operator : CG\JU
 Sample : PB145561BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB145561BL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF060222.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF128849.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.428	530	534	547	rBV	3296606	2984516	67.22%	12.426%
2	6.439	702	706	722	rBV	2664522	2921114	65.80%	12.162%
3	6.781	760	764	767	rBV	776913	600327	13.52%	2.499%
4	7.351	855	861	864	rBV	1961830	1968319	44.33%	8.195%
5	8.063	977	982	986	rBV	877139	777236	17.51%	3.236%
6	9.145	1159	1166	1169	rBV	4220234	3843914	86.58%	16.003%
7	9.822	1276	1281	1284	rBV	1215631	957177	21.56%	3.985%
8	10.622	1411	1417	1420	rBV	2369314	2322330	52.31%	9.669%
9	11.310	1530	1534	1538	rBV	1213000	1014448	22.85%	4.223%
10	12.904	1800	1805	1808	rBV	4238324	4439717	100.00%	18.484%
11	13.957	1980	1984	1988	rBV	1065977	927209	20.88%	3.860%
12	14.051	1994	2000	2004	rBV	150942	184538	4.16%	0.768%
13	15.057	2168	2171	2175	rVB	43381	47285	1.07%	0.197%
14	15.415	2227	2232	2238	rBV	715814	893860	20.13%	3.721%
15	15.851	2303	2306	2311	rVB2	47651	71456	1.61%	0.297%
16	16.345	2386	2390	2395	rBV	43664	65805	1.48%	0.274%




Sum of corrected areas: 24019251

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF061722\
Data File : BF128849.D
Acq On : 17 Jun 2022 12:18
Operator : CG\JU
Sample : PB145561BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB145561BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF060222.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

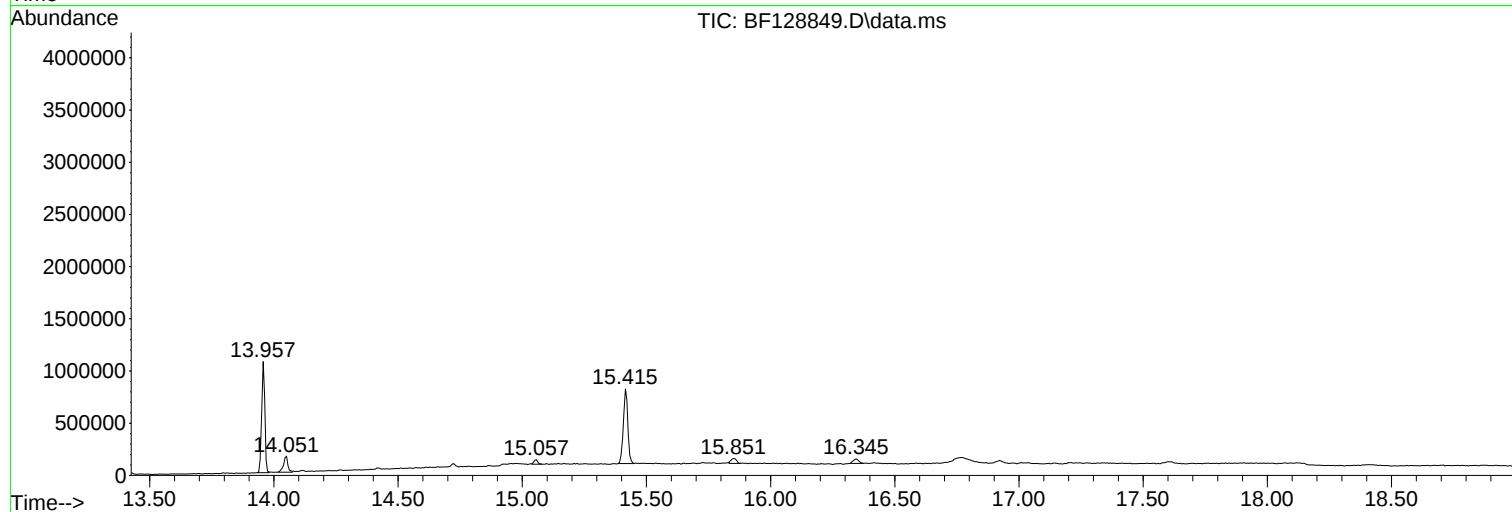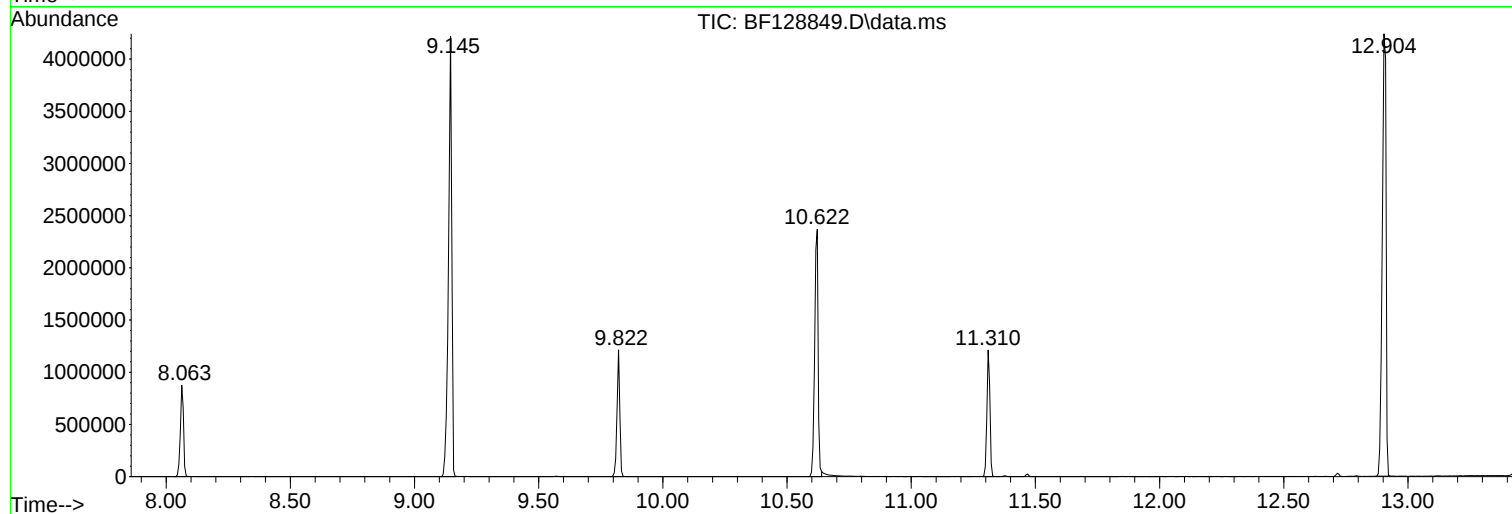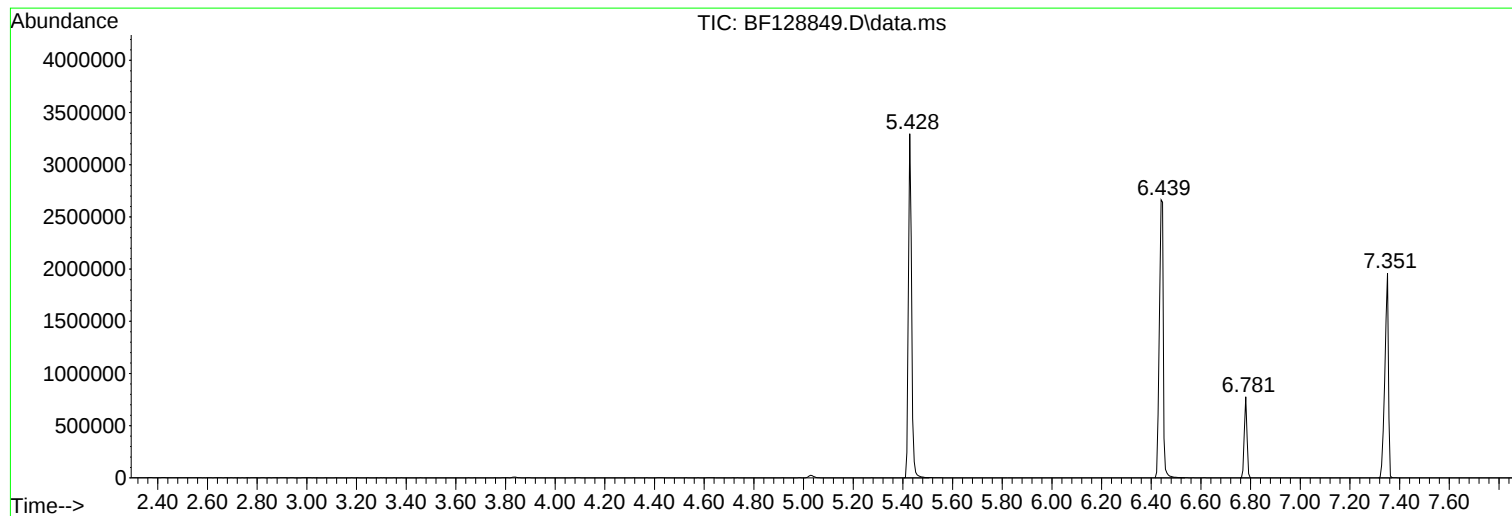

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF061722\
Data File : BF128849.D
Acq On : 17 Jun 2022 12:18
Operator : CG\JU
Sample : PB145561BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB145561BL










Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF060222.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Triphenylphosphine oxide Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
14.051	3.98 ng	184538	Chrysene-d12	13.957

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Triphenylphosphine oxide	278	C18H15OP	000791-28-6	96
2			(E)-7-Benzylidene-1-azabicyclo[3...]	293	C15H19NO3S	1000483-83-4	86
3			Formaldehyde, (triphenylphosphor...]	304	C19H17N2P	015990-54-2	38
4			3-(3,4-Dichlorophenyl)-2-thioxo-...	277	C9H5Cl2NOS2	017046-34-3	32
5			5-Methyl-8-phenylfuro[3',2':5,6]...	277	C16H11N3O2	1000460-07-9	25

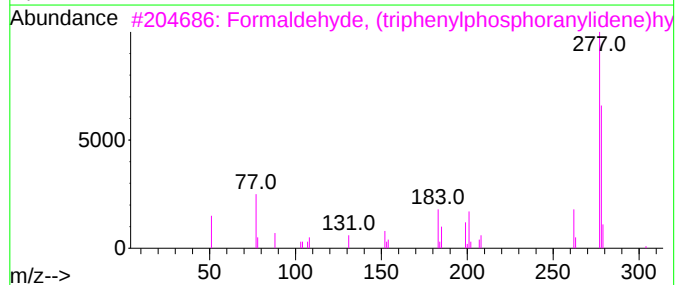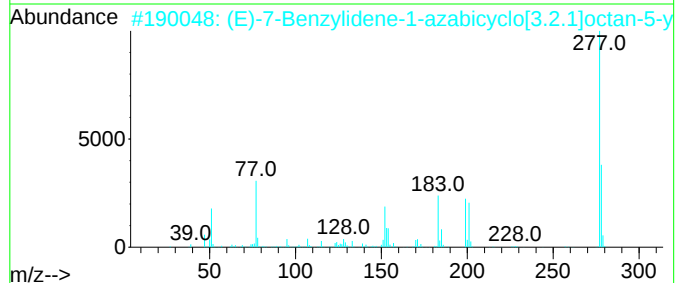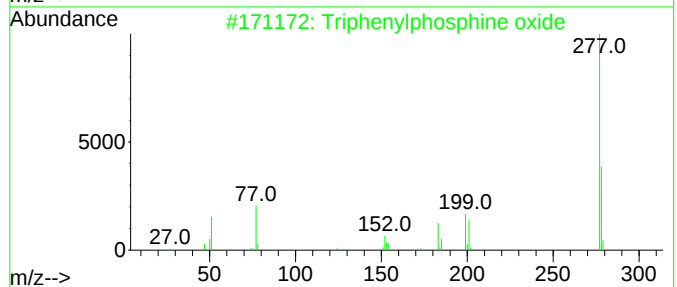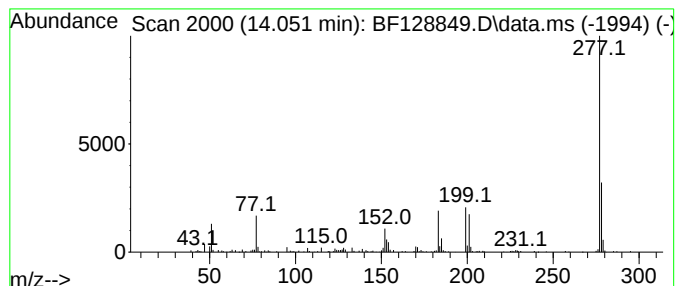

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF061722\
Data File : BF128849.D
Acq On : 17 Jun 2022 12:18
Operator : CG\JU
Sample : PB145561BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB145561BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF060222.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Triphenylphosph...	14.051	4.0	ng	184538	5	13.957	927209	20.0