

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF061722\
 Data File : BF128850.D
 Acq On : 17 Jun 2022 12:48
 Operator : CG\JU
 Sample : PB145586BL
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB145586BL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF060222.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF128850.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.428	530	534	551	rBV	3792171	3384636	76.28%	12.986%
2	6.440	702	706	709	rBV	3242422	3365329	75.85%	12.912%
3	6.781	760	764	767	rBV	918859	716937	16.16%	2.751%
4	7.351	855	861	864	rBV	2294978	2342411	52.79%	8.987%
5	8.063	977	982	986	rBV	1075548	932330	21.01%	3.577%
6	9.145	1159	1166	1169	rBV	4785575	4417333	99.56%	16.948%
7	9.822	1275	1281	1284	rBV	1192073	961569	21.67%	3.689%
8	10.616	1411	1416	1435	rBV	2354365	2369534	53.40%	9.091%
9	11.310	1530	1534	1537	rBV	1236024	1025221	23.11%	3.933%
10	12.904	1800	1805	1808	rBV	4568597	4436940	100.00%	17.023%
11	13.957	1980	1984	1988	rBV	1067080	936768	21.11%	3.594%
12	14.045	1994	1999	2004	rBV	164168	185719	4.19%	0.713%
13	15.057	2168	2171	2174	rVB	43746	50056	1.13%	0.192%
14	15.416	2227	2232	2238	rBV	660566	815408	18.38%	3.128%
15	15.851	2303	2306	2311	rVB2	51901	67909	1.53%	0.261%
16	16.345	2387	2390	2395	rVB2	38344	55801	1.26%	0.214%




Sum of corrected areas: 26063901

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF061722\
Data File : BF128850.D
Acq On : 17 Jun 2022 12:48
Operator : CG\JU
Sample : PB145586BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB145586BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF060222.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

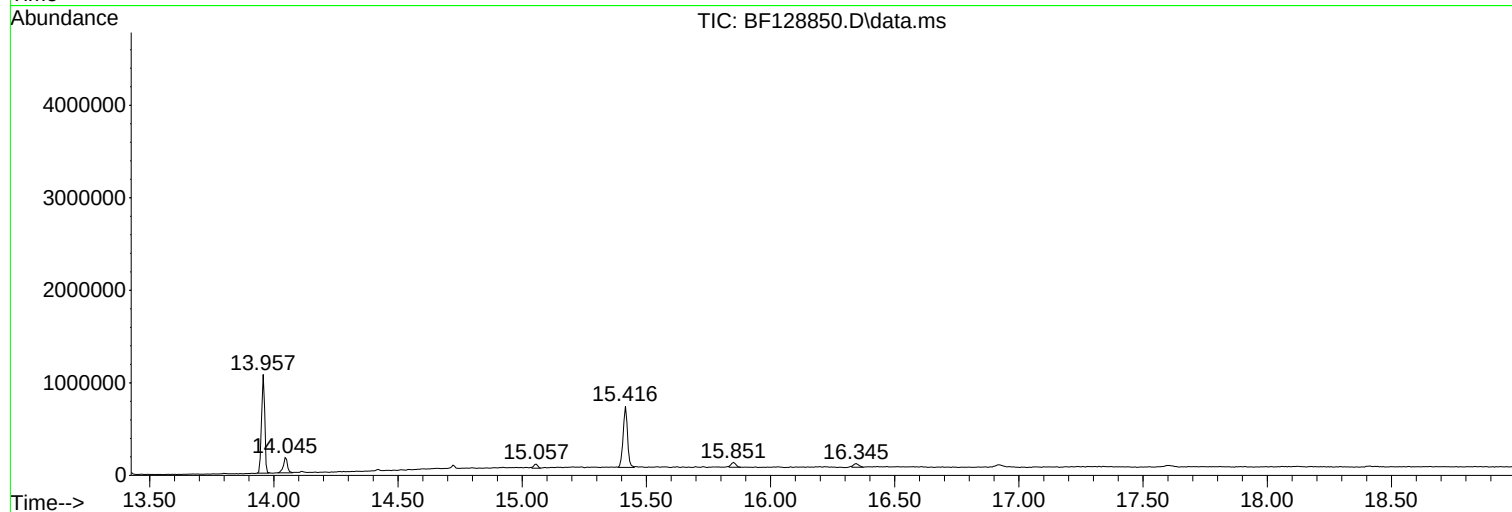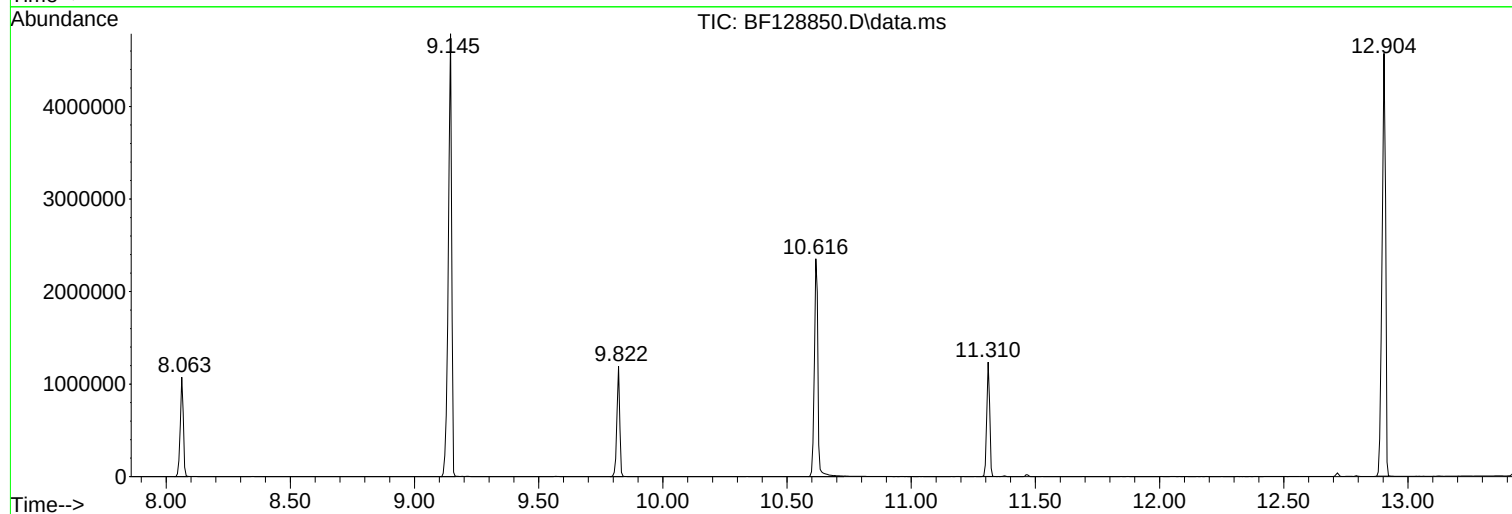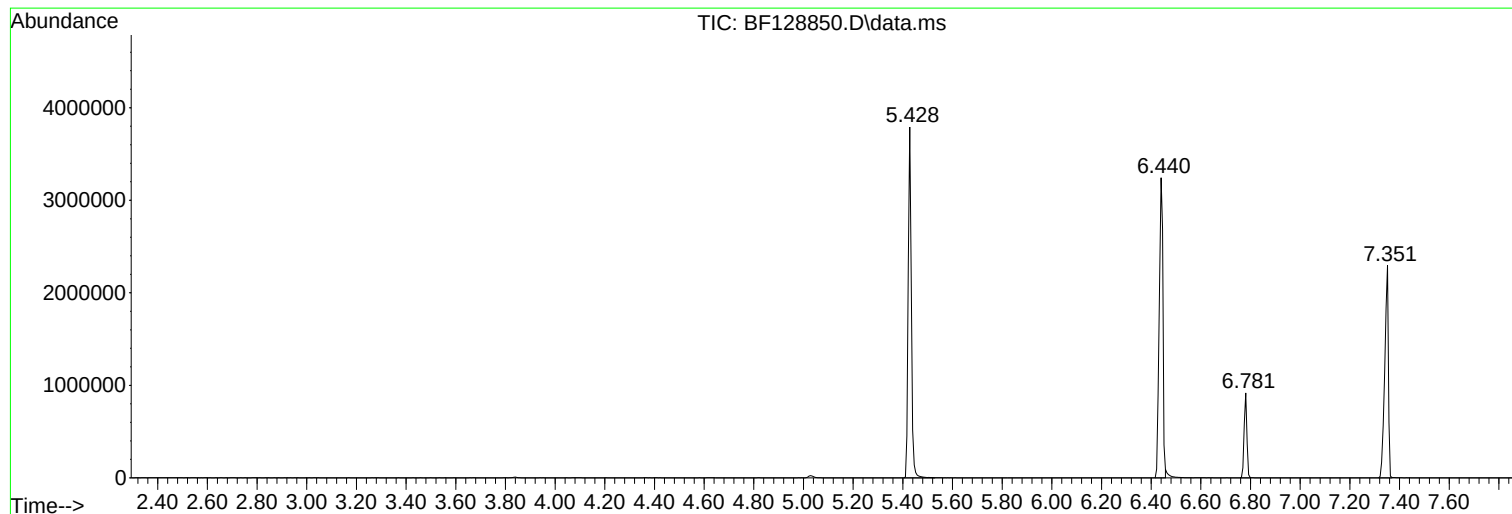

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF061722\
Data File : BF128850.D
Acq On : 17 Jun 2022 12:48
Operator : CG\JU
Sample : PB145586BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB145586BL










Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF060222.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Triphenylphosphine oxide Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
14.045	3.97 ng	185719	Chrysene-d12	13.957

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Triphenylphosphine oxide	278	C18H15OP	000791-28-6	97
2			Formaldehyde, (triphenylphosphor...	304	C19H17N2P	015990-54-2	64
3			(E)-7-Benzylidene-1-azabicyclo[3...	293	C15H19N03S	1000483-83-4	62
4			Vanadium, cycloheptatrienyl-(pen...	277	C17H22V	1000155-20-5	43
5			Carbazol-1-one, 1,2,3,4-tetrahyd...	277	C18H15NO2	299962-12-2	40

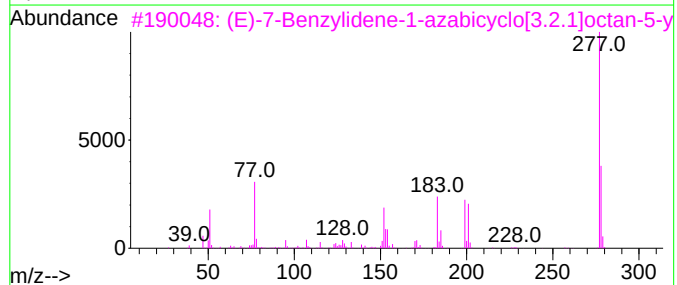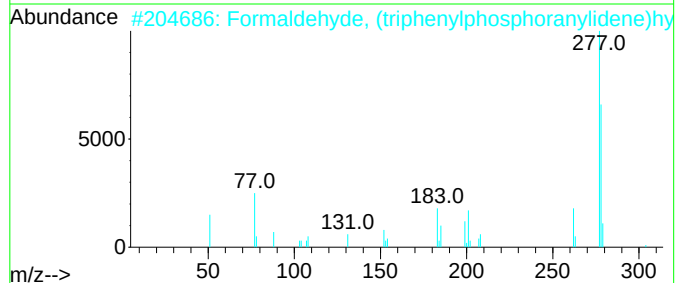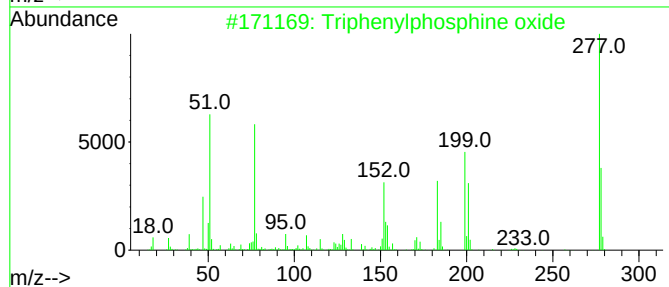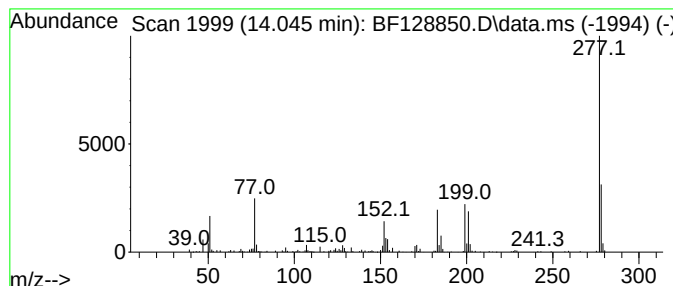

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF061722\
Data File : BF128850.D
Acq On : 17 Jun 2022 12:48
Operator : CG\JU
Sample : PB145586BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB145586BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF060222.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Triphenylphosph...	14.045	4.0	ng	185719	5	13.957	936768	20.0