

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF061722\
 Data File : BF128855.D
 Acq On : 17 Jun 2022 15:39
 Operator : CG\JU
 Sample : N3367-02
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 MJS-TWP-02

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF060222.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF128855.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.416	529	532	540	rBV	1355947	1233089	38.09%	5.689%
2	6.434	702	705	717	rBV	939908	802220	24.78%	3.701%
3	6.781	760	764	767	rBV	558046	483844	14.95%	2.232%
4	7.351	855	861	864	rBV	1783261	1756136	54.25%	8.102%
5	8.063	978	982	990	rVB	783572	612035	18.91%	2.824%
6	8.187	998	1003	1006	rBV	57416	49184	1.52%	0.227%
7	8.222	1006	1009	1023	rVV	497962	554625	17.13%	2.559%
8	8.322	1023	1026	1029	rVB	276175	158939	4.91%	0.733%
9	9.145	1160	1166	1169	rBV	3777141	3236974	100.00%	14.933%
10	9.451	1215	1218	1221	rBV	242013	170395	5.26%	0.786%
11	9.822	1277	1281	1283	rBV	809574	674838	20.85%	3.113%
12	9.845	1283	1285	1288	rVB	88036	68501	2.12%	0.316%
13	10.528	1398	1401	1404	rBV	396870	289193	8.93%	1.334%
14	10.575	1404	1409	1412	rVV	319039	250857	7.75%	1.157%
15	10.616	1412	1416	1419	rVV	1725976	1482301	45.79%	6.838%
16	10.669	1422	1425	1428	rVV3	173785	179865	5.56%	0.830%
17	10.704	1428	1431	1438	rVB	613266	520541	16.08%	2.401%
18	10.810	1445	1449	1451	rBV	45810	42633	1.32%	0.197%
19	11.233	1517	1521	1524	rBV	535700	458981	14.18%	2.117%
20	11.263	1524	1526	1530	rVB	66425	53011	1.64%	0.245%
21	11.310	1530	1534	1537	rBV	815704	698951	21.59%	3.224%
22	11.486	1558	1564	1568	rVB3	69487	113191	3.50%	0.522%
23	11.569	1571	1578	1583	rVV7	25298	66293	2.05%	0.306%
24	11.610	1583	1585	1590	rVB	54963	49544	1.53%	0.229%
25	11.833	1619	1623	1632	rBV	504543	511564	15.80%	2.360%
26	12.304	1698	1703	1706	rBV	82200	66756	2.06%	0.308%
27	12.386	1709	1717	1733	rBV2	523341	943245	29.14%	4.352%
28	12.898	1799	1804	1807	rBV	3288477	2949137	91.11%	13.605%
29	13.275	1865	1868	1878	rVB2	52053	99537	3.08%	0.459%
30	13.369	1878	1884	1887	rBV	144032	153419	4.74%	0.708%
31	13.463	1897	1900	1904	rVB	848016	822806	25.42%	3.796%
32	13.804	1954	1958	1970	rBV5	123147	262687	8.12%	1.212%
33	13.927	1977	1979	1981	rBV	147025	140451	4.34%	0.648%
34	13.951	1981	1983	1987	rVB	576326	512135	15.82%	2.363%
35	14.045	1995	1999	2004	rVB	147554	149121	4.61%	0.688%
36	14.180	2018	2022	2025	rBV3	44820	72720	2.25%	0.335%

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF061722\
Data File : BF128855.D
Acq On : 17 Jun 2022 15:39
Operator : CG\JU
Sample : N3367-02
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
MJS-TWP-02

Integration Parameters: rteint.p
Integrator: RTE
Smoothing : ON Filtering: 5
Sampling : 1 Min Area: 3 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF060222.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

37	14.216	2025	2028	2034	rVB	87903	100848	3.12%	0.465%
38	14.574	2086	2089	2091	rBV	63469	63704	1.97%	0.294%
39	14.604	2091	2094	2097	rVB2	45351	49835	1.54%	0.230%
40	14.792	2123	2126	2130	rBV2	112893	109991	3.40%	0.507%
41	15.016	2160	2164	2167	rBV2	26595	39811	1.23%	0.184%
42	15.051	2167	2170	2177	rVB	42778	61854	1.91%	0.285%
43	15.410	2226	2231	2238	rVB	410376	504512	15.59%	2.327%
44	15.845	2302	2305	2313	rVB3	32473	56027	1.73%	0.258%




Sum of corrected areas: 21676301

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF061722\
Data File : BF128855.D
Acq On : 17 Jun 2022 15:39
Operator : CG\JU
Sample : N3367-02
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
MJS-TWP-02

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF060222.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

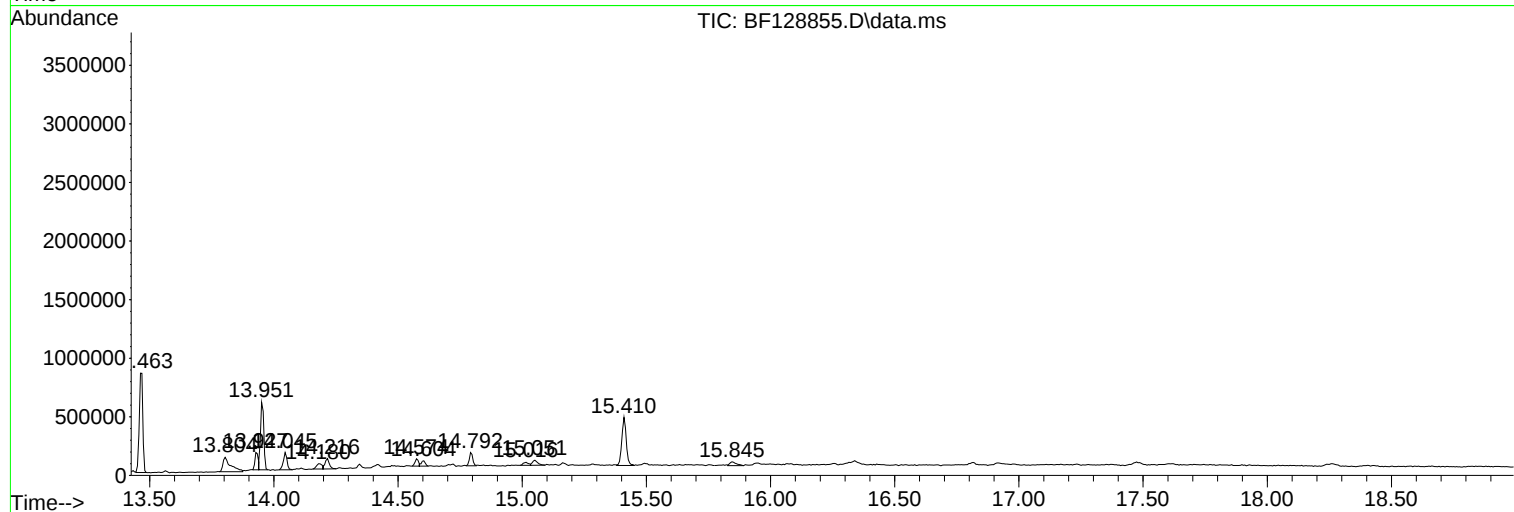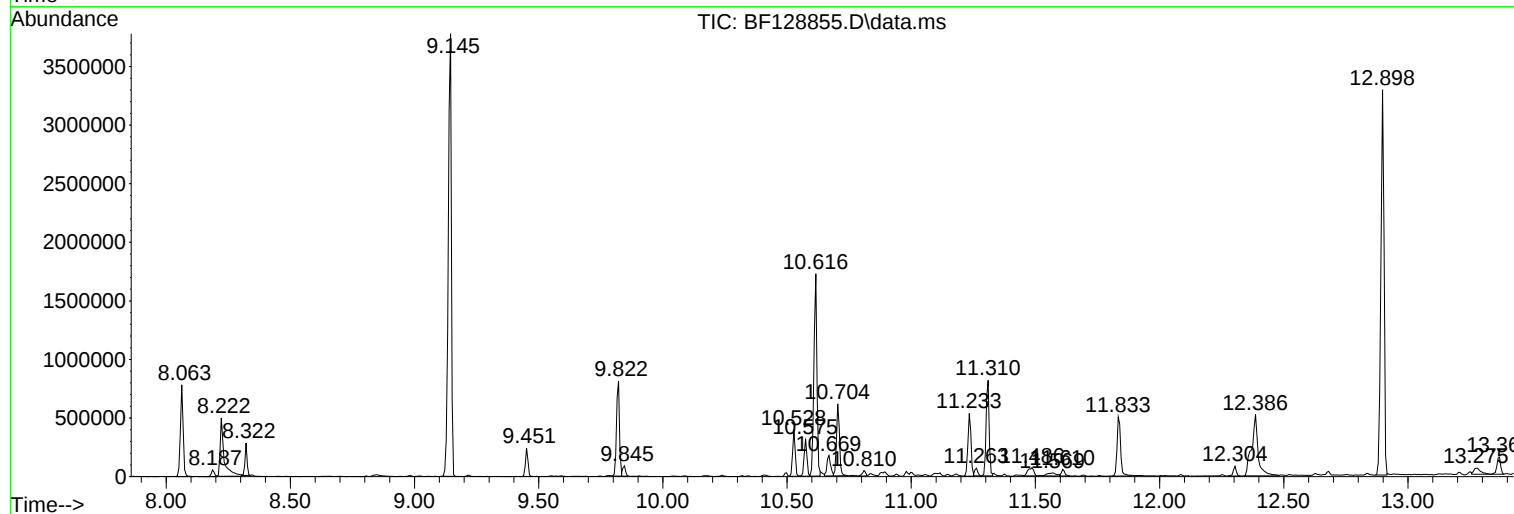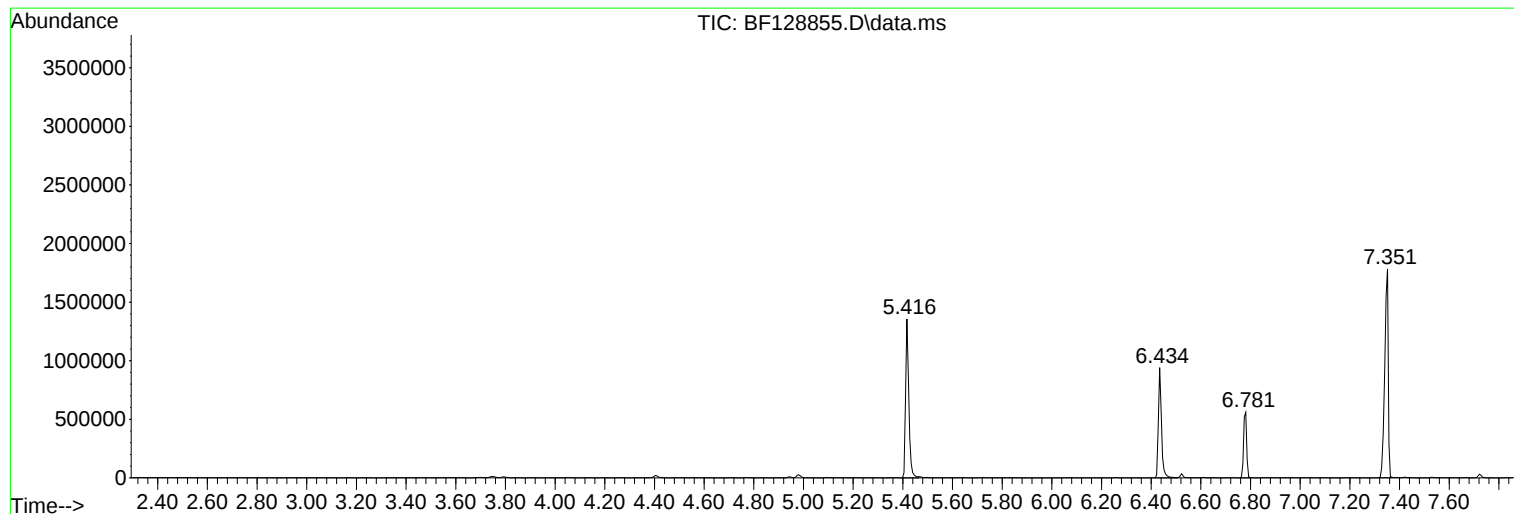

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF061722\
Data File : BF128855.D
Acq On : 17 Jun 2022 15:39
Operator : CG\JU
Sample : N3367-02
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
MJS-TWP-02

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF060222.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF061722\
Data File : BF128855.D
Acq On : 17 Jun 2022 15:39
Operator : CG\JU
Sample : N3367-02
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
MJS-TWP-02

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF060222.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------