
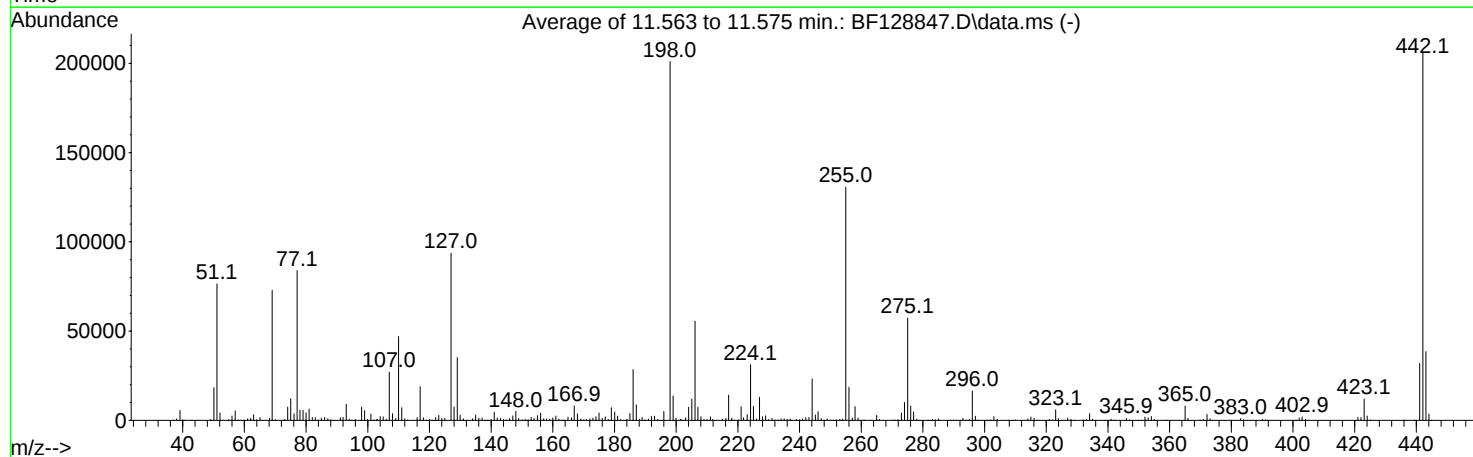


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF061722\
 Data File : BF128847.D
 Acq On : 17 Jun 2022 10:49
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF060222.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Jun 14 14:53:53 2022

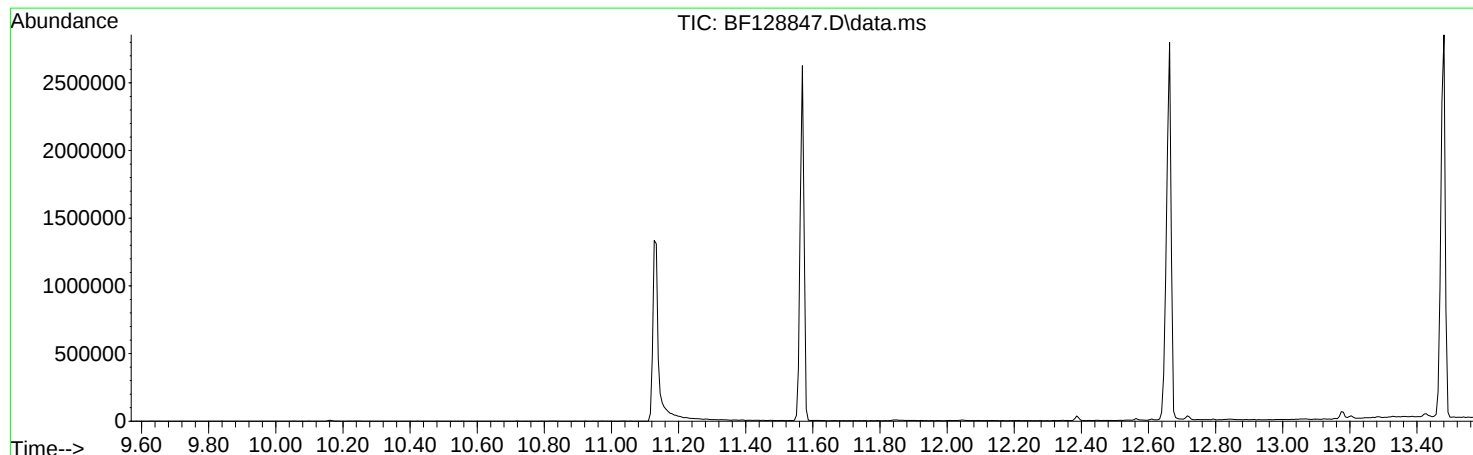




AutoFind: Scans 1577, 1578, 1579; Background Corrected with Scan 1571

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	38.0	76451	PASS
68	69	0.00	2	1.6	1161	PASS
69	198	0.00	100	36.3	72923	PASS
70	69	0.00	2	0.6	435	PASS
127	198	10	80	46.6	93712	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	200939	PASS
199	198	5	9	6.8	13751	PASS
275	198	10	60	28.5	57256	PASS
365	198	1	100	4.0	8074	PASS
441	198	0.01	100	15.9	31911	PASS
442	442	50	100	100.0	206088	PASS
443	442	15	24	18.7	38552	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF061722\
Data File : BF128847.D
Acq On : 17 Jun 2022 10:49
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Jun 18 07:53:33 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF060222.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jun 14 14:53:53 2022
Response via : Initial Calibration

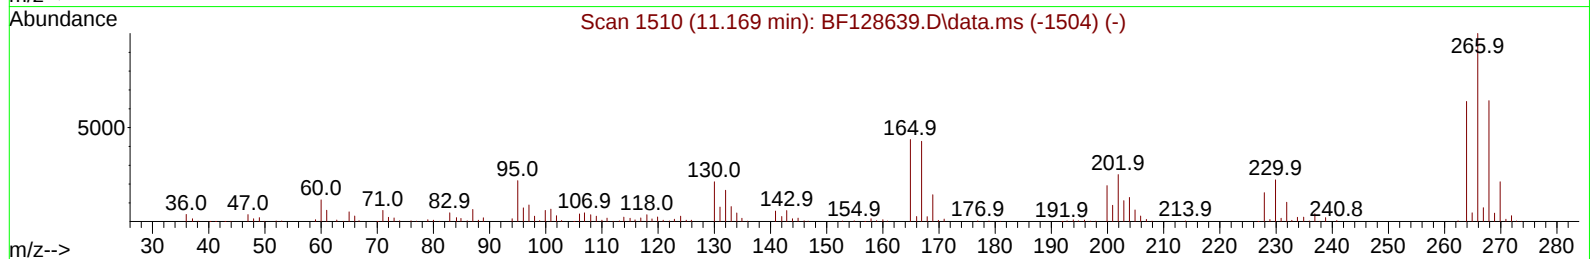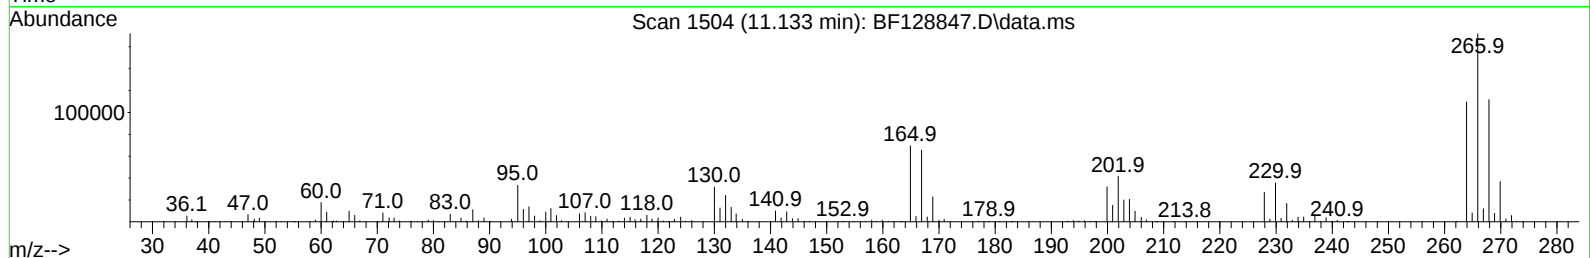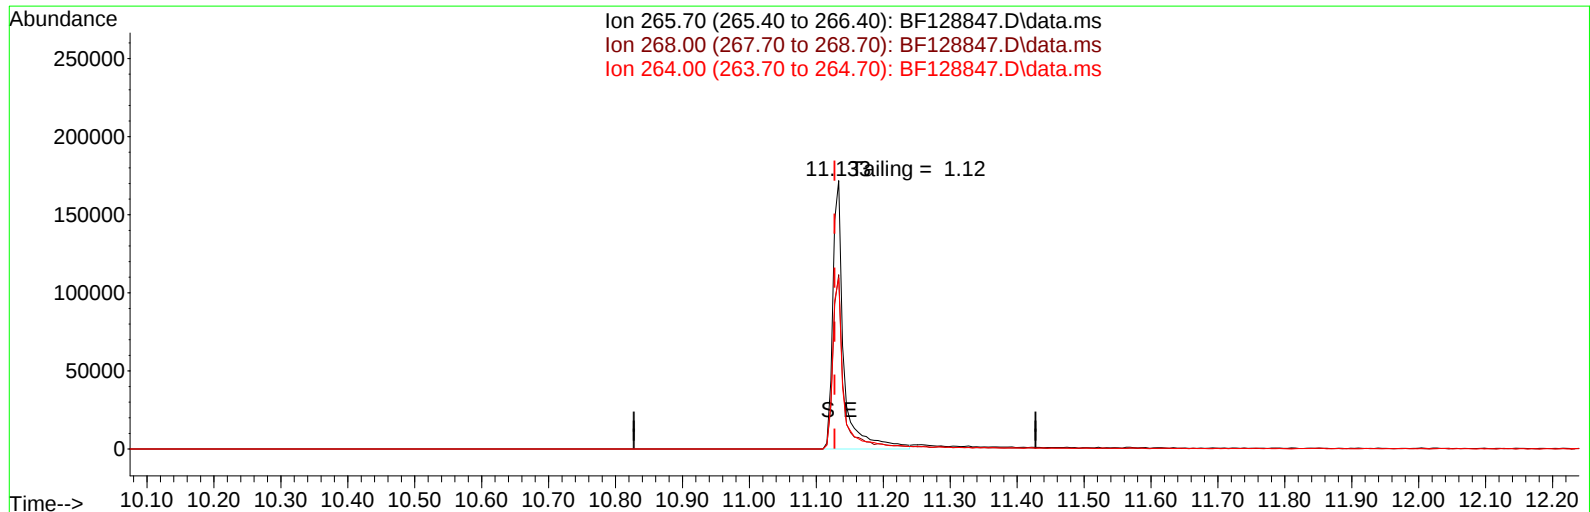

TIC: BF128847.D\data.ms

(70) Pentachlorophenol (C)

11.133min (+ 0.006) 38263.38 ng




response 198468

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.70	64.94
264.00	61.80	63.77
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF061722\
Data File : BF128847.D
Acq On : 17 Jun 2022 10:49
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Jun 18 07:53:33 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF060222.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jun 14 14:53:53 2022
Response via : Initial Calibration

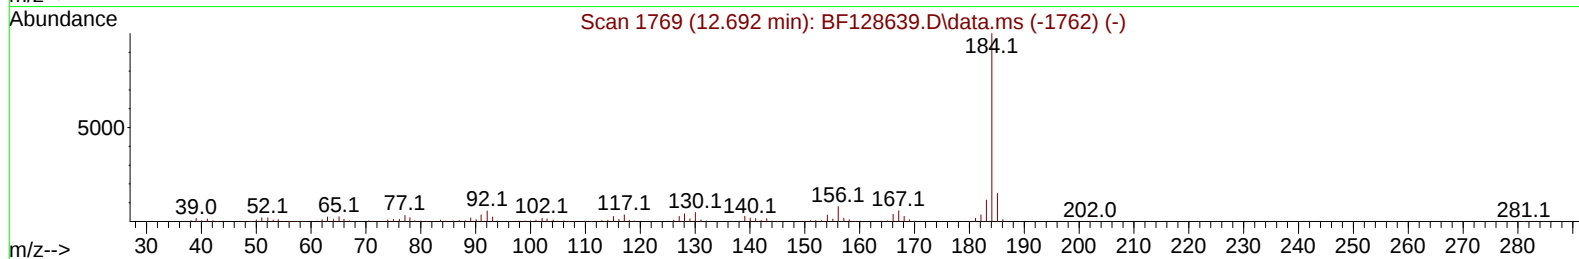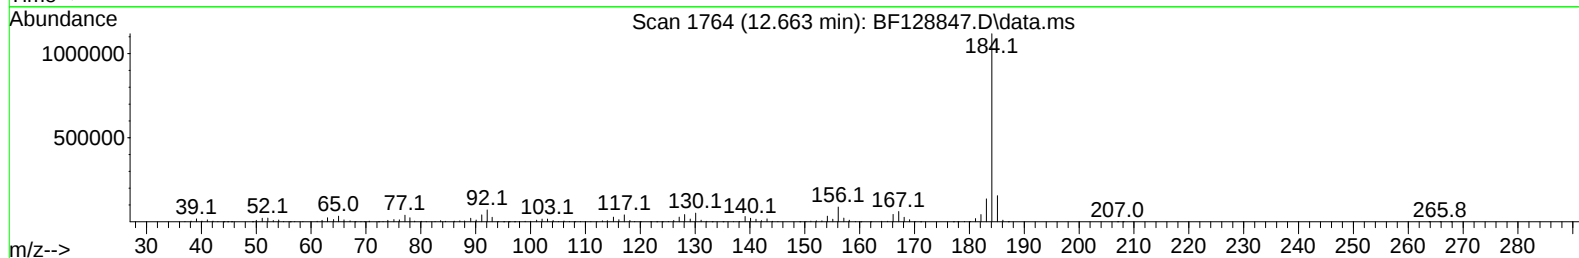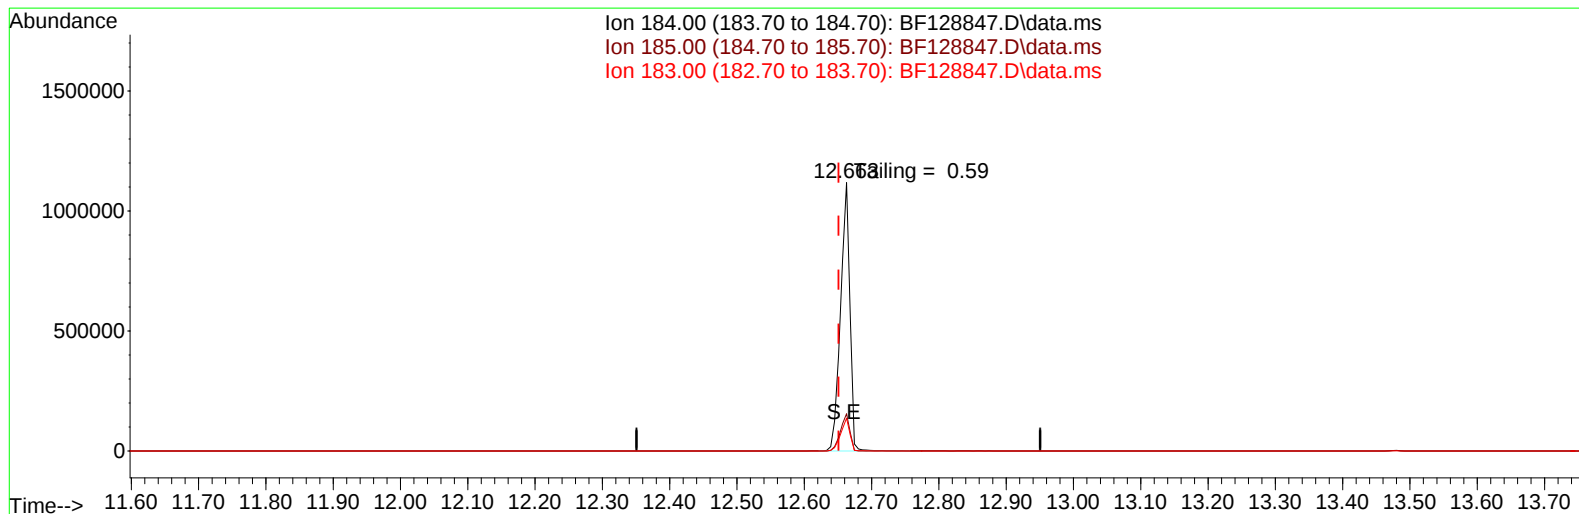

TIC: BF128847.D\data.ms

(77) Benzidine

12.663min (+ 0.012) 341990.17 ng

response 886261

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.90	13.90
183.00	11.60	12.21
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
6/17/2022	BNA_F	<u>BF128847.D</u>
Compound Name	Response	Retention Time
DDT	492086	13.48
DDD	13319	13.18
DDE	1496	12.839
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
14815	506901	2.92

Instrument :
BNA_F
ClientSampleId :
DFTPP