
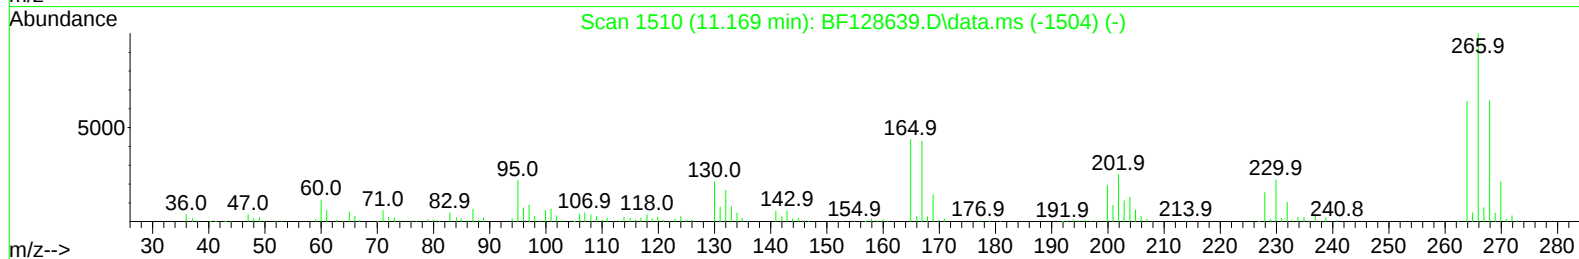
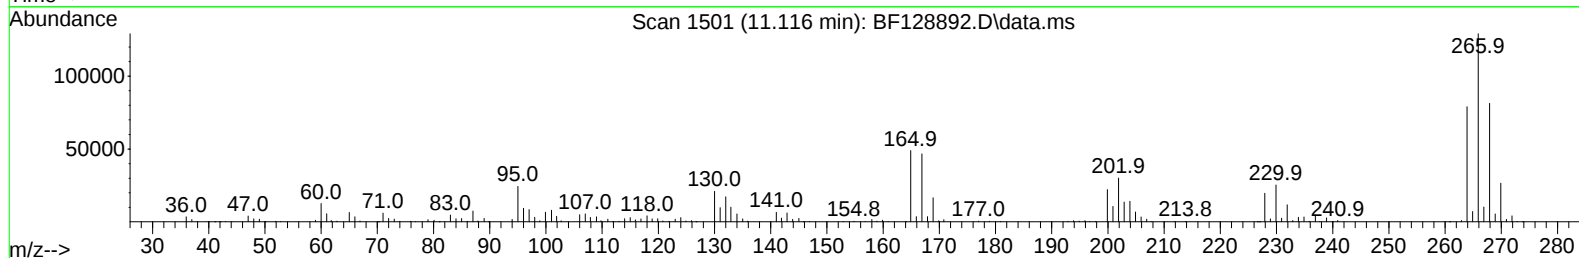


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF062122\
 Data File : BF128892.D
 Acq On : 21 Jun 2022 09:12
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 22 01:45:37 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF060222.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Jun 22 01:02:29 2022
 Response via : Initial Calibration



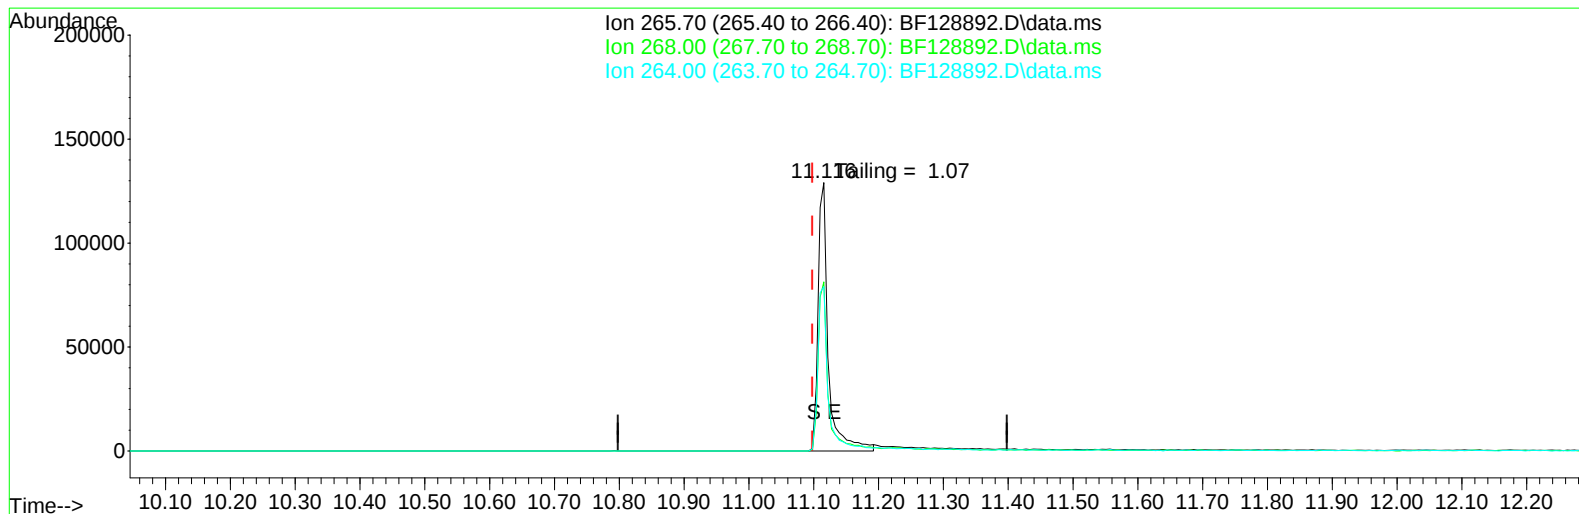


TIC: BF128892.D\data.ms

(70) Pentachlorophenol (C)**11.116min (+ 0.018) 309691.14 ng****response 151252**

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.70	63.03
264.00	61.80	61.24
0.00	0.00	0.00

Quant Time: Jun 22 01:45:37 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF060222.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jun 22 01:02:29 2022
Response via : Initial Calibration

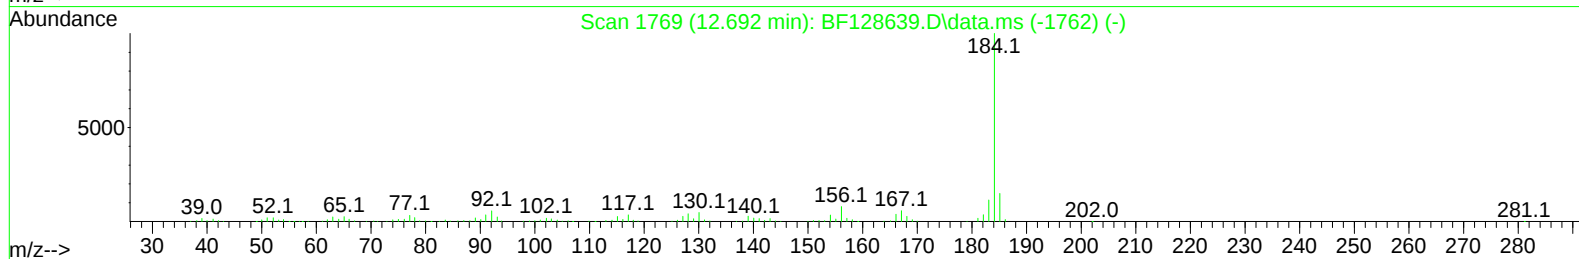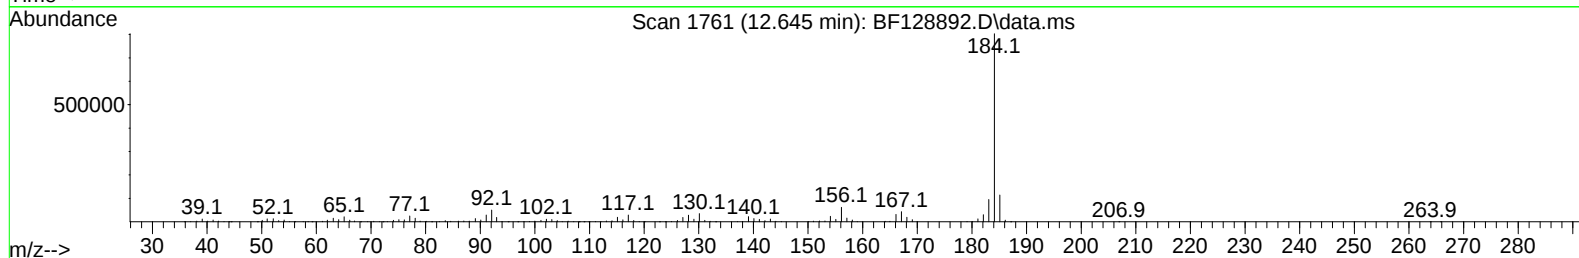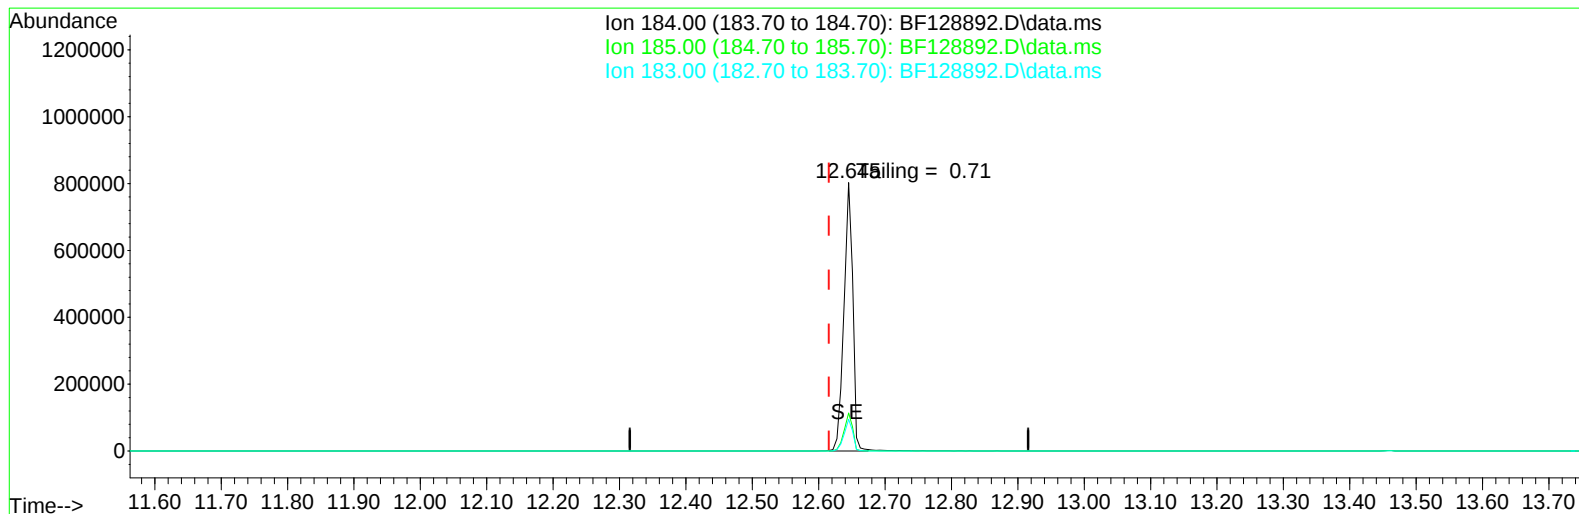

TIC: BF128892.D\data.ms

(77) Benzidine

12.645min (+ 0.029) 687686.90 ng

response 753977

Ion	Exp%	Act%
-----	------	------

184.00	100.00	100.00
--------	--------	--------

185.00	14.90	14.23
--------	-------	-------

183.00	11.60	11.82
--------	-------	-------

0.00 0.00 0.00