
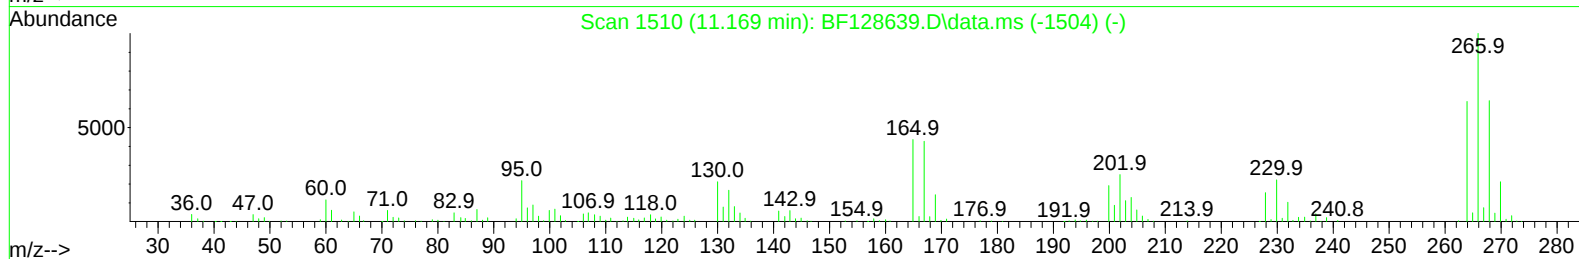
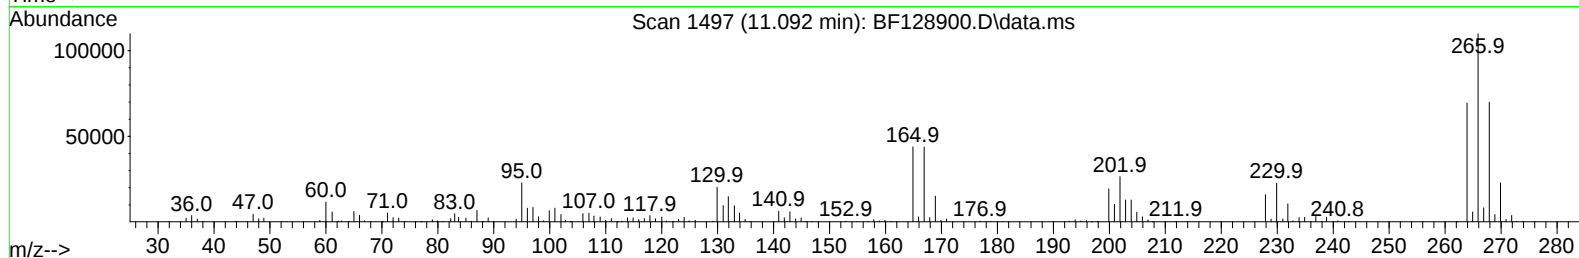


```
Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF062122\  
Data File : BF128900.D  
Acq On    : 21 Jun 2022  16:33  
Operator  : CG\JU  
Sample    : DFTPP  
Misc      :  
ALS Vial  : 1    Sample Multiplier: 1
```

Quant Time: Jun 22 01:50:31 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF060222.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jun 22 01:02:29 2022
Response via : Initial Calibration

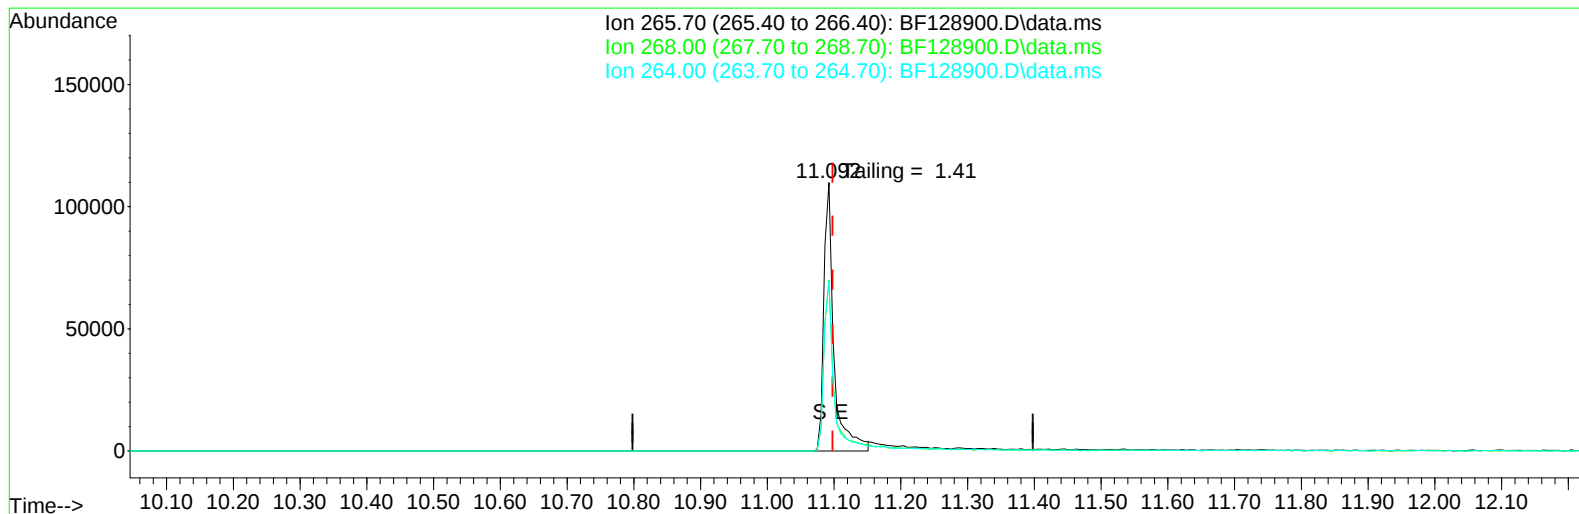

TIC: BF128900.D\data.ms

(70) Pentachlorophenol (C)




11.092min (-0.006) 225666.68 ng

response	124166
----------	--------

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.70	63.60
264.00	61.80	63.24
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF062122\
Data File : BF128900.D
Acq On : 21 Jun 2022 16:33
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 22 01:50:31 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF060222.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jun 22 01:02:29 2022
Response via : Initial Calibration

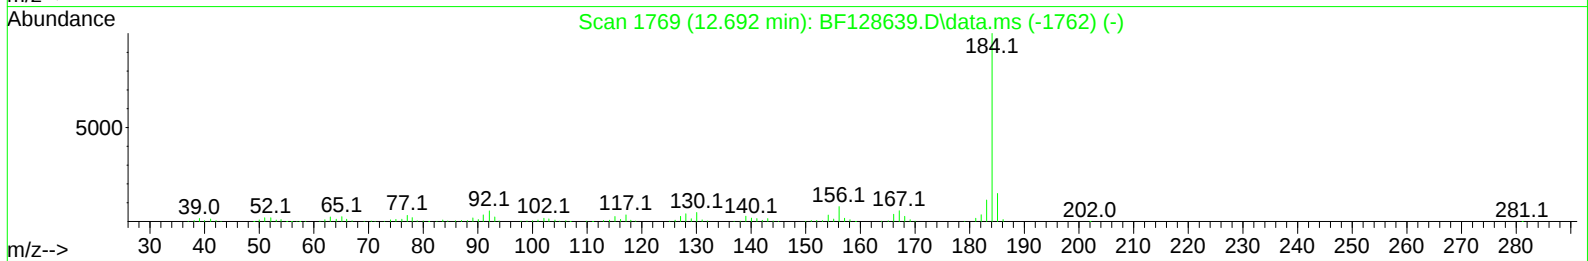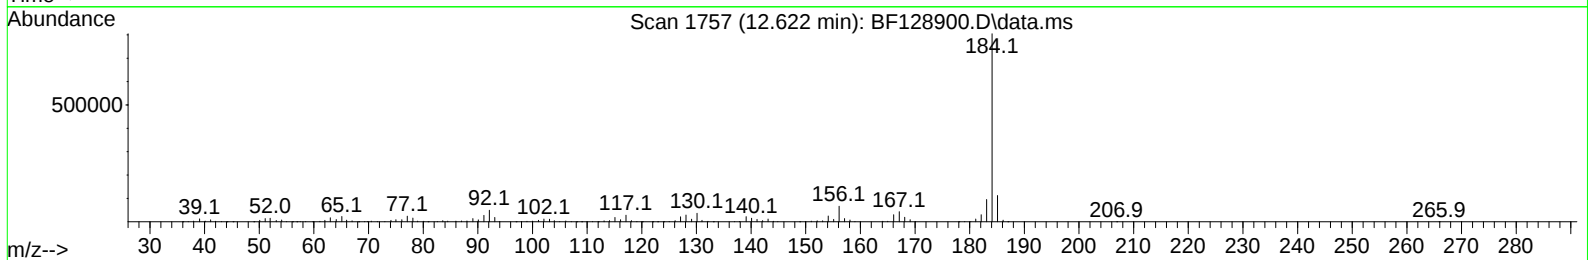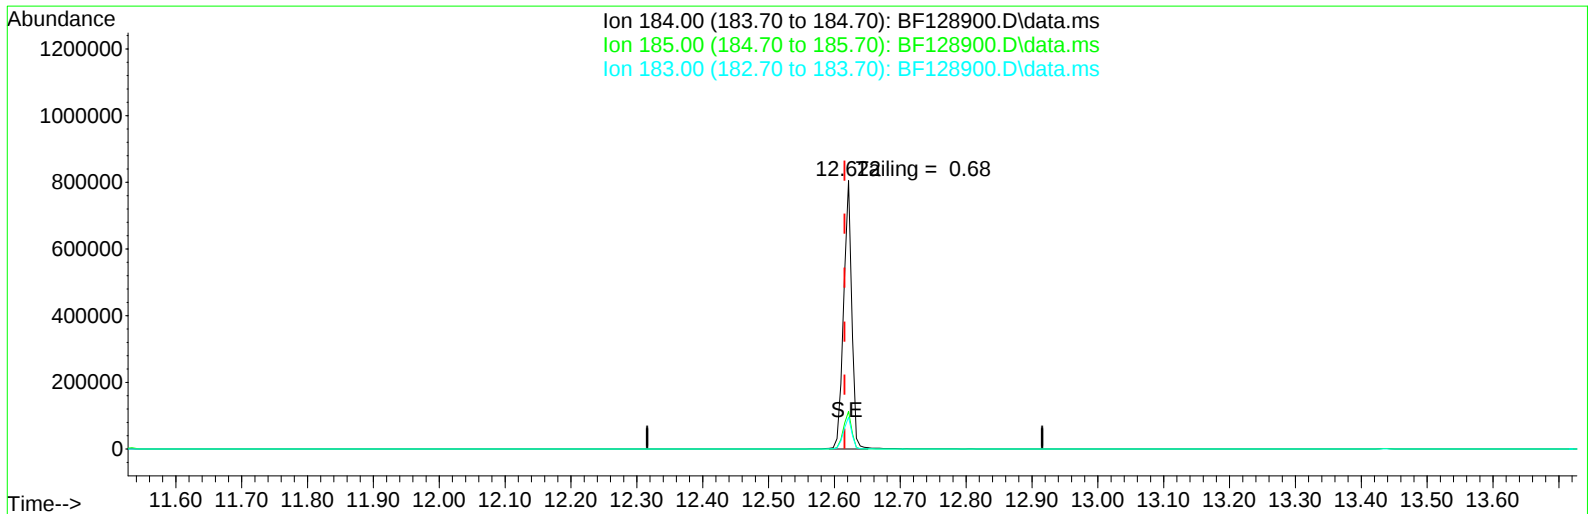

TIC: BF128900.D\data.ms

(77) Benzidine

12.622min (+ 0.006) 202435.55 ng

response 698132

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.90	14.00
183.00	11.60	11.86
0.00	0.00	0.00