

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF062122\
 Data File : BF128894.D
 Acq On : 21 Jun 2022 10:36
 Operator : CG\JU
 Sample : PB145632BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB145632BL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF060222.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF128894.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.422	529	533	548	rBV	3507967	3461921	70.06%	12.672%
2	6.428	700	704	707	rBV	3174798	3464602	70.12%	12.682%
3	6.769	759	762	766	rBV	886850	733615	14.85%	2.685%
4	7.340	853	859	862	rBV	2106843	2428706	49.15%	8.890%
5	8.057	975	981	984	rBV	932766	942003	19.06%	3.448%
6	9.133	1157	1164	1167	rBV	4683322	4585952	92.81%	16.786%
7	9.810	1273	1279	1282	rBV	1310401	1102328	22.31%	4.035%
8	10.604	1408	1414	1417	rBV	2861177	2551340	51.64%	9.339%
9	11.298	1528	1532	1535	rBV	1419705	1146412	23.20%	4.196%
10	12.892	1797	1803	1806	rBV	5080325	4941103	100.00%	18.086%
11	13.939	1977	1981	1985	rBV	1034429	966930	19.57%	3.539%
12	14.033	1991	1997	2001	rBV	51193	59691	1.21%	0.218%
13	15.392	2223	2228	2235	rBV2	658196	797576	16.14%	2.919%
14	16.698	2448	2450	2463	rVB2	50615	137643	2.79%	0.504%




Sum of corrected areas: 27319822

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF062122\
Data File : BF128894.D
Acq On : 21 Jun 2022 10:36
Operator : CG\JU
Sample : PB145632BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB145632BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF060222.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

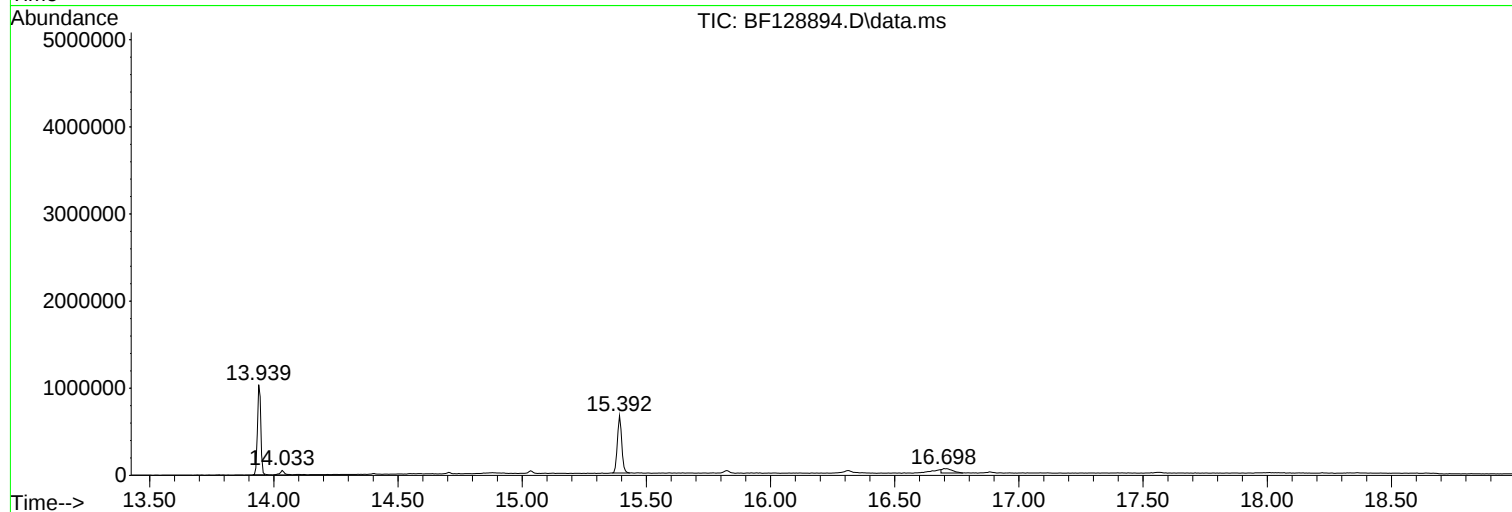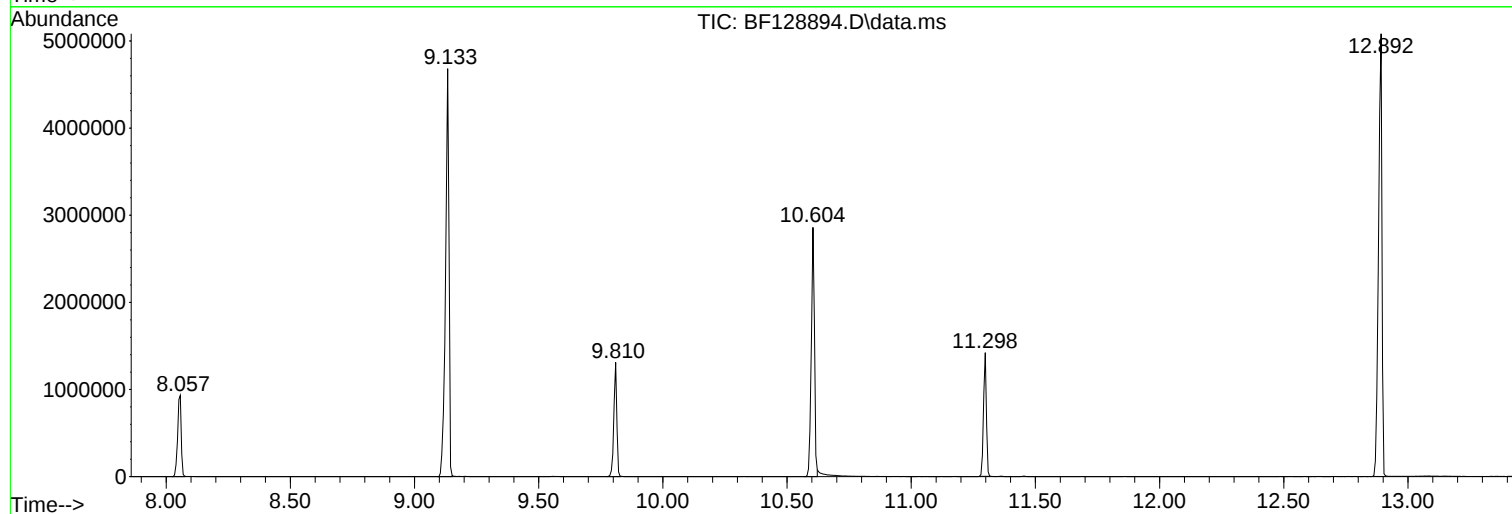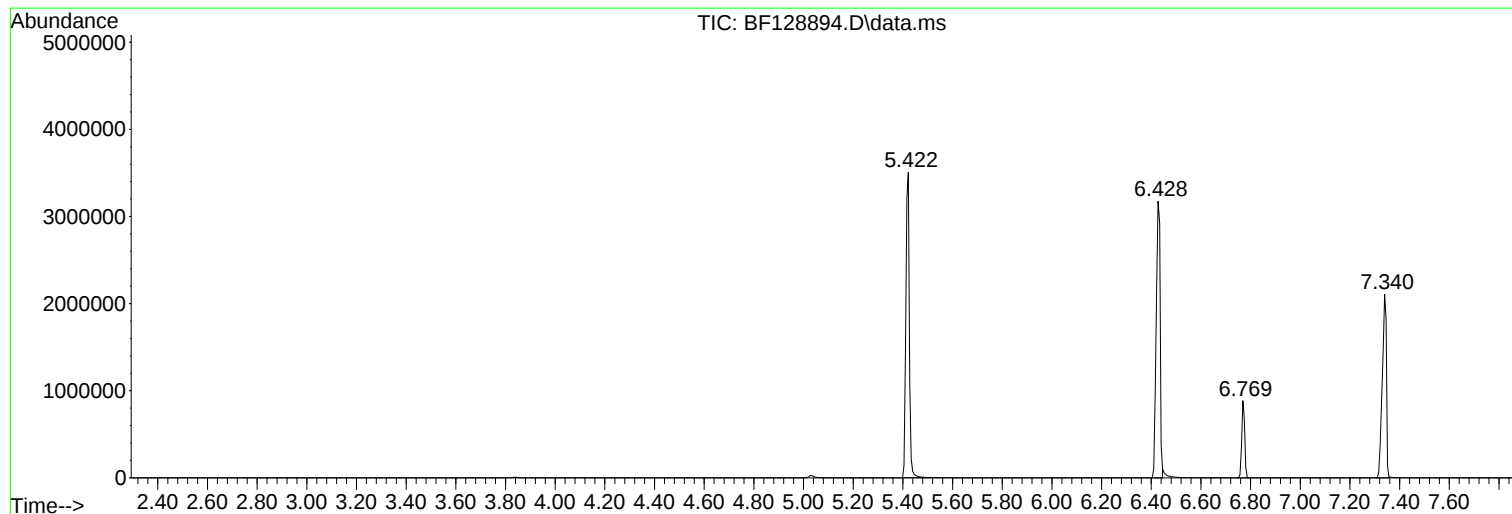

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF062122\
Data File : BF128894.D
Acq On : 21 Jun 2022 10:36
Operator : CG\JU
Sample : PB145632BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB145632BL










Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF060222.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 unknown16.698 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
16.698	3.45 ng	137643	Perylene-d12	15.392

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Serratinane-5,8,13-triol, (5.alpha...	281	C16H27NO3	005532-22-9	30
2			Thiocarbonic acid o-3-chloroprop...	272	C9H9C1N4O2S	1000251-29-2	14
3			Methyl 3-[(2-thienylacetyl)amino...	281	C12H11NO3S2	676594-38-0	14
4			2,6-Dimethylbenzenethiol, S-methyl-	152	C9H12S	1000353-02-2	11
5			Pyrrolidine-2-carboxylic acid, 4...	239	C8H8F3NO4	054615-48-4	11

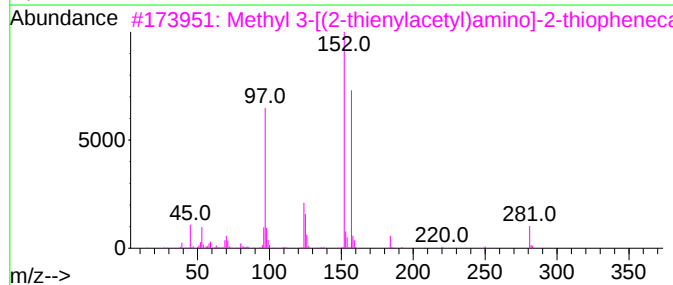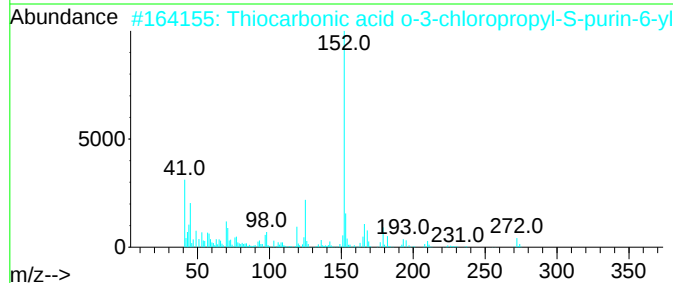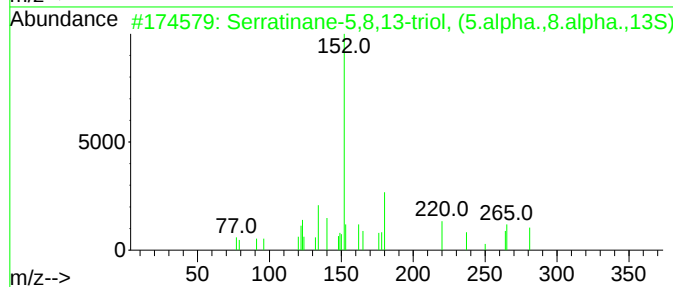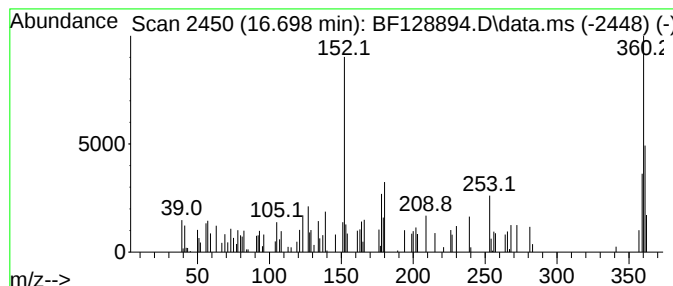

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF062122\
Data File : BF128894.D
Acq On : 21 Jun 2022 10:36
Operator : CG\JU
Sample : PB145632BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB145632BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF060222.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
unknown16.698	16.698	3.5	ng	137643	6	15.392	797576	20.0